

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061724\
 Data File : VU059279.D
 Acq On : 17 Jun 2024 14:48
 Operator : MD/SY
 Sample : VIBLK105
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK105

Quant Time: Jun 18 04:21:01 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jun 17 12:07:46 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	111772	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117	114252	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.810	152	48468	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	37858	4.871	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	97.400%
7) Chloroethane-d5	1.907	69	37007	4.949	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.000%
11) 1,1-Dichloroethene-d2	2.560	65	15569	4.828	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	96.600%
20) 2-Butanone-d5	4.615	46	87270	54.512	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	109.020%
24) Chloroform-d	5.058	84	76456	4.793	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.800%
26) 1,2-Dichloroethane-d4	5.695	65	39893	5.191	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.800%
32) Benzene-d6	5.721	84	151370	4.814	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.200%
36) 1,2-Dichloropropane-d6	6.685	67	48666	5.051	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.000%
41) Toluene-d8	7.894	98	127436	4.360	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.200%
43) trans-1,3-Dichloroprop...	8.177	79	14987	4.967	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	99.400%
46) 2-Hexanone-d5	8.627	63	64716	51.624	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	103.240%
56) 1,1,2,2-Tetrachloroeth...	10.753	84	40634	5.104	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.000%
66) 1,2-Dichlorobenzene-d4	12.190	152	47598	5.518	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	110.400%
Target Compounds						
16) Methylene chloride	3.039	84	7314	0.779	ug/L	Qvalue 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061724\
Data File : VU059279.D
Acq On : 17 Jun 2024 14:48
Operator : MD/SY
Sample : VIBLK105
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK105


Quant Time: Jun 18 04:21:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jun 17 12:07:46 2024
Response via : Initial Calibration

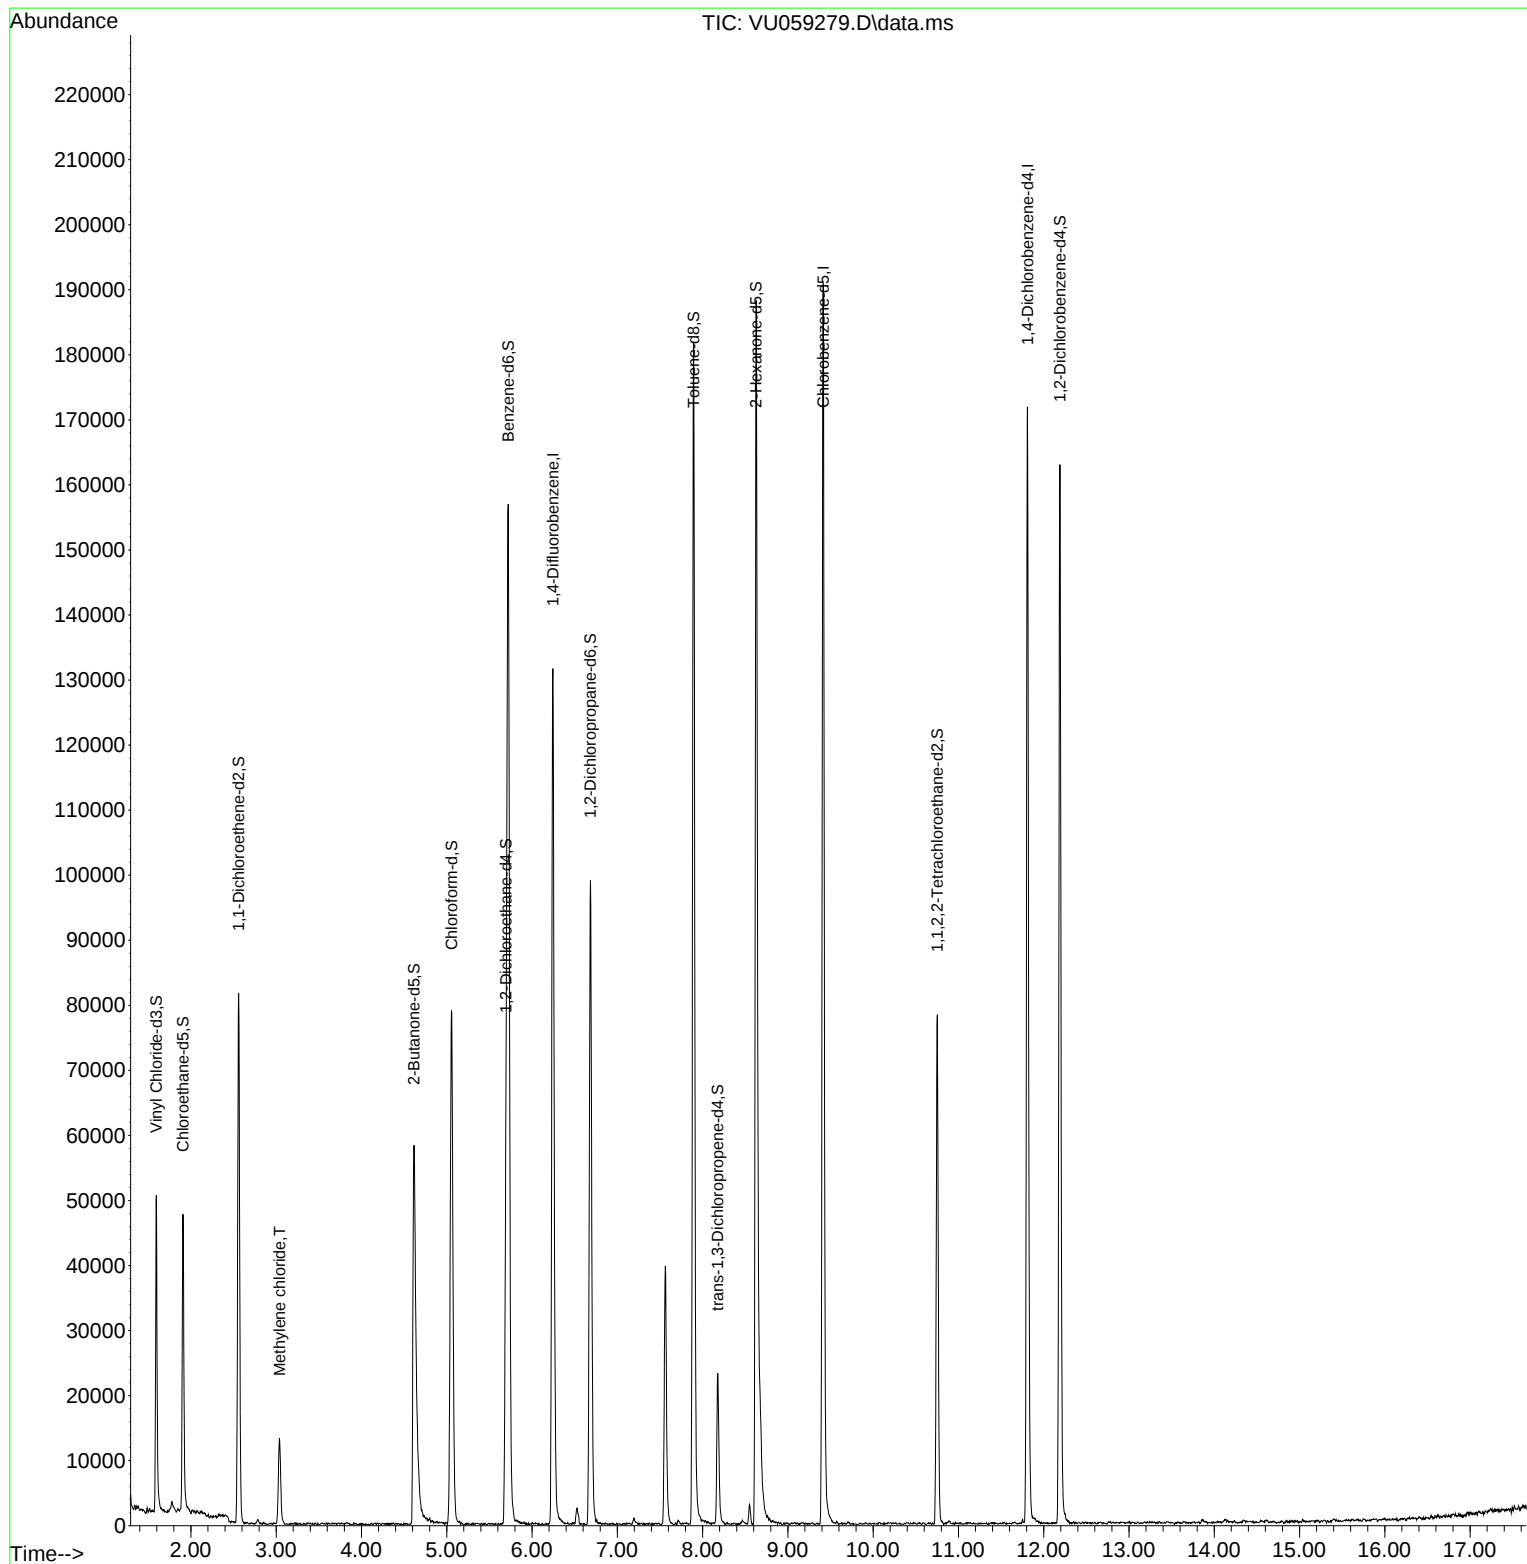

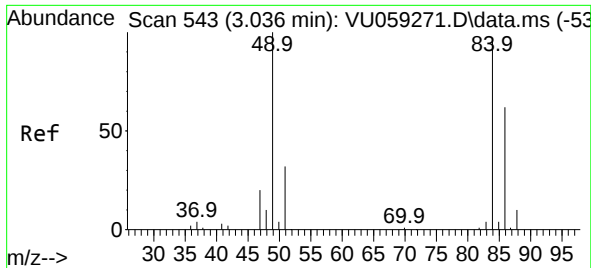

#16
Methylene chloride
Concen: 0.779 ug/L
RT: 3.039 min Scan# 54
Delta R.T. -0.000 min
Lab File: VU059279.D
Acq: 17 Jun 2024 14:48

Instrument :
MSVOA_U
ClientSampleId :
VIBLK105

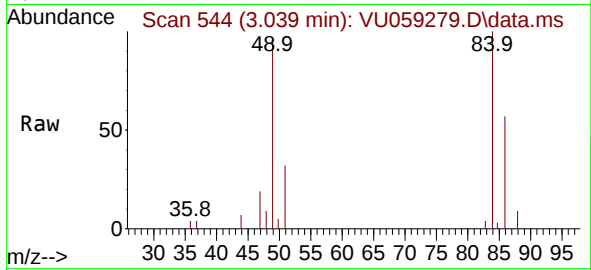

Tgt Ion: 84 Resp: 7314

Ion	Ratio	Lower	Upper
84	100		
86	55.6	42.1	78.1
49	98.4	80.6	149.8

