

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061724\
 Data File : VU059293.D
 Acq On : 17 Jun 2024 20:27
 Operator : MD/SY
 Sample : P2873-14
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0SK2

Quant Time: Jun 18 04:24:28 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jun 17 12:07:46 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	105088	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117	107702	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.811	152	49555	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	31529	4.315	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	86.200%	
7) Chloroethane-d5	1.907	69	32494	4.622	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	92.400%	
11) 1,1-Dichloroethene-d2	2.560	65	12939	4.268	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	85.400%	
20) 2-Butanone-d5	4.615	46	86978	57.785	ug/L	-0.01
Spiked Amount	50.000	Range 40 - 130	Recovery	=	115.560%	
24) Chloroform-d	5.055	84	69231	4.616	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	92.400%	
26) 1,2-Dichloroethane-d4	5.698	65	37035	5.126	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	102.600%	
32) Benzene-d6	5.721	84	134812	4.548	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	91.000%	
36) 1,2-Dichloropropane-d6	6.685	67	43901	4.833	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	96.600%	
41) Toluene-d8	7.894	98	108323	3.931	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	78.600%	
43) trans-1,3-Dichloroprop...	8.177	79	12407	4.362	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	87.200%	
46) 2-Hexanone-d5	8.627	63	62070	52.524	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	105.040%	
56) 1,1,2,2-Tetrachloroeth...	10.753	84	38403	5.117	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	102.400%	
66) 1,2-Dichlorobenzene-d4	12.190	152	43525	4.935	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	98.600%	
Target Compounds						Qvalue
13) Acetone	2.618	43	26042	26.671	ug/L	98
16) Methylene chloride	3.039	84	2633	0.298	ug/L	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061724\
Data File : VU059293.D
Acq On : 17 Jun 2024 20:27
Operator : MD/SY
Sample : P2873-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0SK2

Quant Time: Jun 18 04:24:28 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jun 17 12:07:46 2024
Response via : Initial Calibration

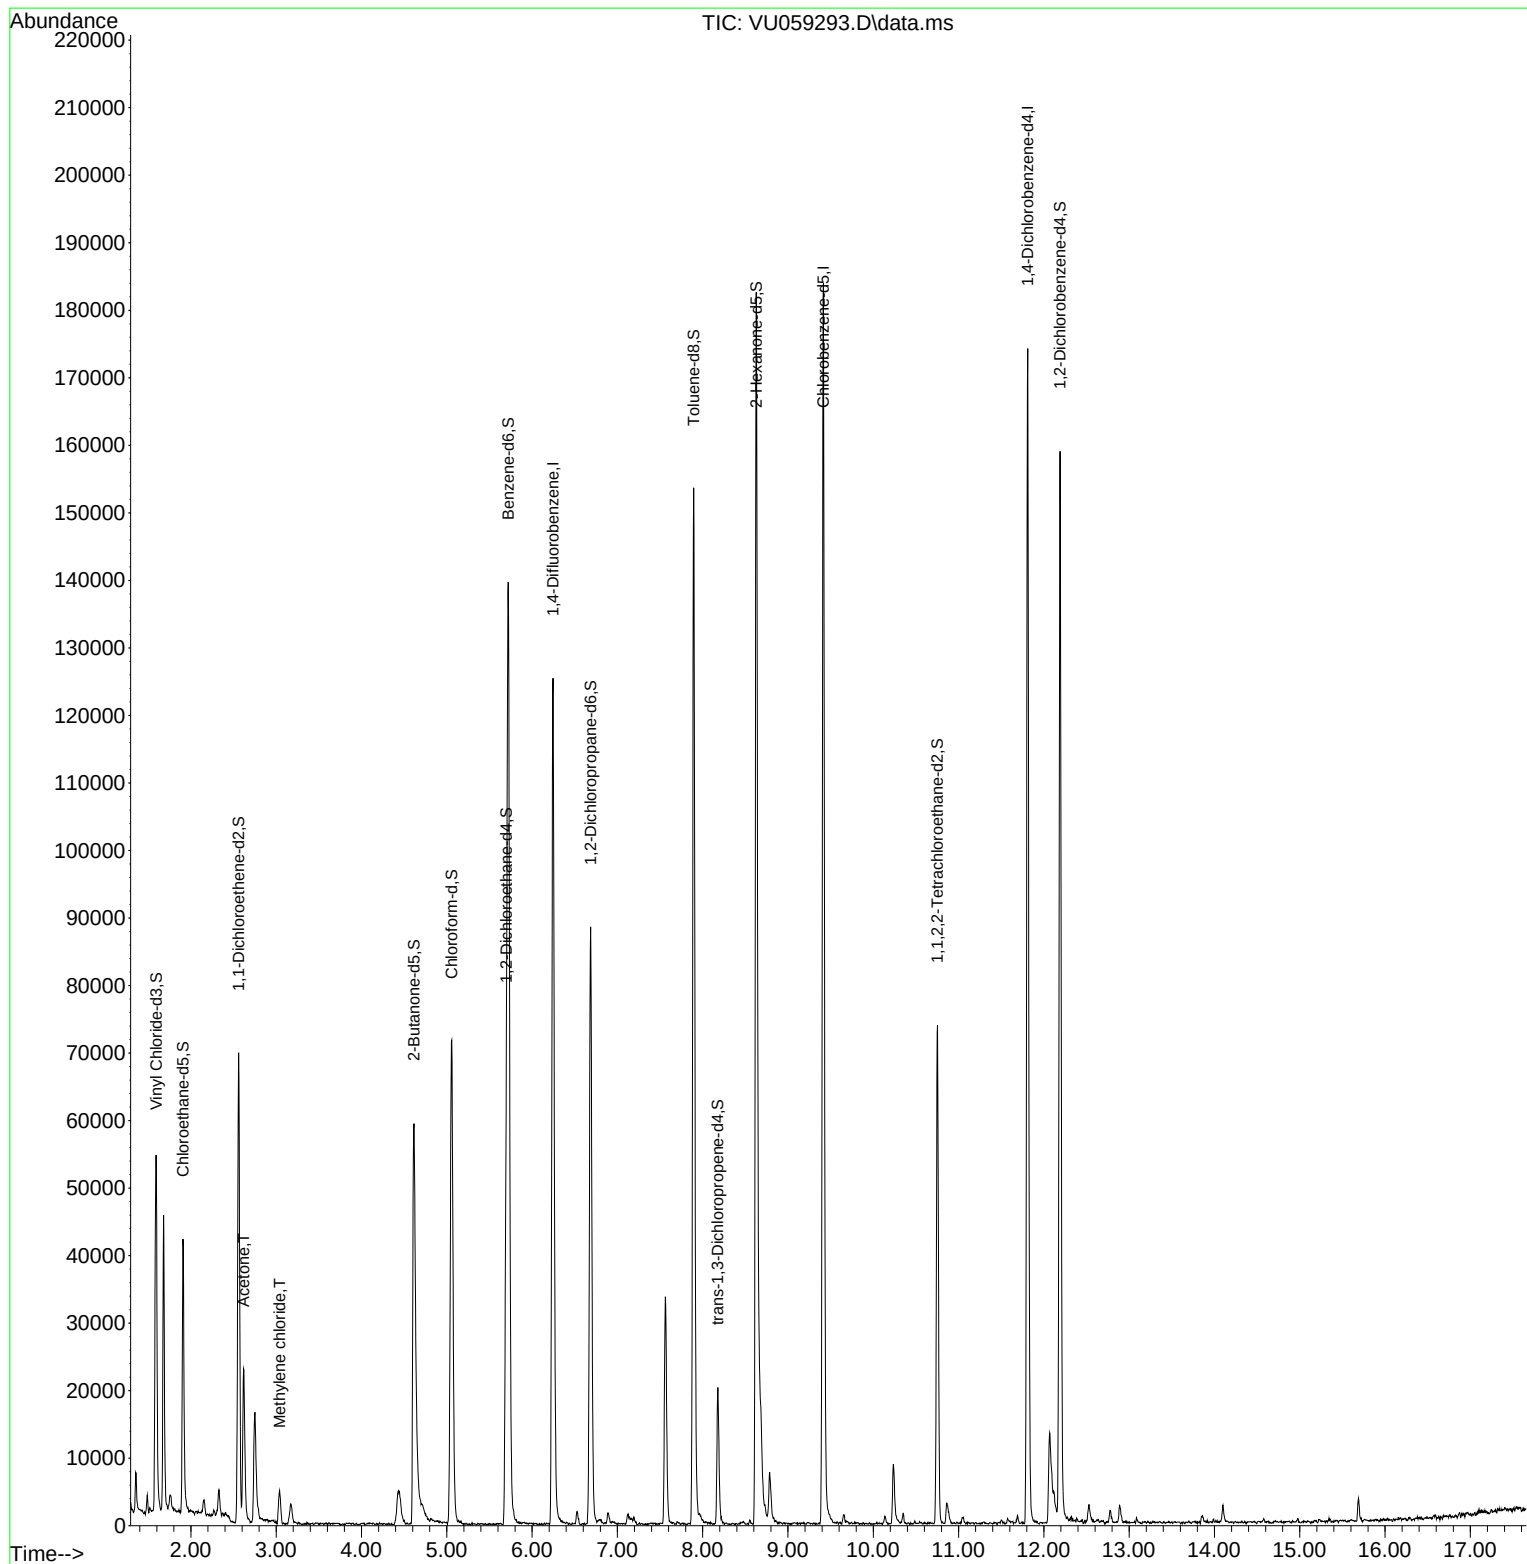

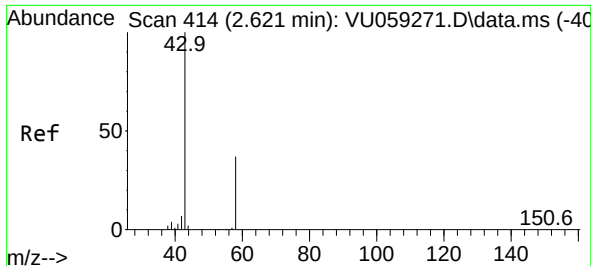

#13

Acetone

Concen: 26.671 ug/L

RT: 2.618 min Scan# 41

Delta R.T. -0.023 min

Lab File: VU059293.D

Acq: 17 Jun 2024 20:27

Instrument :

MSVOA_U

ClientSampleId :





C0SK2

Tgt Ion: 43 Resp: 26042

Ion Ratio Lower Upper

43 100

58 35.1 0.0 68.0

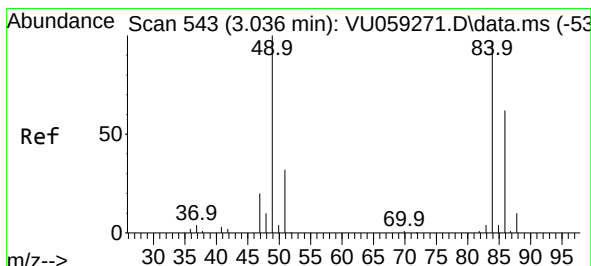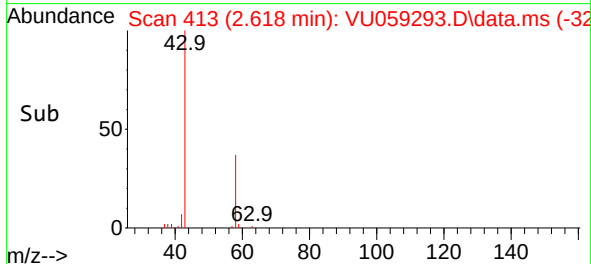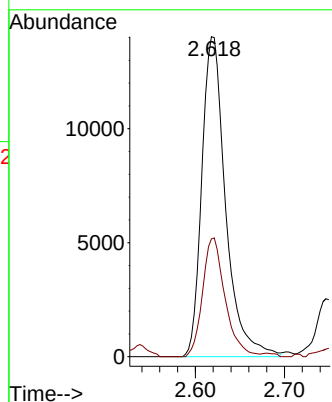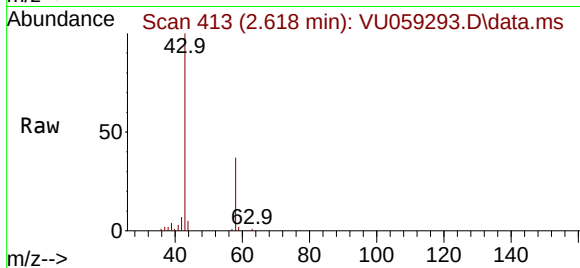

#16

Methylene chloride

Concen: 0.298 ug/L

RT: 3.039 min Scan# 544

Delta R.T. -0.000 min

Lab File: VU059293.D

Acq: 17 Jun 2024 20:27

Tgt Ion: 84 Resp: 2633

Ion Ratio Lower Upper

84 100

86 61.9 42.1 78.1

49 85.5 80.6 149.8

