


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061724\
Data File : VU059268.D
Acq On : 17 Jun 2024 09:06
Operator : MD/SY
Sample : BFB162
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB162

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Mon Jun 17 12:07:46 2024

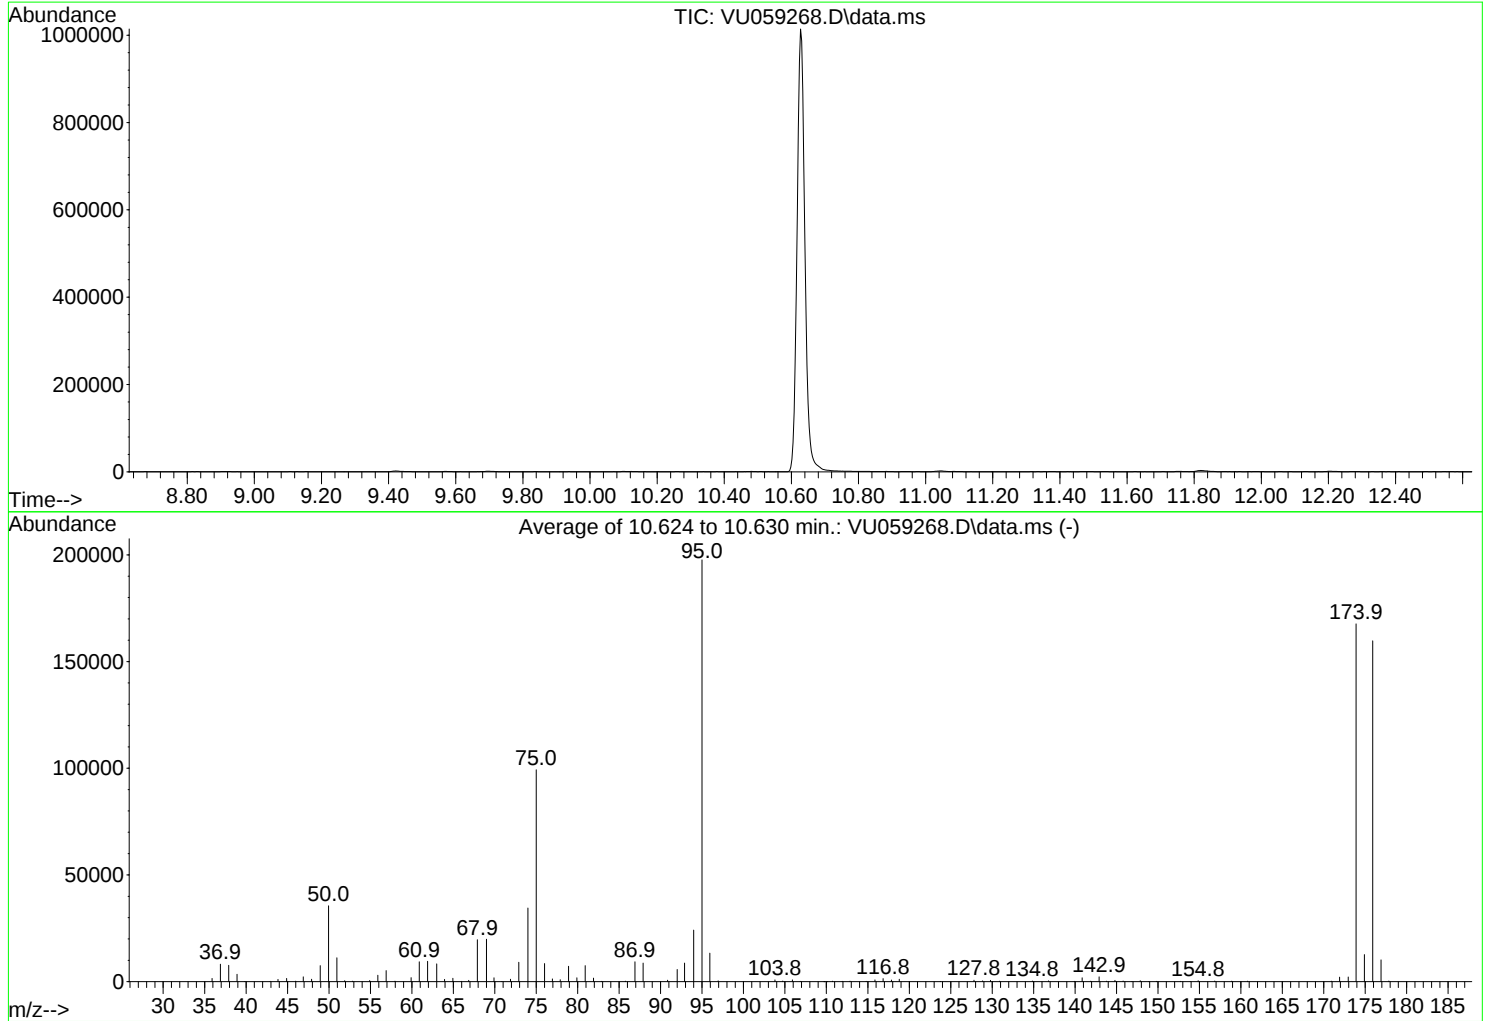

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.0	35557	PASS
75	95	30	80	50.2	99272	PASS
95	95	100	100	100.0	197675	PASS
96	95	5	9	6.8	13370	PASS
173	174	0.00	2	1.3	2173	PASS
174	95	50	120	84.8	167680	PASS
175	174	5	9	7.5	12655	PASS
176	174	95	101	95.3	159744	PASS
177	176	5	9	6.4	10196	PASS

m/z	Abundance
39.80	108.0
43.80	379.0

Instrument :
MSVOA_U
ClientSampleId :
BFB162

m/z	Abundance
35.90	1570.0
36.90	8178.0
37.90	7415.0
38.90	3460.0
39.90	234.0
42.90	108.0
43.90	1382.0
44.90	1451.0
46.00	215.0
46.90	2236.0
47.90	1075.0
48.90	7356.0
50.00	34360.0
51.00	11258.0
51.90	485.0
52.90	171.0
54.90	514.0
55.90	2885.0
56.90	4986.0
57.90	197.0
59.90	1701.0
60.90	8946.0
61.90	9071.0
63.00	7959.0
63.90	1050.0
65.00	1659.0
65.90	161.0
66.90	627.0
67.90	19032.0
69.00	19416.0
69.90	1717.0
71.90	1060.0
72.90	8920.0
74.00	33360.0
75.00	96448.0
76.00	8252.0
76.90	1234.0
77.90	819.0
78.90	7196.0
79.90	1788.0
80.90	7269.0
81.90	1594.0
82.90	112.0
85.80	273.0
86.90	8993.0
87.90	8435.0
90.90	669.0
92.00	5402.0
92.90	8444.0
94.00	23816.0
95.00	190272.0
96.00	13309.0
96.90	327.0
103.80	848.0
104.80	264.0
105.90	751.0
106.80	171.0
109.70	101.0
110.70	201.0
112.00	126.0
112.80	223.0
114.80	167.0
115.90	790.0
116.80	1378.0
117.80	782.0
118.80	1150.0
123.70	112.0
127.80	596.0
128.80	308.0
129.80	555.0
130.90	244.0
134.90	274.0
136.80	341.0
139.90	181.0
140.80	1741.0
141.90	219.0
142.90	2264.0
143.80	175.0
144.80	723.0
145.80	230.0
146.80	115.0
147.90	432.0
148.90	136.0
149.80	189.0
152.70	134.0
154.80	384.0
156.80	291.0
158.90	206.0
160.80	187.0
170.90	313.0
171.90	2145.0
172.90	2103.0

Instrument :
MSVOA_U
ClientSampleId :
BFB162

173.90	156608.0
174.90	12014.0
175.90	149376.0
176.90	9722.0
177.80	305.0

Instrument :
MSVOA_U
ClientSampleId :
BFB162

m/z	Abundance
35.90	1537.0
36.90	8464.0
37.90	7907.0
38.90	3530.0
39.90	215.0
42.90	128.0
43.90	1461.0
44.90	1509.0
46.00	266.0
46.90	2333.0
47.90	1172.0
49.00	7667.0
49.90	36760.0
50.90	11483.0
51.90	476.0
52.90	201.0
54.90	584.0
55.90	3117.0
56.90	5408.0
57.90	223.0
59.90	1929.0
60.90	9591.0
61.90	9844.0
63.00	8688.0
63.90	1056.0
64.90	1611.0
66.00	175.0
66.90	611.0
67.90	20344.0
69.00	20576.0
69.90	1817.0
70.80	114.0
71.90	1172.0
72.90	9433.0
74.00	35744.0
75.00	102928.0
76.00	8674.0
77.00	1312.0
77.90	926.0
78.90	7505.0
79.90	1829.0
80.90	7720.0
81.90	1678.0
82.80	120.0
85.80	260.0
86.90	9558.0
87.90	9052.0
90.80	737.0
92.00	5960.0
92.90	8996.0
94.00	24944.0
95.00	204736.0
96.00	13865.0
97.00	394.0
103.80	909.0
104.80	273.0
105.90	836.0
106.80	194.0
110.80	233.0
111.90	128.0
112.80	218.0
114.80	184.0
115.90	861.0
116.90	1465.0
117.90	794.0
118.80	1158.0
123.80	101.0
127.80	676.0
128.80	380.0
129.80	647.0
130.90	273.0
134.90	323.0
136.80	392.0
139.90	174.0
140.80	1878.0
141.90	265.0
142.90	2345.0
143.80	198.0
144.80	616.0
145.80	301.0
146.90	100.0
147.90	480.0
148.90	108.0
149.80	173.0
152.80	126.0
153.90	127.0
154.90	449.0
156.90	299.0
158.90	236.0
160.80	237.0
170.90	266.0
171.90	2174.0

Instrument :
MSVOA_U
ClientSampleId :
BFB162

172.90	2248.0
173.90	173184.0
174.90	13085.0
175.90	165632.0
176.90	10550.0
177.90	321.0

Instrument :
MSVOA_U
ClientSampleId :
BFB162

m/z	Abundance
35.90	1432.0
36.90	7935.0
37.90	7572.0
38.90	3290.0
39.90	180.0
42.90	124.0
43.90	1523.0
44.90	1492.0
46.00	273.0
46.90	2212.0
47.90	1179.0
48.90	7441.0
49.90	35552.0
50.90	10711.0
51.90	420.0
52.80	211.0
54.90	547.0
55.90	2972.0
56.90	5244.0
58.00	265.0
59.90	1945.0
60.90	9309.0
61.90	9768.0
63.00	8379.0
64.00	1022.0
65.00	1484.0
66.00	167.0
66.80	536.0
67.90	19680.0
69.00	19736.0
69.90	1771.0
70.90	111.0
71.90	1170.0
72.90	8957.0
74.00	34320.0
75.00	98440.0
76.00	8403.0
77.00	1280.0
77.90	924.0
78.90	6928.0
79.90	1729.0
80.90	7439.0
81.90	1593.0
82.80	145.0
85.70	238.0
86.90	9245.0
87.90	8734.0
90.80	732.0
92.00	5788.0
92.90	8673.0
94.00	23656.0
95.00	198016.0
95.90	12936.0
97.00	391.0
103.80	843.0
104.70	278.0
105.90	864.0
106.90	204.0
110.00	100.0
110.80	223.0
111.80	118.0
112.90	189.0
114.80	198.0
115.80	792.0
116.90	1373.0
117.90	760.0
118.80	1075.0
127.80	687.0
128.90	371.0
129.80	699.0
130.90	290.0
134.80	311.0
136.80	364.0
139.90	160.0
140.90	1766.0
141.90	278.0
142.90	2257.0
143.80	202.0
144.80	480.0
145.80	334.0
147.80	459.0
149.80	151.0
152.80	118.0
153.90	173.0
154.90	494.0
156.80	313.0
158.90	237.0
160.80	220.0
170.90	182.0
171.90	2044.0
173.00	2167.0
173.90	173248.0

Instrument :
MSVOA_U
ClientSampleId :
BFB162

174.90	12866.0
175.90	164224.0
176.90	10315.0
177.90	303.0

Instrument :
MSVOA_U
ClientSampleId :
BFB162