

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU061824\  
 Data File : VU059320.D  
 Acq On : 18 Jun 2024 18:45  
 Operator : MD/SY  
 Sample : P2856-16  
 Misc : 5.19g/5.0mL/100uL/5.0mL/MSVOA\_U/MEOH  
 ALS Vial : 28 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :

Quant Time: Jun 19 05:37:39 2024  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMULM052924WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Wed Jun 19 05:32:50 2024  
 Response via : Initial Calibration


| Compound                      | R.T.    | QIon  | Response | Conc     | Units  | Dev(Min) |
|-------------------------------|---------|-------|----------|----------|--------|----------|
| -----                         |         |       |          |          |        |          |
| Internal Standards            |         |       |          |          |        |          |
| 1) 1,4-Difluorobenzene        | 6.242   | 114   | 166222   | 50.000   | ug/L   | 0.00     |
| 28) Chlorobenzene-d5          | 9.415   | 117   | 169048   | 50.000   | ug/L   | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 11.810  | 152   | 86418    | 50.000   | ug/L   | 0.00     |
|                               |         |       |          |          |        |          |
| System Monitoring Compounds   |         |       |          |          |        |          |
| 4) Vinyl Chloride-d3          | 1.592   | 65    | 36356    | 36.530   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000  | Range | 60 - 135 | Recovery | =      | 73.060%  |
| 7) Chloroethane-d5            | 1.872   | 69    | 21205    | 24.873   | ug/L   | -0.04    |
| Spiked Amount                 | 50.000  | Range | 70 - 130 | Recovery | =      | 49.740%# |
| 11) 1,1-Dichloroethene-d2     | 2.592   | 63    | 39       | 0.020    | ug/L   | 0.03     |
| Spiked Amount                 | 50.000  | Range | 60 - 125 | Recovery | =      | 0.040%#  |
| 21) 2-Butanone-d5             | 4.628   | 46    | 72551    | 77.340   | ug/L   | 0.02     |
| Spiked Amount                 | 100.000 | Range | 40 - 130 | Recovery | =      | 77.340%  |
| 24) Chloroform-d              | 5.052   | 84    | 79025    | 39.886   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000  | Range | 70 - 125 | Recovery | =      | 79.780%  |
| 26) 1,2-Dichloroethane-d4     | 5.692   | 65    | 53323    | 43.911   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000  | Range | 70 - 125 | Recovery | =      | 87.820%  |
| 32) Benzene-d6                | 5.714   | 84    | 158748   | 40.915   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000  | Range | 70 - 125 | Recovery | =      | 81.840%  |
| 36) 1,2-Dichloropropane-d6    | 6.682   | 67    | 53610    | 40.074   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000  | Range | 70 - 120 | Recovery | =      | 80.140%  |
| 41) Toluene-d8                | 7.894   | 98    | 132607   | 40.261   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000  | Range | 80 - 120 | Recovery | =      | 80.520%  |
| 43) trans-1,3-Dichloroprop... | 8.177   | 79    | 20790    | 38.446   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000  | Range | 60 - 125 | Recovery | =      | 76.900%  |
| 47) 2-Hexanone-d5             | 8.637   | 63    | 50012    | 80.843   | ug/L   | 0.00     |
| Spiked Amount                 | 100.000 | Range | 45 - 130 | Recovery | =      | 80.840%  |
| 56) 1,1,2,2-Tetrachloroeth... | 10.756  | 84    | 88644    | 39.152   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000  | Range | 65 - 120 | Recovery | =      | 78.300%  |
| 66) 1,2-Dichlorobenzene-d4    | 12.193  | 152   | 57824    | 44.837   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000  | Range | 80 - 120 | Recovery | =      | 89.680%  |
|                               |         |       |          |          |        |          |
| Target Compounds              |         |       |          |          |        | Qvalue   |
| 16) Methylene chloride        | 3.026   | 84    | 3658     | 2.302    | ug/L   | 83       |
| 34) Trichloroethene           | 6.531   | 95    | 108513   | 72.600   | ug/L   | 94       |
| 37) 1,2-Dichloropropane       | 6.682   | 63    | 5665     | 3.268    | ug/L # | 90       |
| 45) 1,1,2-Trichloroethane     | 8.544   | 97    | 5060     | 3.247    | ug/L # | 1        |
| 46) Tetrachloroethene         | 8.547   | 164   | 660813   | 663.747  | ug/L   | 92       |
| 52) Ethylbenzene              | 9.566   | 91    | 147526   | 23.354   | ug/L   | 90       |
| 53) m,p-Xylene                | 9.692   | 106   | 81473    | 35.093   | ug/L   | 90       |
| 54) o-Xylene                  | 10.100  | 106   | 16334    | 7.260    | ug/L   | 99       |
| 62) 1,3,5-Trimethylbenzene    | 11.090  | 105   | 6939     | 1.575    | ug/L   | 98       |
| 63) 1,2,4-Trimethylbenzene    | 11.470  | 105   | 21866    | 4.579    | ug/L   | 100      |
| 71) Naphthalene               | 14.084  | 128   | 360874   | 76.065   | ug/L   | 99       |
| -----                         |         |       |          |          |        |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU061824\  
Data File : VU059320.D  
Acq On : 18 Jun 2024 18:45  
Operator : MD/SY  
Sample : P2856-16  
Misc : 5.19g/5.0mL/100uL/5.0mL/MSVOA\_U/MEOH  
ALS Vial : 28 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :


Quant Time: Jun 19 05:37:39 2024  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMULM052924WMA.M  
Quant Title : VOC Analysis  
QLast Update : Wed Jun 19 05:32:50 2024  
Response via : Initial Calibration

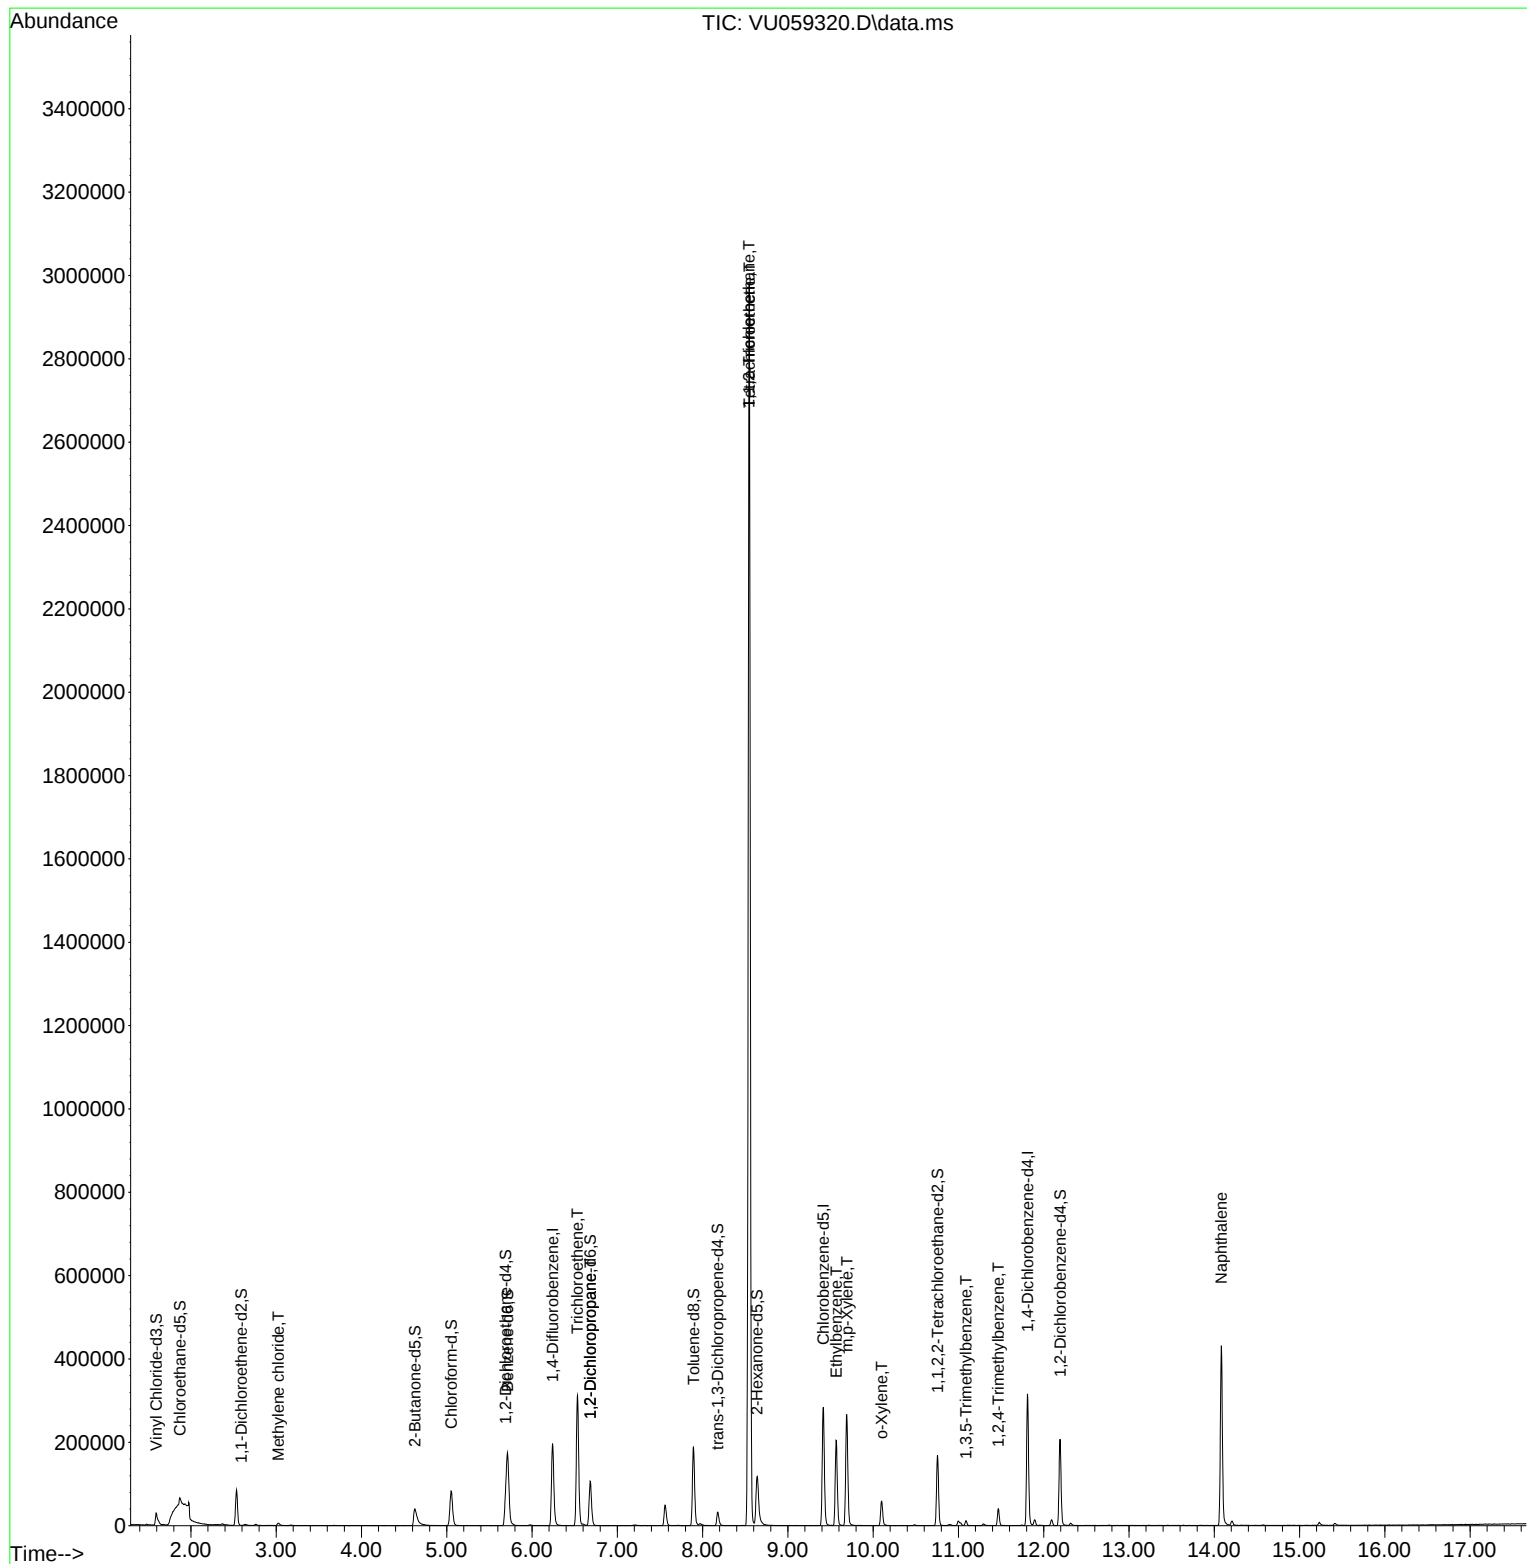



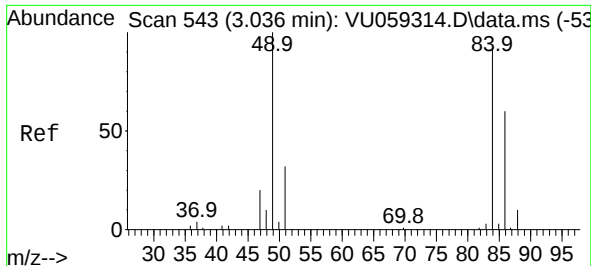


#16  
Methylene chloride  
Concen: 2.302 ug/L  
RT: 3.026 min Scan# 54  
Delta R.T. -0.010 min  
Lab File: VU059320.D  
Acq: 18 Jun 2024 18:45

Instrument :  
MSVOA\_U  
ClientSampleId :



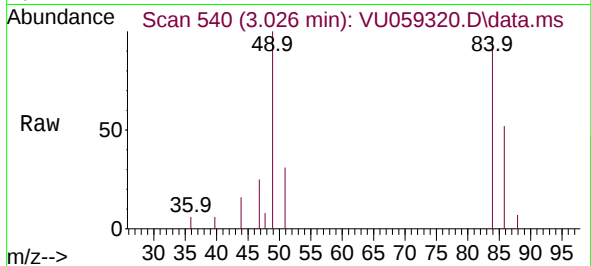



Tgt Ion: 84 Resp: 3658  
Ion Ratio Lower Upper  
84 100  
86 53.7 44.9 83.3  
49 103.1 87.5 162.5

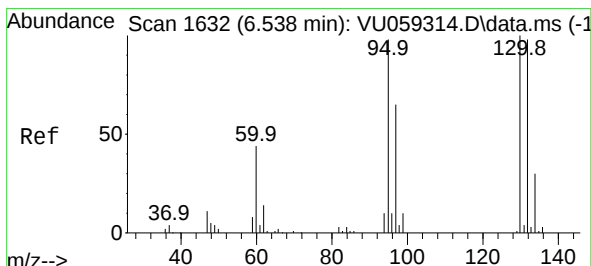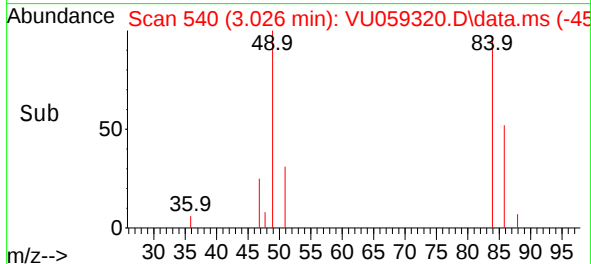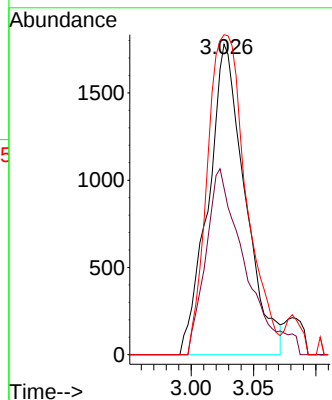

#34  
Trichloroethene  
Concen: 72.600 ug/L  
RT: 6.531 min Scan# 1630  
Delta R.T. -0.007 min  
Lab File: VU059320.D  
Acq: 18 Jun 2024 18:45

Tgt Ion: 95 Resp: 108513  
Ion Ratio Lower Upper  
95 100  
97 64.8 45.2 84.0  
132 94.1 60.6 112.6  
130 98.2 62.9 116.7


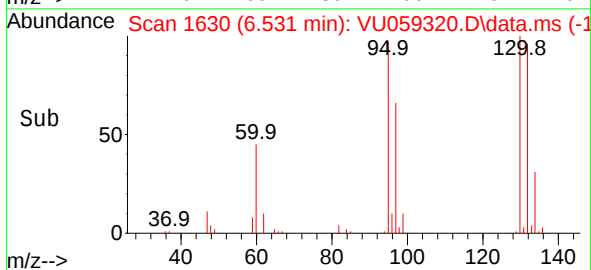
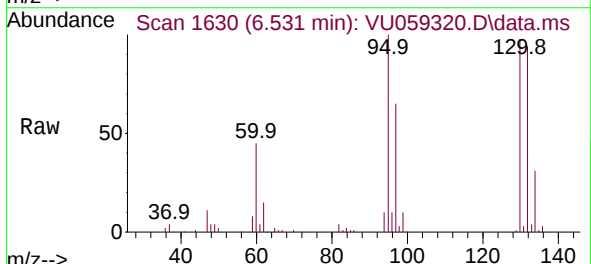
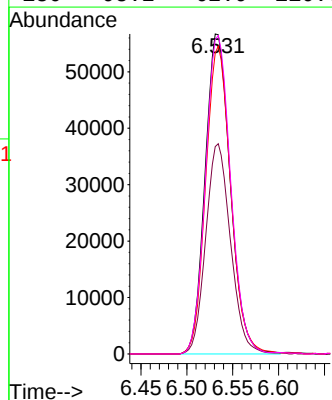


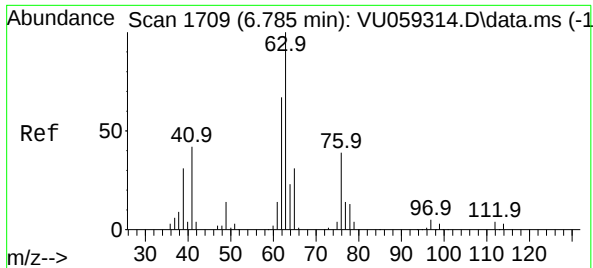

#37  
1,2-Dichloropropane  
Concen: 3.268 ug/L  
RT: 6.682 min Scan# 1  
Delta R.T. -0.103 min  
Lab File: VU059320.D  
Acq: 18 Jun 2024 18:45




Instrument :  
MSVOA\_U  
ClientSampleId :


Tgt Ion: 63 Resp: 5665  
Ion Ratio Lower Upper  
63 100  
112 0.0 2.6 4.0#

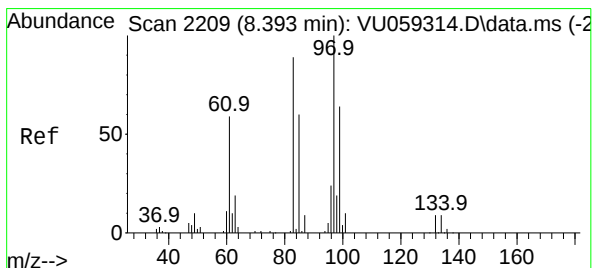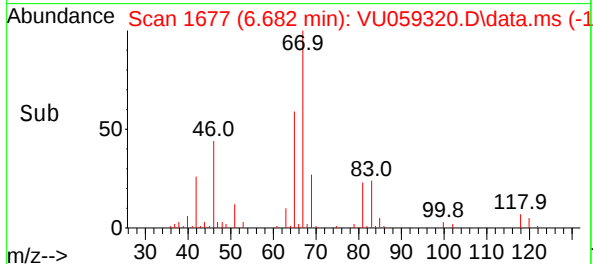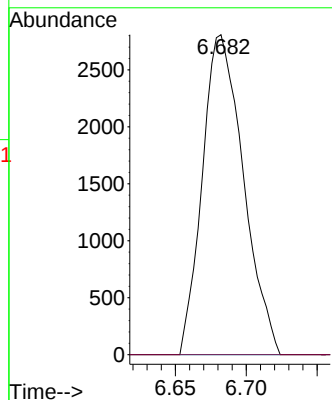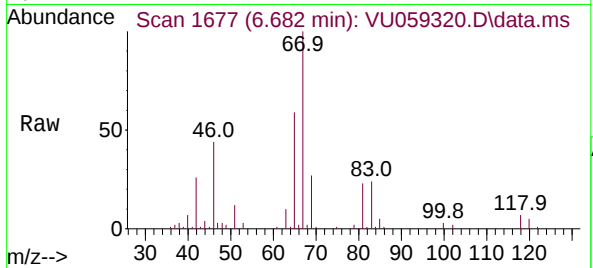

#45  
1,1,2-Trichloroethane  
Concen: 3.247 ug/L  
RT: 8.544 min Scan# 2256  
Delta R.T. 0.151 min  
Lab File: VU059320.D  
Acq: 18 Jun 2024 18:45

Tgt Ion: 97 Resp: 5060  
Ion Ratio Lower Upper  
97 100  
99 14.8 44.0 81.6#  
83 310.7 63.6 118.2#  
85 52.1 40.8 75.8

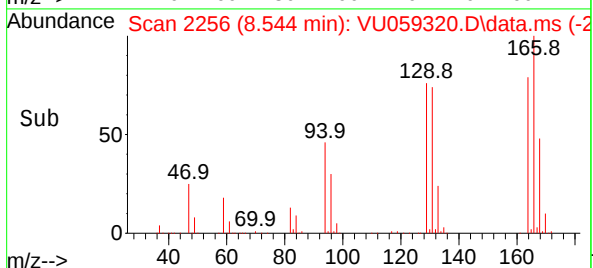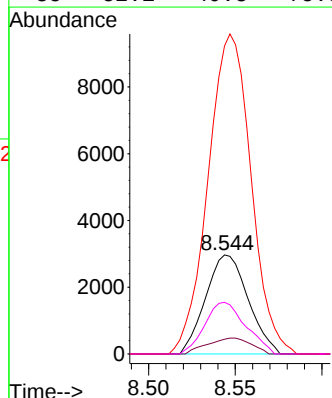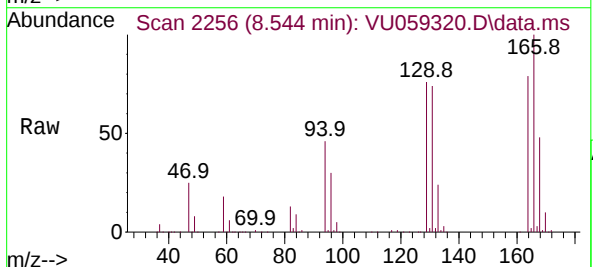

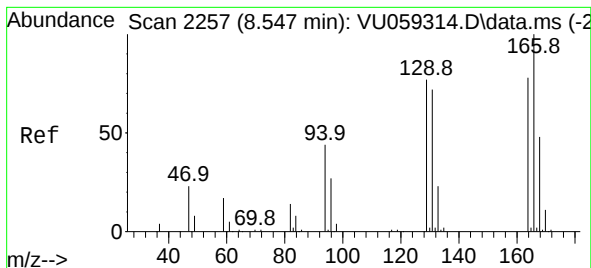

#46

Tetrachloroethene

Concen: 663.747 ug/L

RT: 8.547 min Scan# 21

Delta R.T. -0.000 min MSVOA\_U


Lab File: VU059320.D

Acq: 18 Jun 2024 18:45

Instrument :

MSVOA\_U

ClientSampleId :

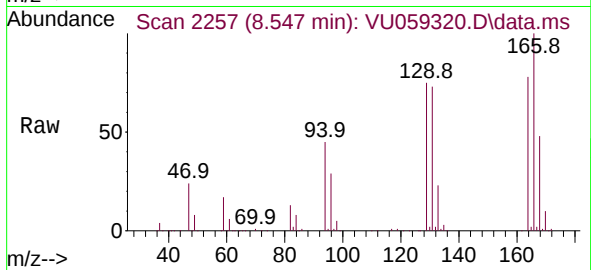

Tgt Ion:164 Resp: 660813




Ion Ratio Lower Upper

164 100

129 95.5 74.5 138.5

131 93.0 70.6 131.0

166 127.8 95.1 176.7

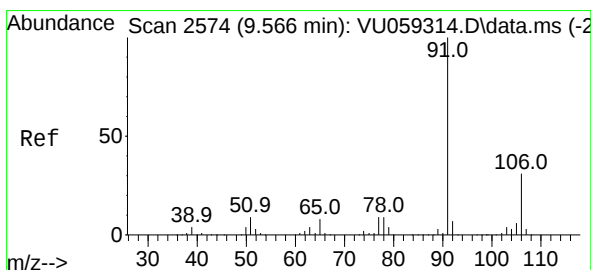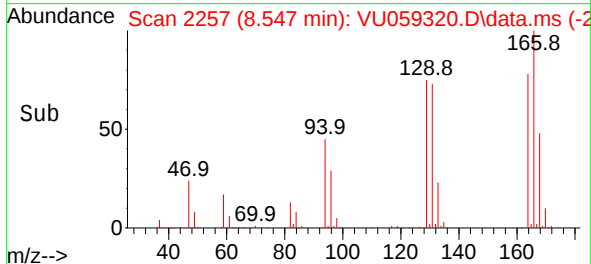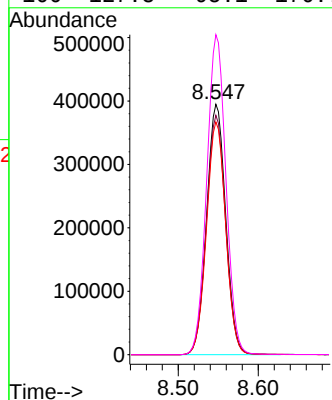

#52

Ethylbenzene

Concen: 23.354 ug/L

RT: 9.566 min Scan# 2574

Delta R.T. -0.000 min

Lab File: VU059320.D




Acq: 18 Jun 2024 18:45


Tgt Ion: 91 Resp: 147526

Ion Ratio Lower Upper

91 100

106 35.3 21.0 39.0


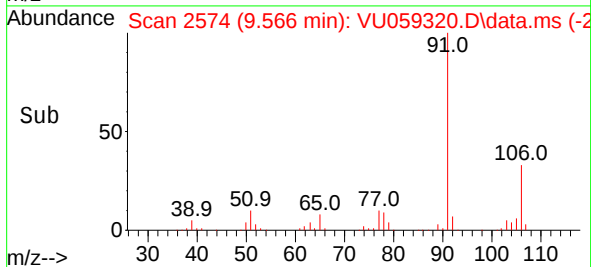
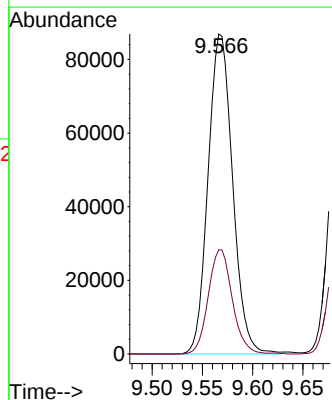
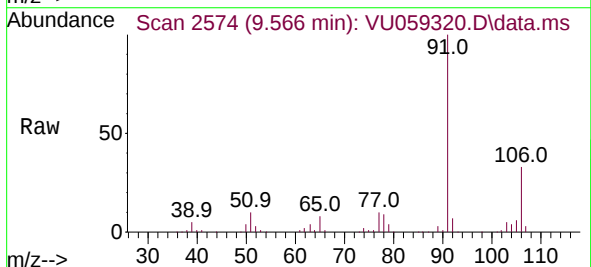


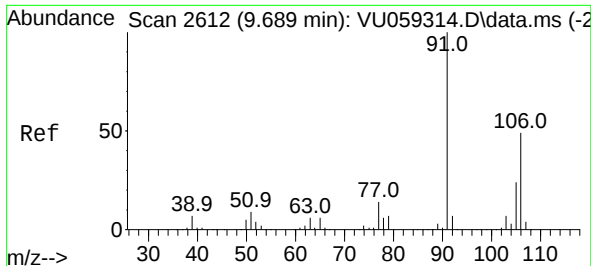

#53  
m,p-Xylene  
Concen: 35.093 ug/L  
RT: 9.692 min Scan# 20  
Delta R.T. 0.003 min  
Lab File: VU059320.D  
Acq: 18 Jun 2024 18:45




Instrument :  
MSVOA\_U  
ClientSampleId :


Tgt Ion:106 Resp: 81473  
Ion Ratio Lower Upper  
106 100  
91 194.3 146.4 272.0

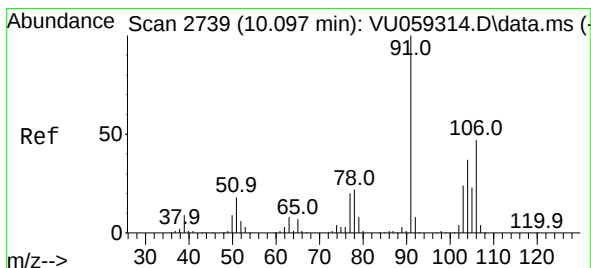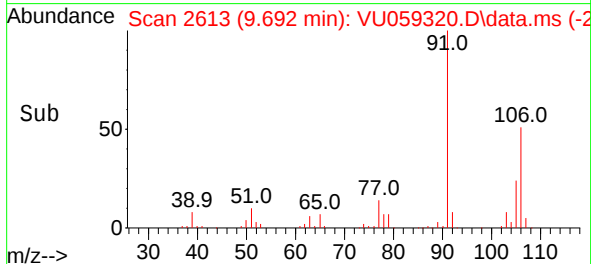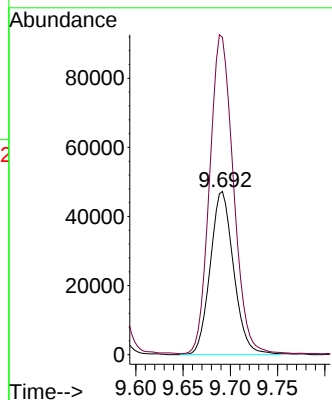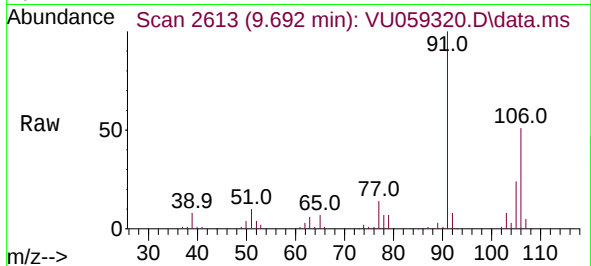

#54  
o-Xylene  
Concen: 7.260 ug/L  
RT: 10.100 min Scan# 2740  
Delta R.T. 0.003 min  
Lab File: VU059320.D  
Acq: 18 Jun 2024 18:45

Tgt Ion:106 Resp: 16334  
Ion Ratio Lower Upper  
106 100  
91 222.6 156.7 290.9

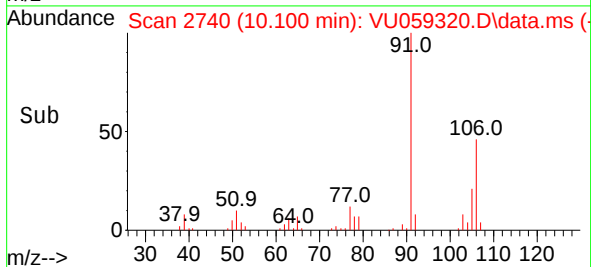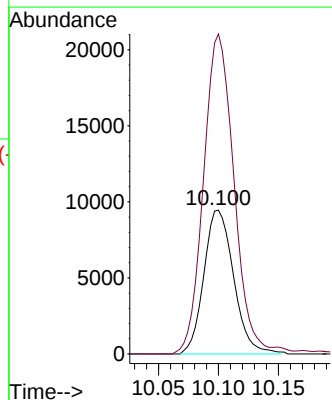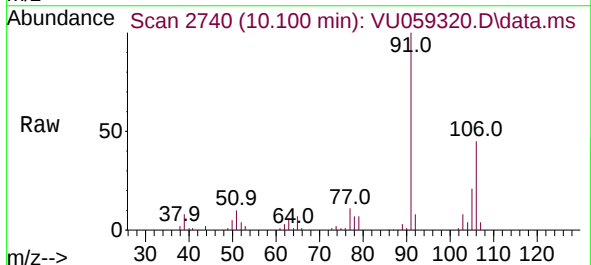

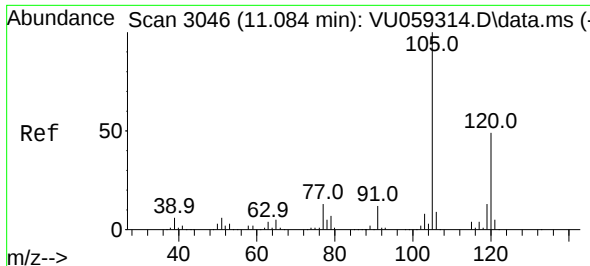

#62

1,3,5-Trimethylbenzene

Concen: 1.575 ug/L

RT: 11.090 min Scan# 3046

Delta R.T. 0.006 min

Lab File: VU059320.D

Acq: 18 Jun 2024 18:45

Instrument :

MSVOA\_U





ClientSampleId :

Tgt Ion:105 Resp: 6939

Ion Ratio Lower Upper

105 100

120 48.8 37.8 56.8

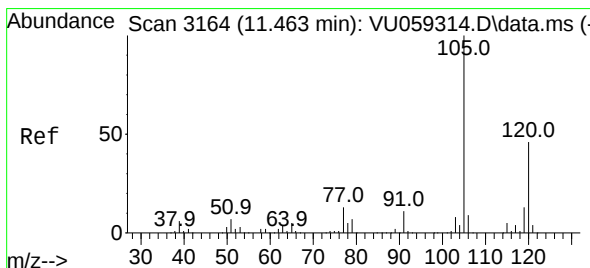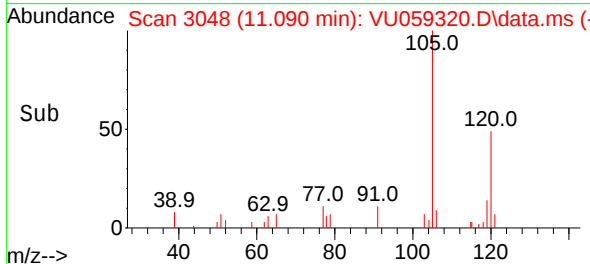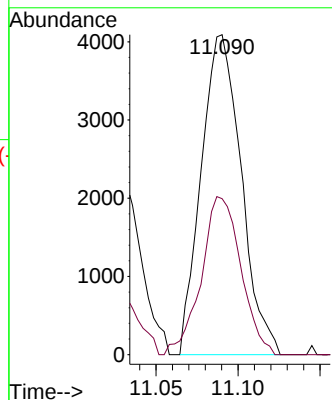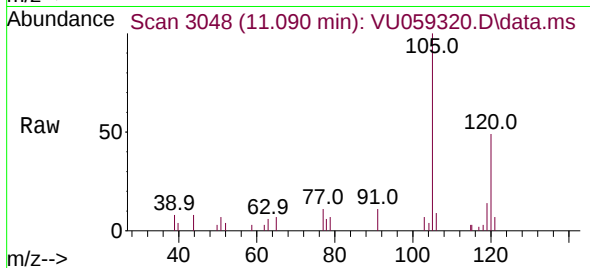

#63

1,2,4-Trimethylbenzene

Concen: 4.579 ug/L

RT: 11.470 min Scan# 3166

Delta R.T. 0.006 min

Lab File: VU059320.D




Acq: 18 Jun 2024 18:45


Tgt Ion:105 Resp: 21866

Ion Ratio Lower Upper

105 100


120 43.7 35.0 52.6

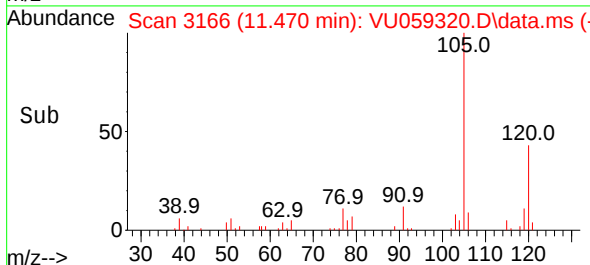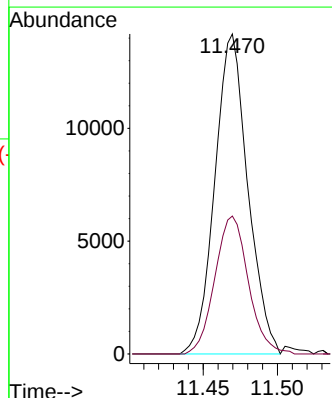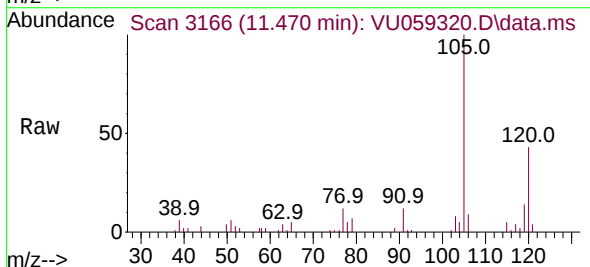

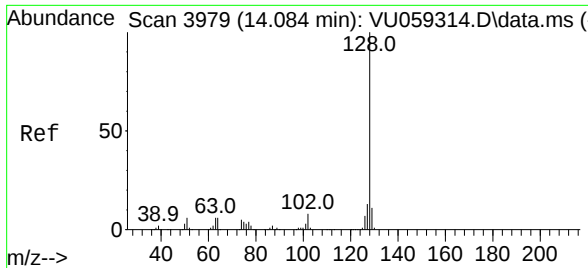

#71  
Naphthalene  
Concen: 76.065 ug/L  
RT: 14.084 min Scan# 3979  
Delta R.T. -0.000 min  
Lab File: VU059320.D  
Acq: 18 Jun 2024 18:45

Instrument :  
MSVOA\_U  
ClientSampleId :

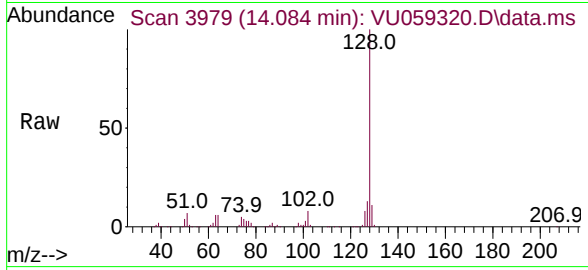

|          |       |       |        |
|----------|-------|-------|--------|
| Tgt Ion: | 128   | Resp: | 360874 |
| Ion      | Ratio | Lower | Upper  |
| 128      | 100   |       |        |
| 127      | 13.2  | 10.4  | 15.6   |
| 129      | 10.8  | 8.5   | 12.7   |

