
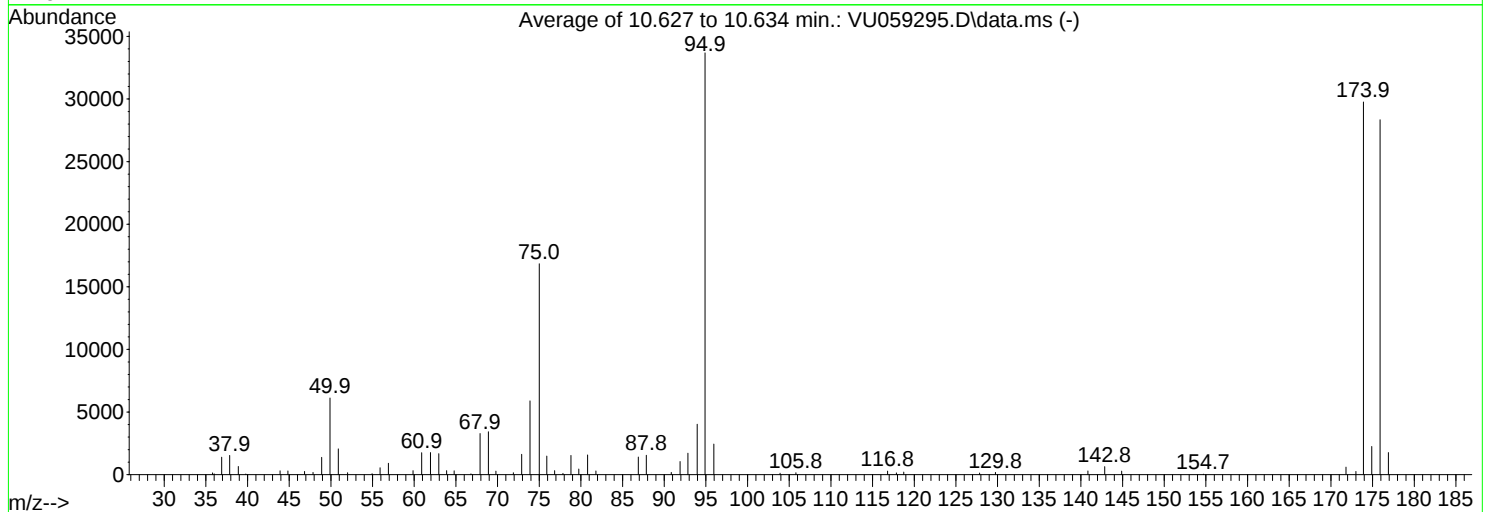


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061824\
Data File : VU059295.D
Acq On : 18 Jun 2024 07:48
Operator : MD/SY
Sample : BFB064
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB064

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Title : VOC Analysis
Last Update : Wed Jun 19 05:32:50 2024

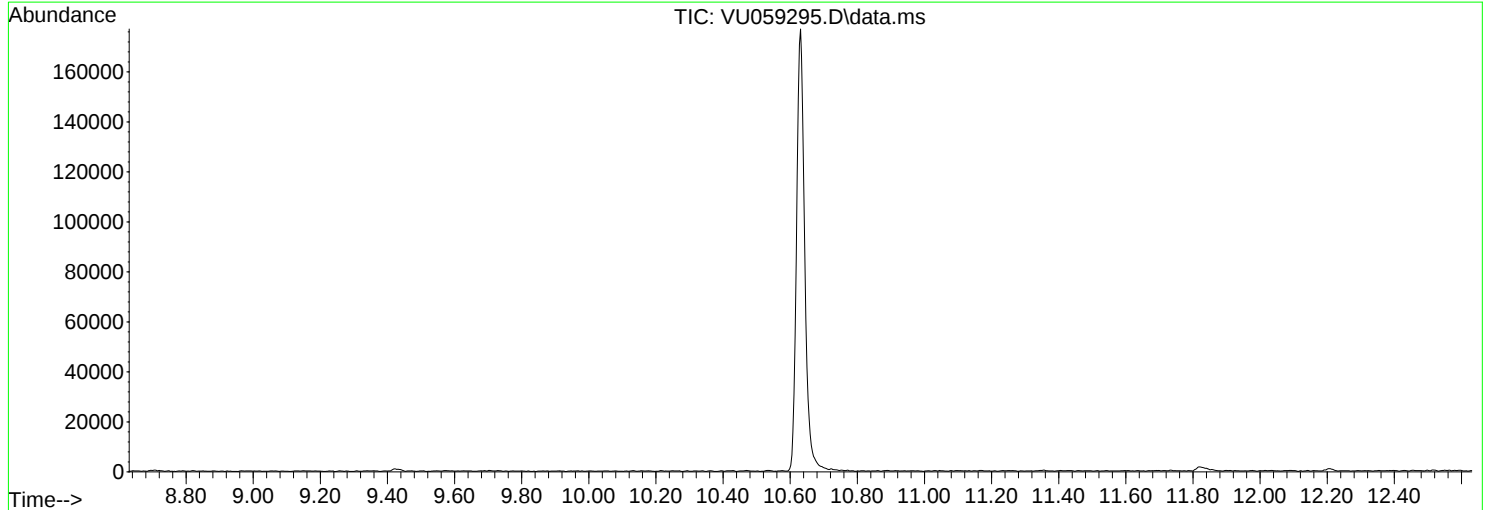

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2892

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.2	6117	PASS
75	95	30	80	50.0	16844	PASS
95	95	100	100	100.0	33688	PASS
96	95	5	9	7.2	2440	PASS
173	174	0.00	2	0.9	260	PASS
174	95	50	120	88.3	29763	PASS
175	174	5	9	7.5	2246	PASS
176	174	95	101	95.2	28339	PASS
177	176	5	9	6.2	1761	PASS

m/z	Abundance
39.90	110.0
43.90	228.0

Instrument :
MSVOA_U
ClientSampleId :
BFB064

m/z	Abundance
35.80	212.0
36.90	1451.0
37.80	1546.0
38.90	644.0
39.70	174.0
43.90	538.0
44.90	317.0
46.90	279.0
47.80	204.0
48.90	1376.0
49.90	6054.0
50.90	2107.0
52.00	138.0
54.90	114.0
55.90	496.0
56.90	963.0
59.90	331.0
60.90	1731.0
61.90	1941.0
63.00	1668.0
63.90	319.0
64.80	273.0
66.80	106.0
67.90	3215.0
68.90	3501.0
69.80	355.0
71.90	172.0
72.90	1640.0
73.90	5927.0
75.00	17176.0
75.90	1475.0
76.80	349.0
78.80	1605.0
79.70	440.0
80.80	1691.0
81.80	289.0
86.90	1365.0
87.90	1514.0
90.90	188.0
91.90	945.0
92.80	1746.0
93.90	3988.0
94.90	33320.0
95.90	2513.0
103.90	141.0
105.80	134.0
116.80	330.0
117.90	156.0
118.70	229.0
127.80	104.0
129.80	187.0
140.90	281.0
142.90	625.0
144.90	296.0
171.80	570.0
173.90	29376.0
174.90	2168.0
175.90	27976.0
176.90	1930.0

Instrument :
MSVOA_U
ClientSampleId :
BFB064

m/z	Abundance
35.80	201.0
36.90	1416.0
37.90	1620.0
38.90	671.0
39.80	167.0
43.90	559.0
44.80	310.0
46.90	229.0
47.90	186.0
48.90	1435.0
49.90	6360.0
50.90	2147.0
52.00	172.0
55.00	114.0
55.90	579.0
56.90	923.0
59.80	335.0
60.90	1811.0
62.00	1842.0
63.00	1747.0
63.90	343.0
64.80	303.0
66.80	104.0
67.90	3384.0
68.90	3580.0
69.80	290.0
71.80	145.0
72.90	1674.0
73.90	6034.0
75.00	17336.0
75.90	1496.0
76.90	328.0
77.90	141.0
78.80	1587.0
79.80	437.0
80.80	1622.0
81.80	283.0
86.90	1429.0
87.90	1651.0
90.90	191.0
91.90	1085.0
92.90	1768.0
94.00	4127.0
94.90	34736.0
96.00	2587.0
103.90	109.0
105.80	145.0
116.80	282.0
117.90	147.0
118.80	202.0
127.80	137.0
129.80	174.0
140.80	312.0
142.90	640.0
144.90	306.0
171.80	602.0
173.00	394.0
173.90	30688.0
174.90	2333.0
175.90	29344.0
176.90	1811.0

Instrument :
MSVOA_U
ClientSampleId :
BFB064

m/z	Abundance
36.00	204.0
36.90	1331.0
37.90	1418.0
38.90	635.0
39.90	137.0
43.90	514.0
44.80	257.0
46.70	255.0
47.90	145.0
48.90	1345.0
49.90	5936.0
50.90	1912.0
52.00	156.0
55.90	590.0
56.90	823.0
59.90	296.0
60.90	1730.0
62.00	1513.0
62.90	1594.0
63.90	304.0
64.80	349.0
67.90	3253.0
68.90	3197.0
69.80	203.0
72.00	130.0
72.90	1568.0
73.90	5723.0
75.00	16019.0
75.90	1471.0
76.90	273.0
77.80	153.0
78.80	1418.0
79.80	449.0
80.80	1399.0
81.80	296.0
86.90	1430.0
87.80	1490.0
90.80	159.0
91.90	1105.0
92.90	1637.0
94.00	3945.0
94.90	33008.0
96.00	2220.0
103.90	102.0
105.80	168.0
116.80	237.0
117.80	125.0
118.80	192.0
127.90	144.0
129.70	161.0
140.80	289.0
142.80	637.0
144.90	240.0
154.70	104.0
171.80	620.0
173.00	387.0
173.90	29224.0
174.90	2237.0
175.90	27696.0
176.90	1543.0

Instrument :
MSVOA_U
ClientSampleId :
BFB064