


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU062018\
 Data File : VU024749.D
 Acq On : 20 Jun 2018 10:13
 Operator : MD/SY
 Sample : BFB
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U061318W.M
 Title : SW846 8260
 Last Update : Wed Jun 13 13:55:26 2018

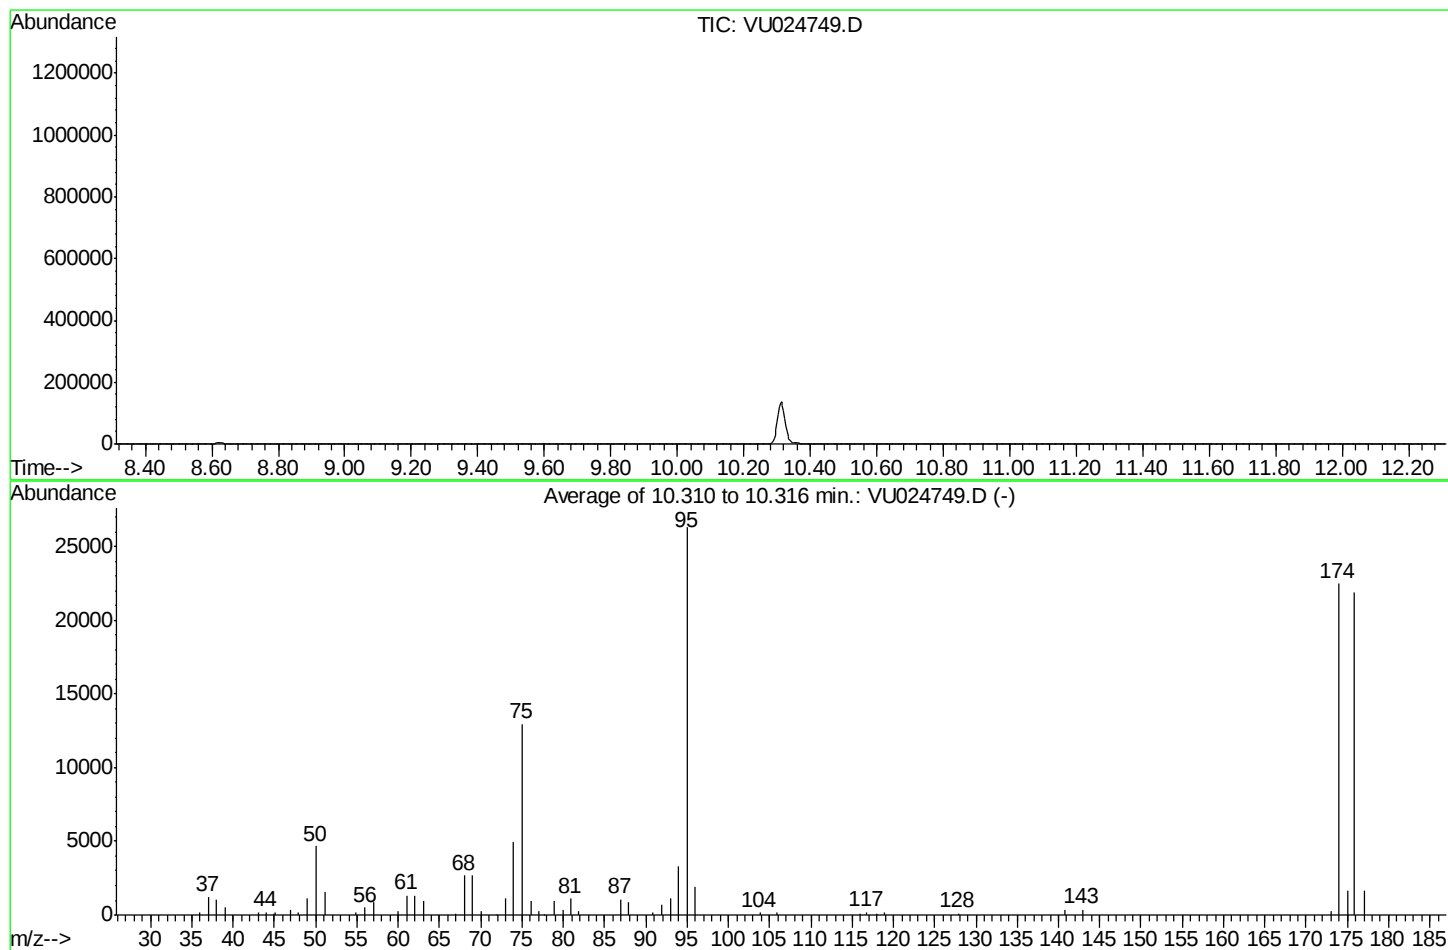

AutoFind: Scans 3023, 3024, 3025; Background Corrected with Scan 3011

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	4673	PASS
75	95	30	60	49.4	12986	PASS
95	95	100	100	100.0	26304	PASS
96	95	5	9	7.2	1885	PASS
173	174	0.00	2	1.3	303	PASS
174	95	50	100	85.4	22461	PASS
175	174	5	9	7.2	1615	PASS
176	174	95	101	97.3	21853	PASS
177	176	5	9	7.5	1633	PASS