

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062024\
 Data File : VU059370.D
 Acq On : 20 Jun 2024 11:24
 Operator : MD/SY
 Sample : P2856-16DL 10X
 Misc : 5.19g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COSJ0DL

Quant Time: Jun 21 05:57:00 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 21 05:55:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	203815	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	213240	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	91534	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	38604	31.634	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	63.260%	
7) Chloroethane-d5	1.898	69	36814	35.217	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	70.440%	
11) 1,1-Dichloroethene-d2	2.557	63	51682	21.456	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	42.920%#	
21) 2-Butanone-d5	4.615	46	65113	56.608	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	56.610%	
24) Chloroform-d	5.055	84	84281	34.693	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	69.380%#	
26) 1,2-Dichloroethane-d4	5.695	65	54016	36.277	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	72.560%	
32) Benzene-d6	5.721	84	164750	33.662	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	67.320%#	
36) 1,2-Dichloropropane-d6	6.682	67	54495	32.293	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	64.580%#	
41) Toluene-d8	7.891	98	138466	33.327	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	66.660%#	
43) trans-1,3-Dichloroprop...	8.174	79	20619	30.228	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	60.460%	
47) 2-Hexanone-d5	8.624	63	39034	50.021	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	50.020%	
56) 1,1,2,2-Tetrachloroeth...	10.749	84	86950	30.445	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	60.880%#	
66) 1,2-Dichlorobenzene-d4	12.187	152	53537	39.193	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	78.380%#	
Target Compounds						
					Qvalue	
34) Trichloroethene	6.537	95	12173	6.456	ug/L	92
46) Tetrachloroethene	8.547	164	78113	62.200	ug/L	88
52) Ethylbenzene	9.566	91	15431	1.937	ug/L	97
53) m,p-Xylene	9.692	106	7571	2.585	ug/L	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062024\
Data File : VU059370.D
Acq On : 20 Jun 2024 11:24
Operator : MD/SY
Sample : P2856-16DL 10X
Misc : 5.19g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0SJ0DL

Quant Time: Jun 21 05:57:00 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 21 05:55:12 2024
Response via : Initial Calibration

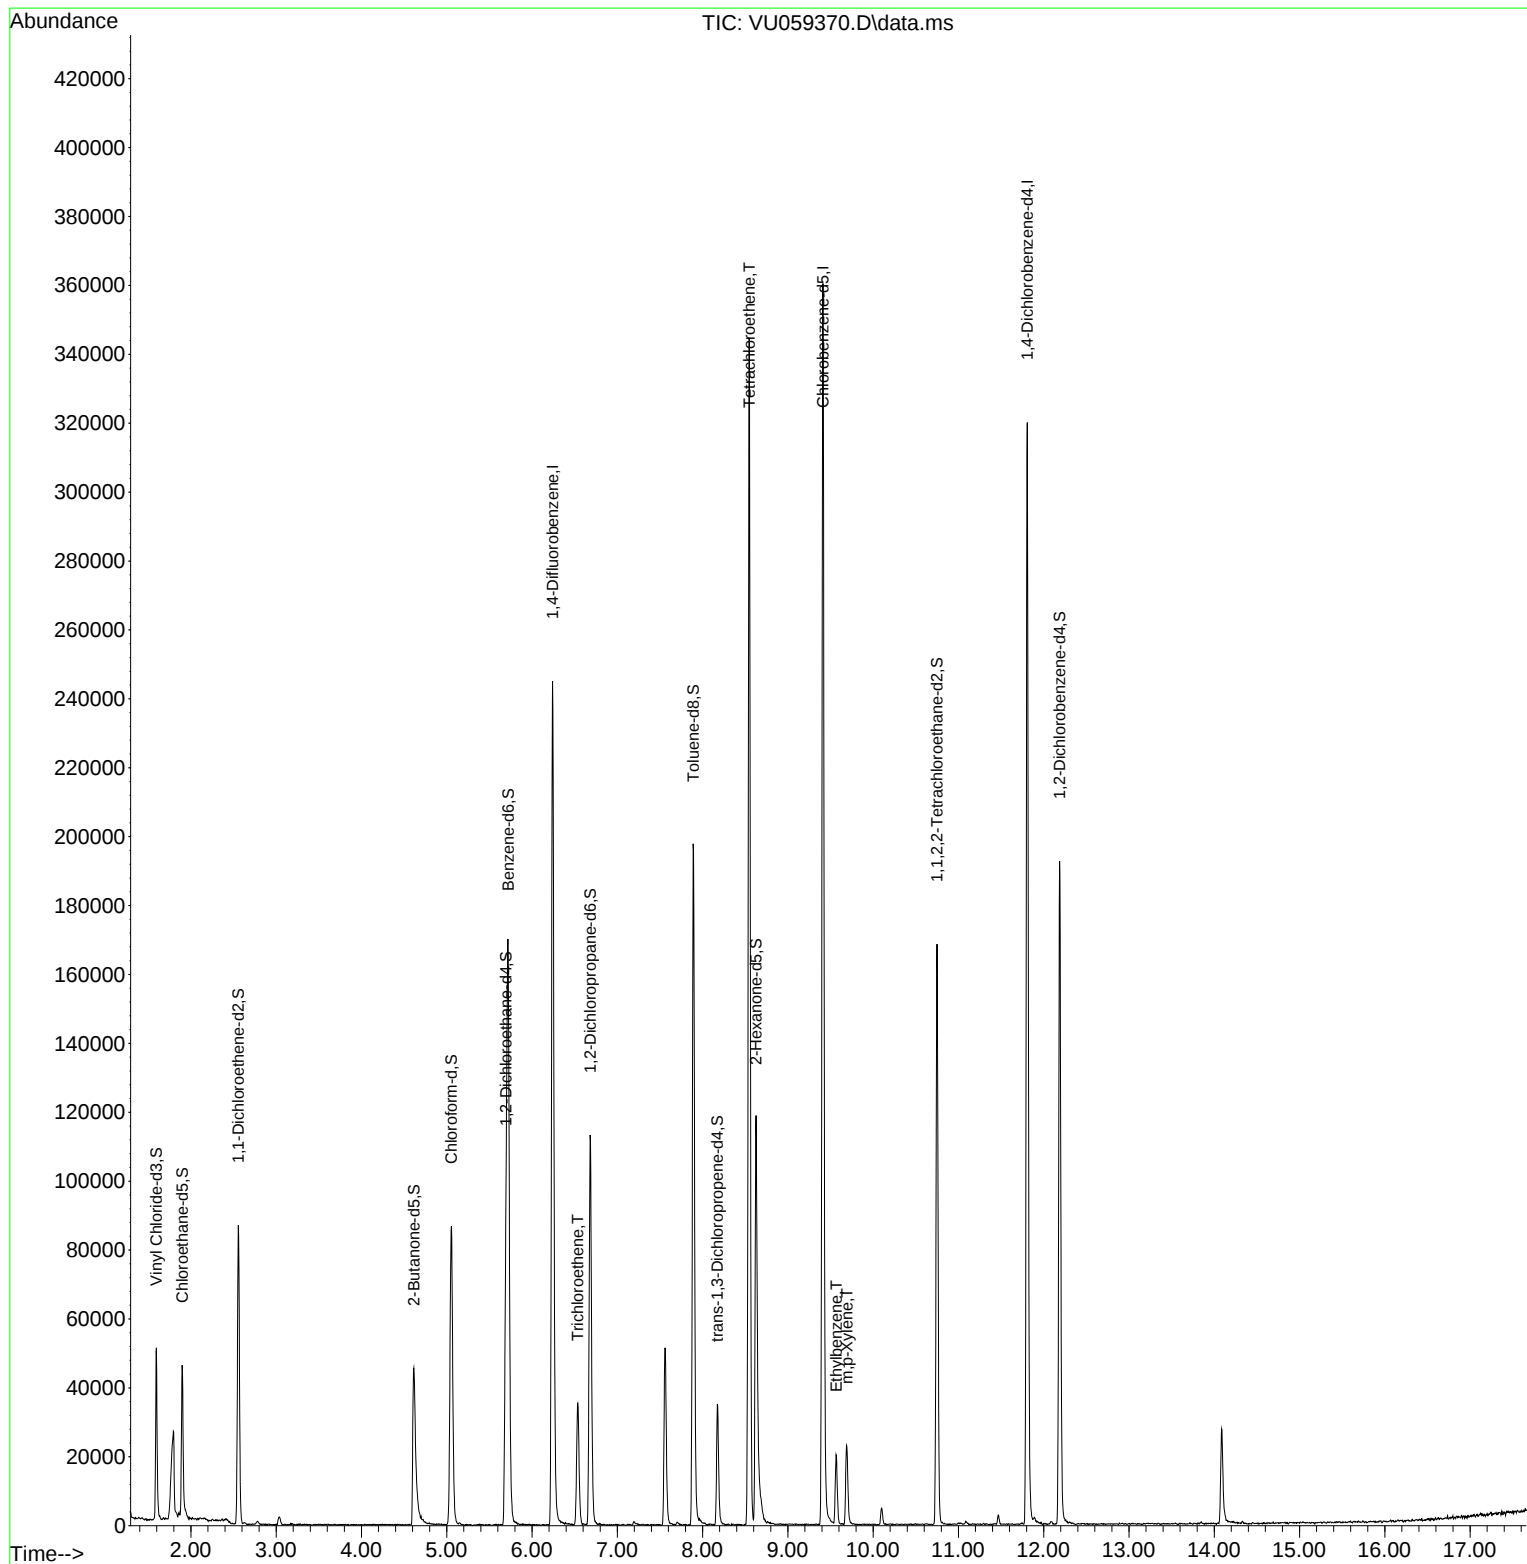




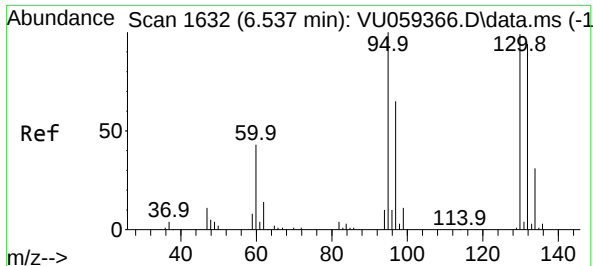


#34
Trichloroethene
Concen: 6.456 ug/L
RT: 6.537 min Scan# 1
Delta R.T. -0.000 min
Lab File: VU059370.D
Acq: 20 Jun 2024 11:24

Instrument :
MSVOA_U
ClientSampleId :
COSJ0DL

Tgt Ion: 95 Resp: 12173




Ion	Ratio	Lower	Upper
95	100		
97	63.5	45.2	84.0
132	96.1	60.6	112.6
130	100.1	62.9	116.7

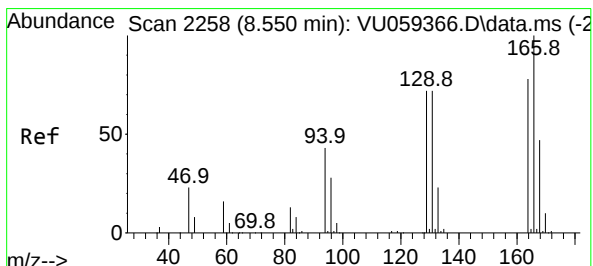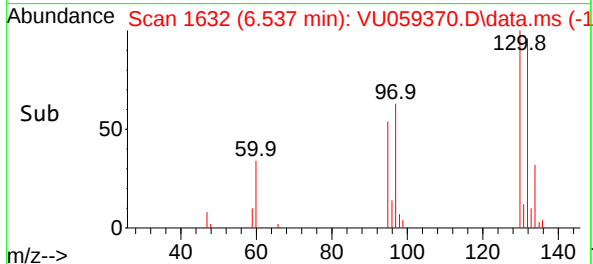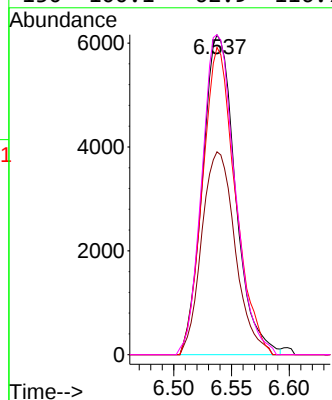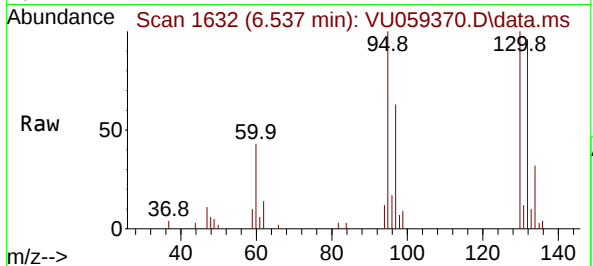


#46
Tetrachloroethene
Concen: 62.200 ug/L
RT: 8.547 min Scan# 2257
Delta R.T. -0.003 min
Lab File: VU059370.D
Acq: 20 Jun 2024 11:24

Tgt Ion: 164 Resp: 78113

Ion	Ratio	Lower	Upper
164	100		
129	90.4	74.5	138.5
131	90.8	70.6	131.0
166	123.8	95.1	176.7


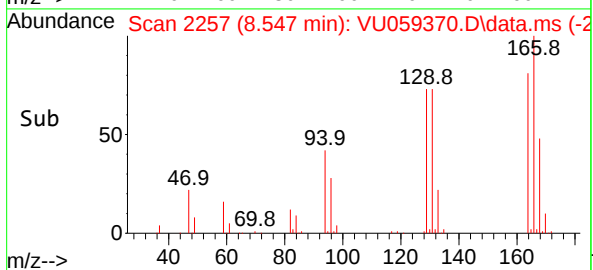
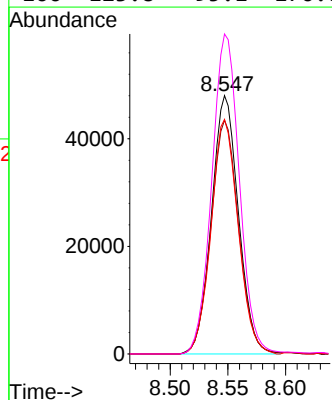
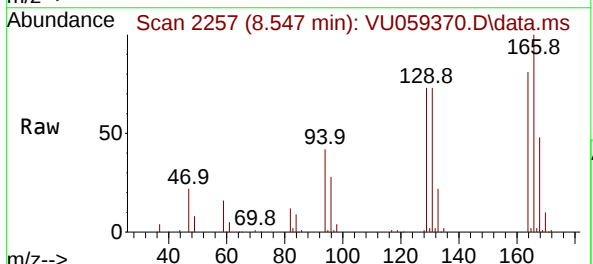


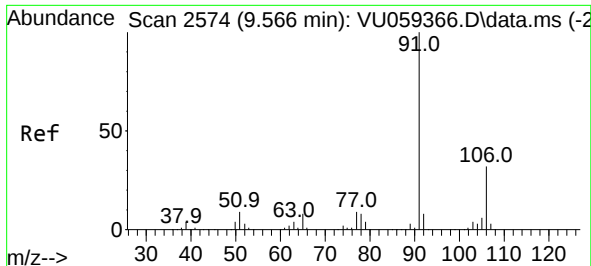

#52
Ethylbenzene
Concen: 1.937 ug/L
RT: 9.566 min Scan# 21
Delta R.T. -0.000 min
Lab File: VU059370.D
Acq: 20 Jun 2024 11:24

Instrument :
MSVOA_U
ClientSampleId :
COSJ0DL

Tgt Ion: 91 Resp: 15431
Ion Ratio Lower Upper
91 100
106 31.8 21.0 39.0

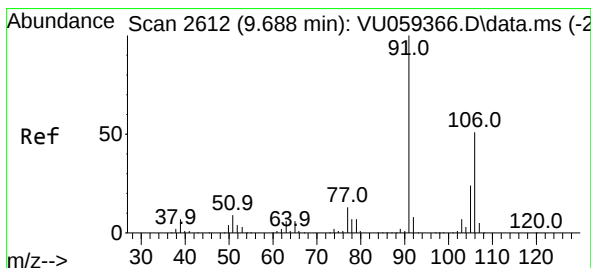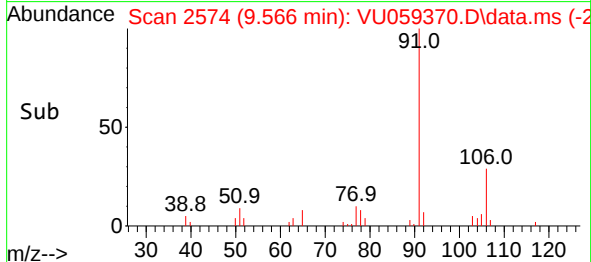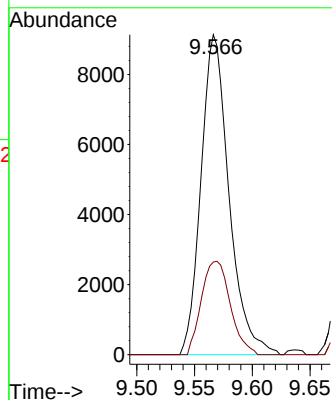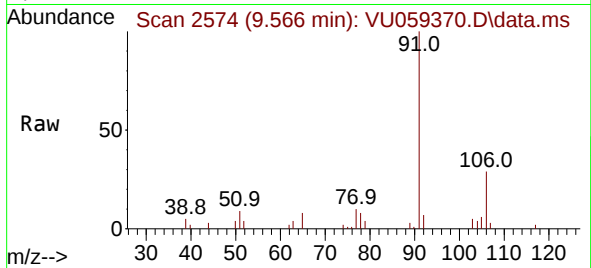

#53
m,p-Xylene
Concen: 2.585 ug/L
RT: 9.692 min Scan# 2613
Delta R.T. 0.003 min
Lab File: VU059370.D
Acq: 20 Jun 2024 11:24

Tgt Ion: 106 Resp: 7571
Ion Ratio Lower Upper
106 100
91 174.4 146.4 272.0

