

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062024\
 Data File : VU059367.D
 Acq On : 20 Jun 2024 10:15
 Operator : MD/SY
 Sample : VU0620MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK078

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M

Title : VOC Analysis

Signal : TIC: VU059367.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	88	95	115	rVB	75184	88617	13.56%	1.701%
2	1.907	184	192	210	rVB	67015	91006	13.92%	1.747%
3	2.560	383	395	409	rBV	120583	194672	29.78%	3.737%
4	2.791	457	467	478	rVB	1927	3146	0.48%	0.060%
5	2.946	512	515	516	rBV2	230	118	0.02%	0.002%
6	2.978	521	525	528	rBV2	269	226	0.03%	0.004%
7	3.036	536	543	551	rVB5	1949	3327	0.51%	0.064%
8	3.222	597	601	602	rBV2	250	192	0.03%	0.004%
9	3.348	633	640	641	rBV2	625	625	0.10%	0.012%
10	3.476	676	680	685	rBV	335	366	0.06%	0.007%
11	3.518	690	693	698	rBV2	205	210	0.03%	0.004%
12	3.570	705	709	711	rBV2	210	189	0.03%	0.004%
13	3.679	738	743	747	rBV2	292	340	0.05%	0.007%
14	3.701	747	750	754	rBV2	166	133	0.02%	0.003%
15	3.766	767	770	774	rVB	293	220	0.03%	0.004%
16	3.817	782	786	790	rBV2	254	255	0.04%	0.005%
17	4.071	858	865	866	rBV2	212	222	0.03%	0.004%
18	4.113	877	878	882	rBV	188	134	0.02%	0.003%
19	4.171	893	896	900	rVB	277	204	0.03%	0.004%
20	4.203	900	906	908	rBV2	247	314	0.05%	0.006%
21	4.271	923	927	931	rBV2	284	249	0.04%	0.005%
22	4.386	960	963	966	rBV2	150	145	0.02%	0.003%
23	4.415	968	972	975	rVB2	164	146	0.02%	0.003%
24	4.434	975	978	984	rBV2	286	328	0.05%	0.006%
25	4.573	1019	1021	1023	rVB	379	130	0.02%	0.002%
26	4.611	1023	1033	1068	rBV	64116	167475	25.62%	3.215%
27	5.055	1155	1171	1193	rBV	119526	268679	41.10%	5.158%
28	5.174	1205	1208	1209	rBV3	235	134	0.02%	0.003%
29	5.209	1215	1219	1223	rVB3	539	476	0.07%	0.009%
30	5.248	1228	1231	1233	rBV	206	173	0.03%	0.003%
31	5.309	1247	1250	1252	rBV	266	193	0.03%	0.004%
32	5.389	1272	1275	1276	rBV	318	205	0.03%	0.004%
33	5.441	1286	1291	1295	rVB	233	288	0.04%	0.006%
34	5.463	1295	1298	1302	rBV	220	191	0.03%	0.004%
35	5.560	1324	1328	1333	rVV2	171	228	0.03%	0.004%
36	5.608	1339	1343	1348	rVB	203	174	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062024\
 Data File : VU059367.D
 Acq On : 20 Jun 2024 10:15
 Operator : MD/SY
 Sample : VU0620MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK078

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

37	5.717	1357	1377	1414	rBV2	238471	653678	100.00%	12.550%
38	5.920	1436	1440	1441	rBV2	339	262	0.04%	0.005%
39	5.981	1457	1459	1461	rVB	284	141	0.02%	0.003%
40	6.071	1481	1487	1491	rBV2	252	327	0.05%	0.006%
41	6.094	1491	1494	1498	rVB2	281	208	0.03%	0.004%
42	6.116	1498	1501	1505	rBV2	278	216	0.03%	0.004%
43	6.242	1528	1540	1563	rBV	248283	479333	73.33%	9.203%
44	6.428	1595	1598	1601	rBV	355	284	0.04%	0.005%
45	6.528	1620	1629	1646	rVB8	5194	11103	1.70%	0.213%
46	6.618	1654	1657	1661	rBV2	253	256	0.04%	0.005%
47	6.682	1664	1677	1695	rBV	150712	294742	45.09%	5.659%
48	6.811	1714	1717	1721	rVB2	366	267	0.04%	0.005%
49	6.981	1762	1770	1771	rBV	251	255	0.04%	0.005%
50	7.039	1784	1788	1791	rBV2	194	173	0.03%	0.003%
51	7.058	1792	1794	1797	rVB	284	138	0.02%	0.003%
52	7.103	1804	1808	1811	rBV	386	338	0.05%	0.006%
53	7.148	1819	1822	1825	rBV	178	180	0.03%	0.003%
54	7.196	1830	1837	1843	rBV4	1437	2107	0.32%	0.040%
55	7.241	1849	1851	1856	rVB3	371	300	0.05%	0.006%
56	7.560	1934	1950	1974	rBV	69934	127710	19.54%	2.452%
57	7.891	2041	2053	2073	rBV	263617	468706	71.70%	8.999%
58	8.174	2130	2141	2167	rVV	48366	84500	12.93%	1.622%
59	8.293	2177	2178	2182	rBV2	232	148	0.02%	0.003%
60	8.399	2209	2211	2215	rVB3	550	317	0.05%	0.006%
61	8.444	2222	2225	2227	rBV2	229	140	0.02%	0.003%
62	8.479	2232	2236	2240	rVB	321	301	0.05%	0.006%
63	8.505	2240	2244	2246	rBV2	295	208	0.03%	0.004%
64	8.547	2254	2257	2264	rVB3	1239	1330	0.20%	0.026%
65	8.627	2271	2282	2323	rBV2	157955	332929	50.93%	6.392%
66	8.926	2369	2375	2379	rBV4	445	485	0.07%	0.009%
67	8.968	2385	2388	2391	rBV2	345	255	0.04%	0.005%
68	8.997	2395	2397	2401	rVB	239	141	0.02%	0.003%
69	9.029	2403	2407	2410	rBV2	187	202	0.03%	0.004%
70	9.155	2443	2446	2447	rBV	195	132	0.02%	0.003%
71	9.225	2465	2468	2469	rBV	178	115	0.02%	0.002%
72	9.257	2476	2478	2480	rBV	213	116	0.02%	0.002%
73	9.309	2489	2494	2497	rBV2	224	274	0.04%	0.005%
74	9.412	2513	2526	2549	rBV	355362	607457	92.93%	11.662%
75	9.698	2611	2615	2628	rVB3	1158	1461	0.22%	0.028%
76	10.061	2726	2728	2734	rBV	165	142	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062024\
 Data File : VU059367.D
 Acq On : 20 Jun 2024 10:15
 Operator : MD/SY
 Sample : VU0620MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK078

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

77	10.106	2734	2742	2746	rBV3	852	1246	0.19%	0.024%
78	10.212	2772	2775	2778	rBV2	207	166	0.03%	0.003%
79	10.524	2869	2872	2873	rBV	210	121	0.02%	0.002%
80	10.640	2904	2908	2911	rBV2	315	276	0.04%	0.005%
81	10.704	2924	2928	2930	rBV	258	236	0.04%	0.005%
82	10.749	2930	2942	2958	rBV	229351	371387	56.81%	7.130%
83	10.962	3005	3008	3011	rBV	252	220	0.03%	0.004%
84	11.061	3032	3039	3041	rBV	233	333	0.05%	0.006%
85	11.531	3183	3185	3188	rVB2	220	118	0.02%	0.002%
86	11.688	3231	3234	3238	rBV2	347	317	0.05%	0.006%
87	11.743	3245	3251	3258	rVB4	1486	2047	0.31%	0.039%
88	11.807	3259	3271	3292	rBV	298342	494688	75.68%	9.497%
89	12.100	3356	3362	3366	rBV2	294	384	0.06%	0.007%
90	12.132	3370	3372	3375	rBV2	242	126	0.02%	0.002%
91	12.187	3377	3389	3414	rBV	247167	412149	63.05%	7.913%
92	12.392	3450	3453	3455	rBV2	371	214	0.03%	0.004%
93	12.627	3523	3526	3529	rBV2	318	219	0.03%	0.004%
94	12.839	3589	3592	3595	rBV	256	180	0.03%	0.003%
95	13.228	3708	3713	3714	rBV3	1025	875	0.13%	0.017%
96	13.293	3730	3733	3737	rBV	245	180	0.03%	0.003%
97	13.842	3898	3904	3919	rVB4	3364	5140	0.79%	0.099%
98	14.093	3974	3982	3999	rBV2	8752	16808	2.57%	0.323%
99	14.331	4049	4056	4066	rVB3	4219	5780	0.88%	0.111%
100	14.370	4066	4068	4074	rBV3	436	376	0.06%	0.007%




Sum of corrected areas: 5208693

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062024\
Data File : VU059367.D
Acq On : 20 Jun 2024 10:15
Operator : MD/SY
Sample : VU0620MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK078

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

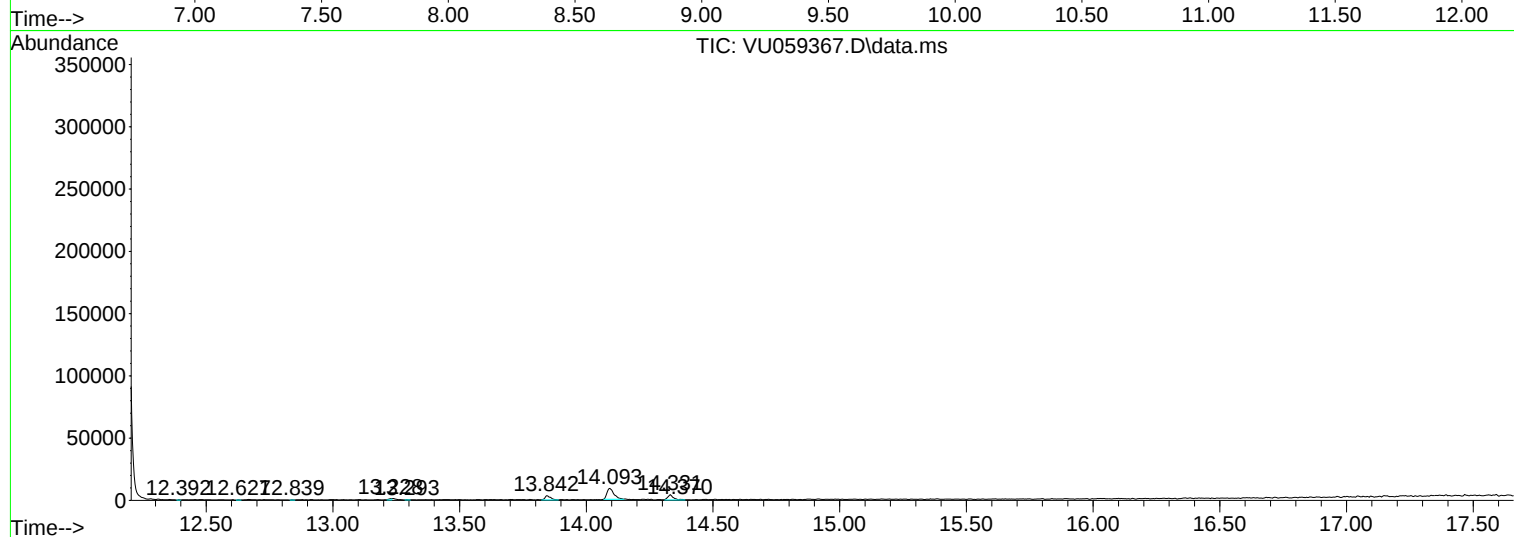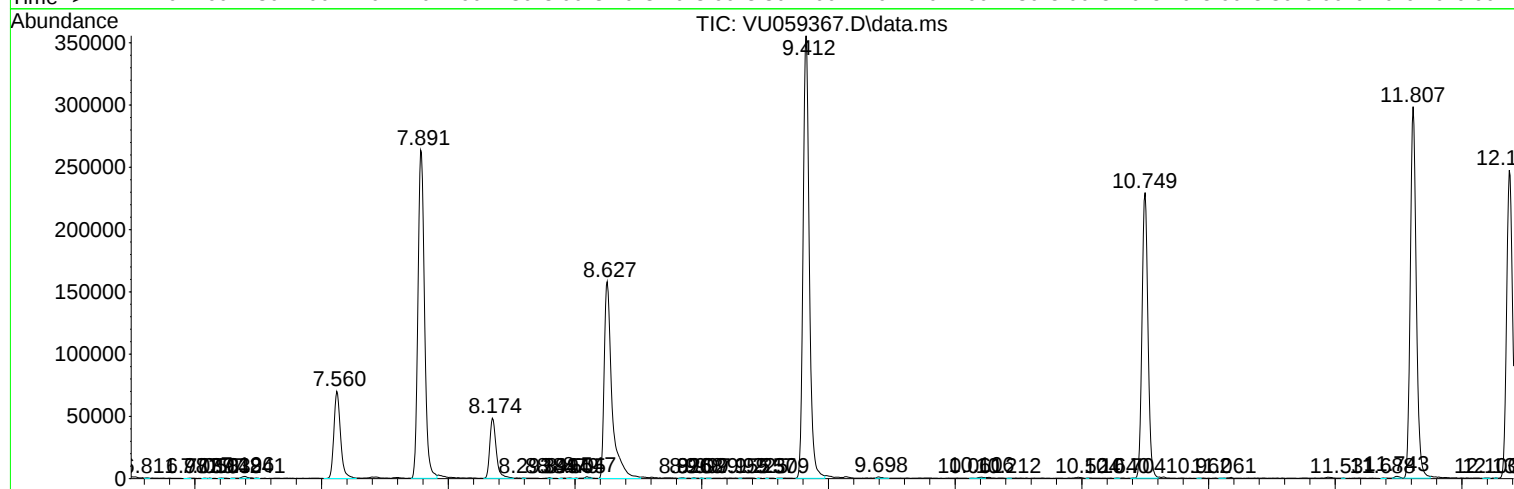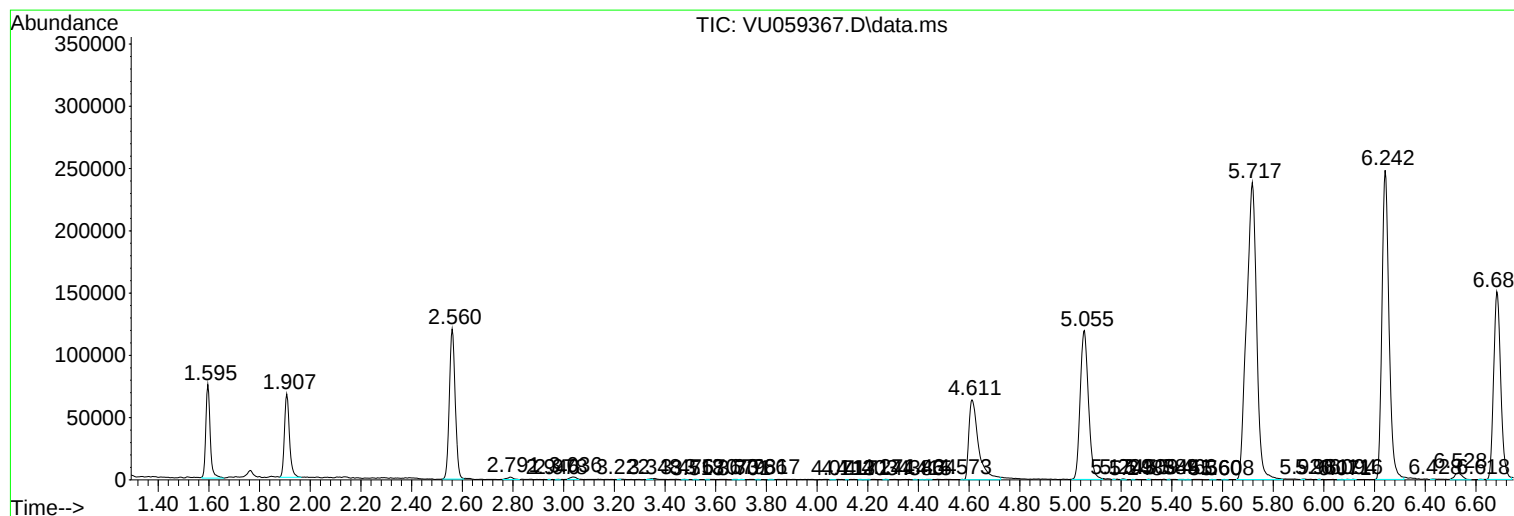

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062024\
Data File : VU059367.D
Acq On : 20 Jun 2024 10:15
Operator : MD/SY
Sample : VU0620MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK078

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062024\
Data File : VU059367.D
Acq On : 20 Jun 2024 10:15
Operator : MD/SY
Sample : VU0620MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK078

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc