


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062024\
Data File : VU059365.D
Acq On : 20 Jun 2024 08:16
Operator : MD/SY
Sample : BFB065
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB065

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Title : VOC Analysis
Last Update : Sat Jun 22 00:01:31 2024

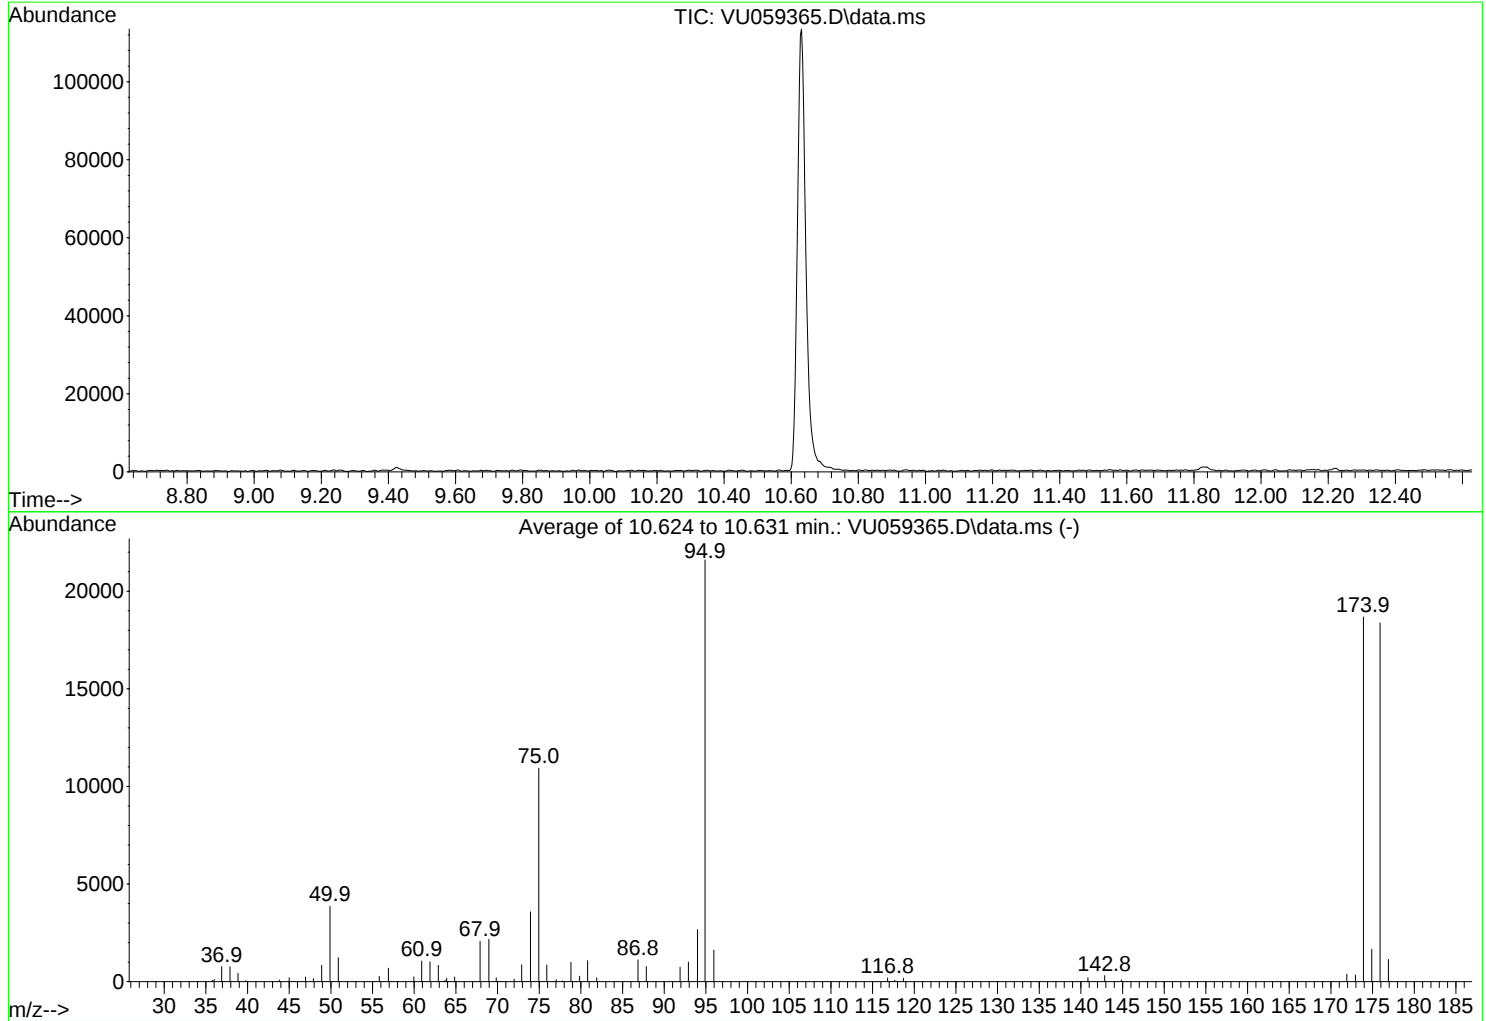

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2893

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	3860	PASS
75	95	30	80	50.6	10935	PASS
95	95	100	100	100.0	21608	PASS
96	95	5	9	7.5	1618	PASS
173	174	0.00	2	1.8	338	PASS
174	95	50	120	86.4	18677	PASS
175	174	5	9	8.9	1656	PASS
176	174	95	101	98.4	18378	PASS
177	176	5	9	6.2	1139	PASS

m/z	Abundance
39.80	102.0
43.80	265.0

Instrument :
MSVOA_U
ClientSampleId :
BFB065

m/z	Abundance
35.80	203.0
36.90	728.0
37.90	688.0
38.80	400.0
39.80	138.0
43.80	316.0
45.00	225.0
46.90	185.0
47.90	140.0
48.90	755.0
49.90	3731.0
50.90	1075.0
55.80	292.0
56.90	582.0
59.90	182.0
60.90	1026.0
61.90	1008.0
62.90	838.0
63.70	188.0
64.90	184.0
67.90	1831.0
69.00	2127.0
69.80	157.0
72.00	108.0
72.90	810.0
74.00	3402.0
75.00	10206.0
75.90	748.0
77.80	102.0
78.80	874.0
79.80	192.0
80.80	1029.0
82.00	170.0
86.80	1171.0
87.90	728.0
91.90	640.0
92.90	916.0
94.00	2406.0
94.90	20216.0
95.90	1471.0
116.80	146.0
117.60	114.0
118.70	162.0
140.80	158.0
142.80	224.0
171.90	361.0
173.00	321.0
173.90	16976.0
174.90	1640.0
175.90	16357.0
176.90	1008.0

Instrument :
MSVOA_U
ClientSampleId :
BFB065

m/z	Abundance
36.00	191.0
36.90	788.0
37.90	773.0
38.90	453.0
39.80	163.0
43.80	352.0
45.00	198.0
47.00	254.0
47.90	170.0
48.90	833.0
49.90	4003.0
50.90	1251.0
55.80	270.0
56.90	721.0
60.00	272.0
60.90	1100.0
61.90	1045.0
62.90	858.0
63.90	251.0
64.90	242.0
67.90	2134.0
68.90	2216.0
69.90	211.0
72.00	136.0
72.90	894.0
74.00	3648.0
75.00	11296.0
75.90	873.0
77.00	141.0
78.80	1020.0
79.90	290.0
80.80	1138.0
81.90	212.0
86.90	1120.0
87.90	785.0
91.90	765.0
92.90	1021.0
94.00	2799.0
94.90	22304.0
96.00	1685.0
116.80	199.0
117.70	110.0
118.70	187.0
140.90	198.0
142.80	314.0
144.80	126.0
171.90	389.0
172.90	358.0
173.90	19296.0
174.90	1734.0
175.90	18936.0
176.90	1177.0

Instrument :
MSVOA_U
ClientSampleId :
BFB065

m/z	Abundance
36.00	155.0
36.90	791.0
37.90	819.0
38.90	428.0
39.80	170.0
43.90	389.0
45.00	163.0
46.90	275.0
47.90	166.0
48.90	918.0
49.90	3847.0
50.90	1339.0
55.80	246.0
56.90	774.0
60.00	288.0
60.90	1046.0
61.90	987.0
62.90	823.0
63.90	271.0
64.80	297.0
67.90	2238.0
68.90	2168.0
69.90	217.0
72.00	150.0
72.90	886.0
73.90	3669.0
74.90	11302.0
75.90	945.0
77.10	154.0
78.80	1080.0
79.90	343.0
80.80	1056.0
81.80	221.0
86.90	1047.0
87.80	791.0
91.90	801.0
92.90	1075.0
94.00	2777.0
94.90	22304.0
96.00	1697.0
116.80	210.0
118.70	170.0
140.80	261.0
142.90	402.0
144.90	157.0
171.90	409.0
172.90	336.0
173.90	19760.0
174.90	1593.0
175.90	19840.0
176.90	1231.0

Instrument :
MSVOA_U
ClientSampleId :
BFB065