

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062124\
 Data File : VU059403.D
 Acq On : 21 Jun 2024 11:17
 Operator : MD/SY
 Sample : P2964-24
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Jun 22 00:03:34 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 22 00:01:31 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	209774	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	212719	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	94255	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	63276	50.379	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 100.760%			
7) Chloroethane-d5	1.907	69	53842	50.043	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 100.080%			
11) 1,1-Dichloroethene-d2	2.560	63	77166	31.125	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 62.260%			
21) 2-Butanone-d5	4.615	46	95311	80.508	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 80.510%			
24) Chloroform-d	5.055	84	115851	46.334	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 92.660%			
26) 1,2-Dichloroethane-d4	5.695	65	75185	49.060	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 98.120%			
32) Benzene-d6	5.721	84	234684	48.069	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 96.140%			
36) 1,2-Dichloropropane-d6	6.682	67	75638	44.932	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 89.860%			
41) Toluene-d8	7.894	98	204848	49.426	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 98.860%			
43) trans-1,3-Dichloroprop...	8.174	79	31658	46.525	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 93.060%			
47) 2-Hexanone-d5	8.627	63	55678	71.525	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 71.520%			
56) 1,1,2,2-Tetrachloroeth...	10.749	84	116944	41.047	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 82.100%			
66) 1,2-Dichlorobenzene-d4	12.190	152	78888	56.084	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 112.160%			
Target Compounds					Qvalue	
37) 1,2-Dichloropropane	6.682	63	8144	3.734	ug/L #	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062124\
Data File : VU059403.D
Acq On : 21 Jun 2024 11:17
Operator : MD/SY
Sample : P2964-24
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Jun 22 00:03:34 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jun 22 00:01:31 2024
Response via : Initial Calibration

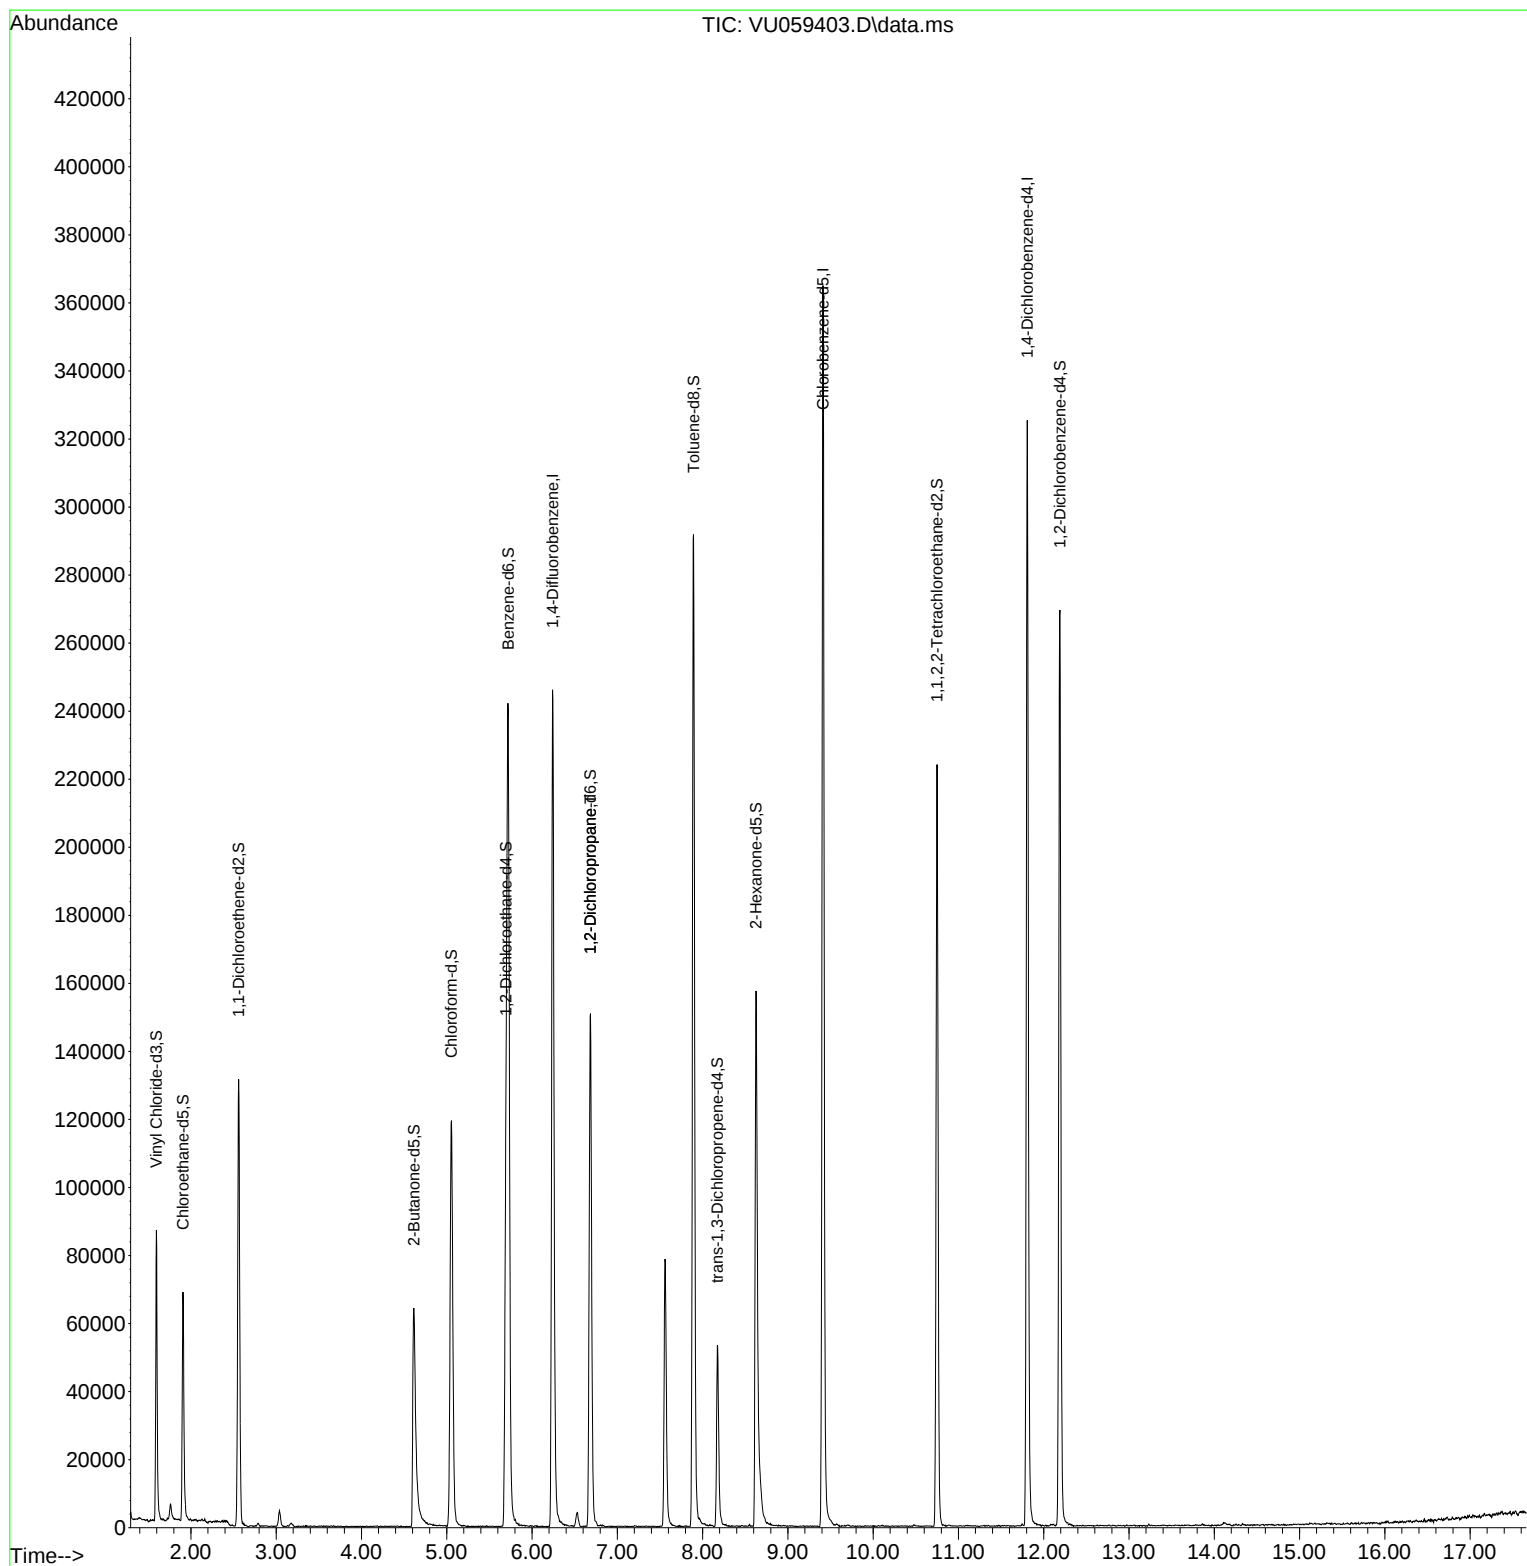

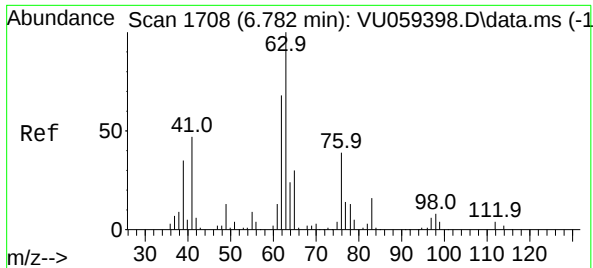

#37
1,2-Dichloropropane
Concen: 3.734 ug/L
RT: 6.682 min Scan# 1
Delta R.T. -0.100 min
Lab File: VU059403.D
Acq: 21 Jun 2024 11:17

Instrument :
MSVOA_U
ClientSampleId :

Tgt Ion: 63 Resp: 8144
Ion Ratio Lower Upper
63 100
112 0.0 2.6 4.0#

