

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062124\
 Data File : VU059400.D
 Acq On : 21 Jun 2024 10:02
 Operator : MD/SY
 Sample : VU0621WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK082

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

Signal : TIC: VU059400.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.592	86	94	115	rBV	93169	108972	16.12%	2.015%
2	1.756	139	145	152	rBV2	4138	5257	0.78%	0.097%
3	1.904	182	191	208	rBV	69909	95455	14.12%	1.765%
4	2.557	382	394	413	rBV	138608	228222	33.75%	4.219%
5	2.673	428	430	439	rVB3	334	341	0.05%	0.006%
6	2.711	439	442	447	rBV2	207	202	0.03%	0.004%
7	2.785	458	465	473	rVB	1036	1498	0.22%	0.028%
8	2.840	478	482	484	rBV2	254	196	0.03%	0.004%
9	3.036	534	543	555	rVB4	3272	5506	0.81%	0.102%
10	3.174	580	586	590	rVV2	431	435	0.06%	0.008%
11	3.351	638	641	645	rVV2	633	519	0.08%	0.010%
12	3.644	727	732	735	rVB	250	246	0.04%	0.005%
13	3.679	740	743	747	rBV	185	204	0.03%	0.004%
14	3.837	789	792	799	rVB2	160	172	0.03%	0.003%
15	3.994	838	841	843	rBV	209	171	0.03%	0.003%
16	4.268	921	926	933	rBV	260	296	0.04%	0.005%
17	4.303	933	937	945	rVB2	268	266	0.04%	0.005%
18	4.518	999	1004	1007	rBV2	208	242	0.04%	0.004%
19	4.612	1023	1033	1071	rBV	60314	154131	22.80%	2.850%
20	4.843	1101	1105	1111	rBV3	382	450	0.07%	0.008%
21	5.052	1152	1170	1192	rBV	119886	268531	39.71%	4.965%
22	5.229	1221	1225	1228	rBV3	318	258	0.04%	0.005%
23	5.718	1357	1377	1409	rBV2	252285	676158	100.00%	12.501%
24	6.001	1461	1465	1468	rBV2	223	177	0.03%	0.003%
25	6.026	1468	1473	1475	rBV2	358	303	0.04%	0.006%
26	6.242	1527	1540	1561	rBV	251704	488969	72.32%	9.040%
27	6.528	1620	1629	1639	rVB8	4173	7914	1.17%	0.146%
28	6.682	1665	1677	1695	rBV2	152972	298406	44.13%	5.517%
29	6.811	1712	1717	1719	rVB2	240	221	0.03%	0.004%
30	6.830	1719	1723	1726	rBV2	224	224	0.03%	0.004%
31	7.120	1809	1813	1822	rVV2	237	347	0.05%	0.006%
32	7.203	1835	1839	1842	rVV2	219	231	0.03%	0.004%
33	7.248	1848	1853	1856	rBV2	185	212	0.03%	0.004%
34	7.357	1883	1887	1890	rBV2	192	192	0.03%	0.004%
35	7.403	1896	1901	1906	rBV2	151	199	0.03%	0.004%
36	7.560	1938	1950	1972	rBV2	77636	140686	20.81%	2.601%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062124\
 Data File : VU059400.D
 Acq On : 21 Jun 2024 10:02
 Operator : MD/SY
 Sample : VU0621WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK082

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

37	7.702	1990	1994	1998	rBV4	454	350	0.05%	0.006%
38	7.795	2021	2023	2029	rVB3	265	260	0.04%	0.005%
39	7.891	2041	2053	2080	rBV	295882	526847	77.92%	9.741%
40	8.004	2086	2088	2094	rVB2	644	519	0.08%	0.010%
41	8.091	2112	2115	2118	rBV2	472	370	0.05%	0.007%
42	8.139	2126	2130	2131	rBV2	389	228	0.03%	0.004%
43	8.174	2131	2141	2165	rVV	52203	91604	13.55%	1.694%
44	8.271	2168	2171	2179	rVV2	323	373	0.06%	0.007%
45	8.345	2185	2194	2197	rBV2	328	429	0.06%	0.008%
46	8.361	2197	2199	2203	rBV	227	228	0.03%	0.004%
47	8.547	2254	2257	2261	rBV3	489	355	0.05%	0.007%
48	8.583	2265	2268	2271	rVB	270	197	0.03%	0.004%
49	8.628	2271	2282	2322	rBV	147892	309427	45.76%	5.721%
50	9.017	2395	2403	2406	rBV2	242	292	0.04%	0.005%
51	9.271	2477	2482	2485	rBV2	190	201	0.03%	0.004%
52	9.351	2502	2507	2510	rBV	237	289	0.04%	0.005%
53	9.412	2513	2526	2560	rBV	363172	626948	92.72%	11.591%
54	9.570	2572	2575	2578	rBV2	392	277	0.04%	0.005%
55	9.663	2601	2604	2606	rBV2	278	184	0.03%	0.003%
56	9.705	2615	2617	2621	rVB	282	243	0.04%	0.004%
57	9.779	2632	2640	2641	rBV	166	204	0.03%	0.004%
58	9.907	2676	2680	2686	rVB	236	217	0.03%	0.004%
59	10.103	2734	2741	2743	rBV2	467	571	0.08%	0.011%
60	10.136	2748	2751	2755	rVV3	327	272	0.04%	0.005%
61	10.277	2793	2795	2803	rVV2	272	252	0.04%	0.005%
62	10.338	2812	2814	2818	rVB2	276	202	0.03%	0.004%
63	10.357	2818	2820	2824	rBV2	199	185	0.03%	0.003%
64	10.483	2853	2859	2861	rVV2	303	287	0.04%	0.005%
65	10.631	2900	2905	2908	rBV2	257	260	0.04%	0.005%
66	10.705	2924	2928	2930	rBV	262	197	0.03%	0.004%
67	10.750	2930	2942	2961	rVV	220423	355945	52.64%	6.581%
68	11.007	3019	3022	3024	rBV	233	173	0.03%	0.003%
69	11.074	3037	3043	3047	rBV2	344	461	0.07%	0.009%
70	11.155	3064	3068	3070	rBV2	318	200	0.03%	0.004%
71	11.444	3155	3158	3162	rBV2	222	201	0.03%	0.004%
72	11.473	3162	3167	3170	rBV3	368	370	0.05%	0.007%
73	11.746	3248	3252	3256	rVB3	562	457	0.07%	0.008%
74	11.807	3259	3271	3290	rBV	328648	539540	79.79%	9.975%
75	11.959	3314	3318	3327	rBV4	510	726	0.11%	0.013%
76	12.116	3364	3367	3370	rVB2	267	180	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062124\
 Data File : VU059400.D
 Acq On : 21 Jun 2024 10:02
 Operator : MD/SY
 Sample : VU0621WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK082

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

77	12.187	3377	3389	3413	rBV	263718	452049	66.86%	8.358%
78	12.402	3451	3456	3461	rBV2	239	268	0.04%	0.005%
79	12.914	3611	3615	3618	rBV2	349	311	0.05%	0.006%
80	13.078	3663	3666	3670	rBV2	178	189	0.03%	0.003%
81	13.258	3720	3722	3728	rBV2	283	207	0.03%	0.004%
82	13.653	3842	3845	3848	rBV	318	220	0.03%	0.004%
83	13.846	3901	3905	3908	rBV2	638	621	0.09%	0.011%
84	14.016	3952	3958	3962	rBV2	270	372	0.06%	0.007%
85	14.081	3975	3978	3979	rBV	346	201	0.03%	0.004%
86	14.113	3980	3988	3994	rVV5	1784	2893	0.43%	0.053%
87	14.232	4022	4025	4029	rBV2	215	203	0.03%	0.004%
88	14.312	4048	4050	4053	rBV	320	183	0.03%	0.003%
89	14.344	4053	4060	4069	rVV5	760	1420	0.21%	0.026%
90	14.467	4096	4098	4102	rBV	271	175	0.03%	0.003%
91	14.685	4163	4166	4170	rBV	350	247	0.04%	0.005%
92	14.727	4176	4179	4182	rBV2	292	248	0.04%	0.005%
93	14.788	4195	4198	4199	rBV	350	221	0.03%	0.004%
94	14.881	4225	4227	4233	rVB2	461	430	0.06%	0.008%
95	15.460	4402	4407	4409	rBV2	604	528	0.08%	0.010%
96	15.621	4455	4457	4461	rVB3	462	269	0.04%	0.005%
97	15.749	4495	4497	4499	rBV2	413	225	0.03%	0.004%
98	16.212	4639	4641	4642	rBV2	461	221	0.03%	0.004%
99	16.299	4666	4668	4670	rBV2	404	203	0.03%	0.004%
100	16.495	4726	4729	4731	rBV3	855	562	0.08%	0.010%




Sum of corrected areas: 5408796

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062124\
Data File : VU059400.D
Acq On : 21 Jun 2024 10:02
Operator : MD/SY
Sample : VU0621WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK082

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

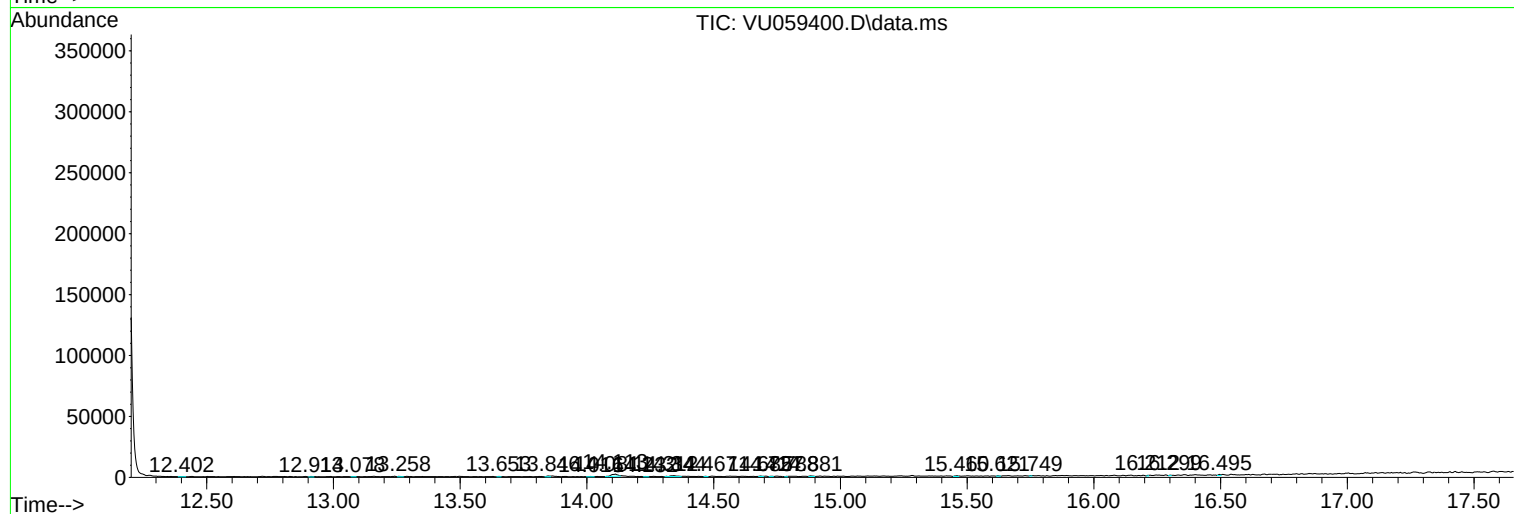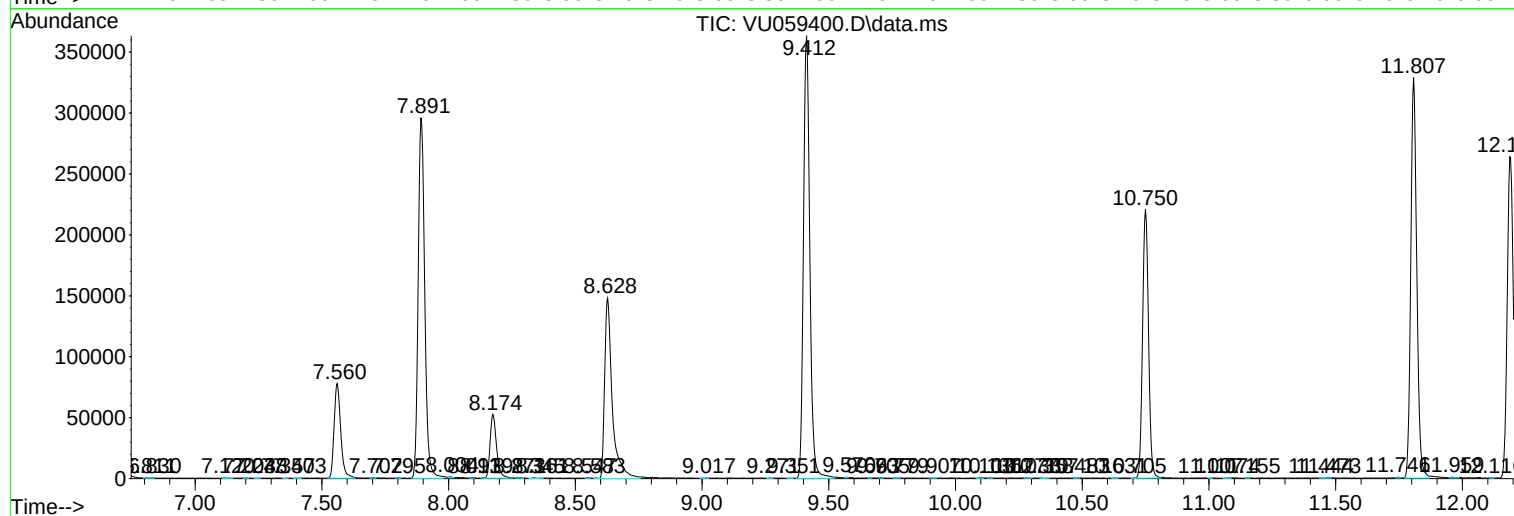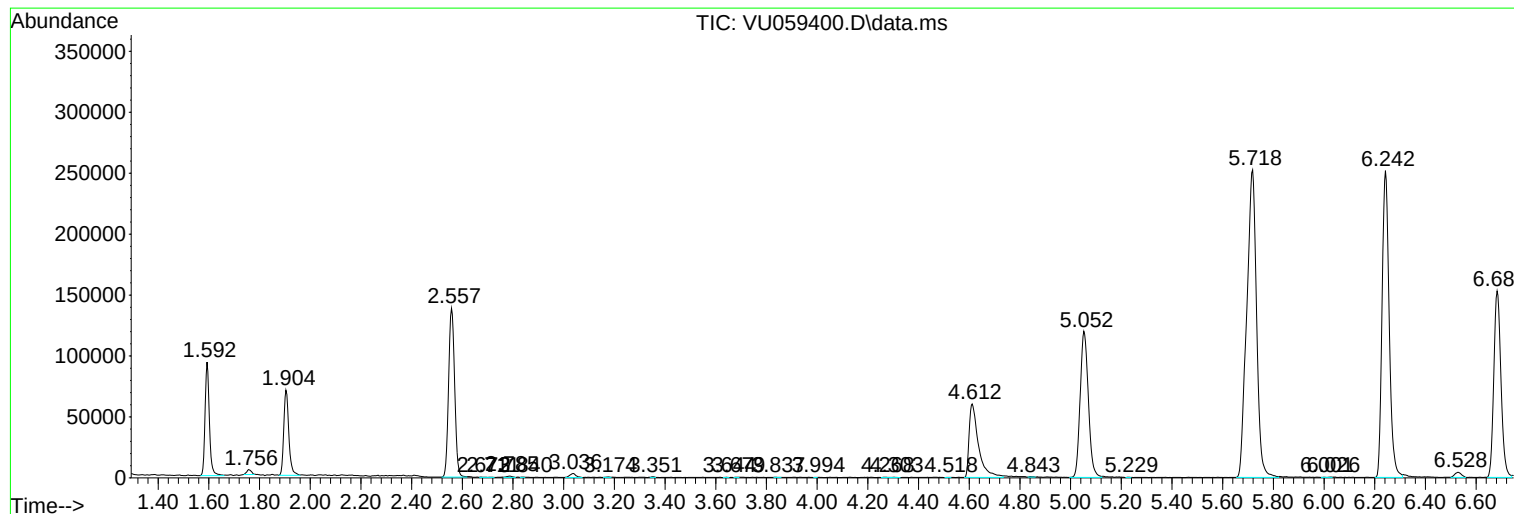

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062124\
Data File : VU059400.D
Acq On : 21 Jun 2024 10:02
Operator : MD/SY
Sample : VU0621WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK082

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062124\
Data File : VU059400.D
Acq On : 21 Jun 2024 10:02
Operator : MD/SY
Sample : VU0621WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK082

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------