

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062124\
 Data File : VU059403.D
 Acq On : 21 Jun 2024 11:17
 Operator : MD/SY
 Sample : P2964-24
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

Signal : TIC: VU059403.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	112	rBV	85356	101825	15.28%	1.894%
2	1.907	184	192	214	rBV	67159	93804	14.07%	1.745%
3	2.560	382	395	409	rBV	131268	213054	31.97%	3.963%
4	2.702	432	439	441	rBV2	305	367	0.06%	0.007%
5	2.740	448	451	455	rBV2	218	226	0.03%	0.004%
6	2.759	455	457	459	rVV	282	163	0.02%	0.003%
7	2.788	459	466	473	rVB2	975	1439	0.22%	0.027%
8	2.824	473	477	479	rBV	234	185	0.03%	0.003%
9	3.039	532	544	557	rVV3	4621	8070	1.21%	0.150%
10	3.181	578	588	591	rBV3	884	1467	0.22%	0.027%
11	3.348	638	640	642	rBV	338	169	0.03%	0.003%
12	3.496	681	686	689	rBV2	145	162	0.02%	0.003%
13	3.673	737	741	744	rBV2	249	186	0.03%	0.003%
14	3.724	753	757	763	rBV2	192	202	0.03%	0.004%
15	4.062	859	862	867	rVB2	197	163	0.02%	0.003%
16	4.271	922	927	929	rBV	199	160	0.02%	0.003%
17	4.528	1004	1007	1010	rBV	172	161	0.02%	0.003%
18	4.615	1024	1034	1066	rBV	64138	162851	24.44%	3.029%
19	4.846	1104	1106	1109	rVB2	325	170	0.03%	0.003%
20	5.055	1156	1171	1198	rVV	119195	267149	40.08%	4.969%
21	5.255	1229	1233	1236	rBV	263	246	0.04%	0.005%
22	5.345	1256	1261	1264	rVV	179	187	0.03%	0.003%
23	5.470	1296	1300	1304	rVB	282	191	0.03%	0.004%
24	5.505	1305	1311	1315	rBV2	135	166	0.02%	0.003%
25	5.718	1357	1377	1401	rBV2	241894	666459	100.00%	12.396%
26	5.846	1415	1417	1421	rVB2	452	182	0.03%	0.003%
27	5.894	1429	1432	1435	rBV4	250	199	0.03%	0.004%
28	5.981	1455	1459	1462	rVB2	277	205	0.03%	0.004%
29	6.004	1462	1466	1471	rVB	271	276	0.04%	0.005%
30	6.033	1471	1475	1477	rBV2	232	187	0.03%	0.003%
31	6.065	1483	1485	1490	rVB2	294	189	0.03%	0.004%
32	6.190	1521	1524	1527	rBV	189	156	0.02%	0.003%
33	6.242	1527	1540	1565	rBV	245939	476847	71.55%	8.869%
34	6.473	1610	1612	1616	rVB	287	197	0.03%	0.004%
35	6.531	1618	1630	1643	rVB6	4154	8312	1.25%	0.155%
36	6.685	1665	1678	1696	rBV	150638	297802	44.68%	5.539%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062124\
 Data File : VU059403.D
 Acq On : 21 Jun 2024 11:17
 Operator : MD/SY
 Sample : P2964-24
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

37	6.933	1753	1755	1758	rBV2	276	221	0.03%	0.004%
38	7.000	1772	1776	1782	rBV2	178	227	0.03%	0.004%
39	7.203	1834	1839	1843	rBV3	280	292	0.04%	0.005%
40	7.341	1876	1882	1885	rBV2	155	182	0.03%	0.003%
41	7.560	1938	1950	1971	rBV2	78514	141952	21.30%	2.640%
42	7.727	1999	2002	2003	rVV2	351	176	0.03%	0.003%
43	7.894	2041	2054	2073	rBV	291493	512664	76.92%	9.535%
44	8.174	2131	2141	2160	rBV2	53227	93774	14.07%	1.744%
45	8.457	2225	2229	2230	rBV2	316	198	0.03%	0.004%
46	8.550	2257	2258	2263	rVB2	560	320	0.05%	0.006%
47	8.627	2272	2282	2320	rBV2	157358	326172	48.94%	6.067%
48	8.798	2333	2335	2337	rVB2	445	168	0.03%	0.003%
49	9.412	2512	2526	2566	rBV	364840	621304	93.22%	11.556%
50	9.705	2611	2617	2619	rBV2	348	361	0.05%	0.007%
51	9.762	2632	2635	2641	rVB2	225	191	0.03%	0.004%
52	9.907	2676	2680	2683	rVV2	195	155	0.02%	0.003%
53	10.029	2715	2718	2723	rBV2	152	159	0.02%	0.003%
54	10.065	2723	2729	2733	rBV2	273	303	0.05%	0.006%
55	10.479	2852	2858	2861	rBV3	488	488	0.07%	0.009%
56	10.749	2930	2942	2962	rVV	223866	368382	55.27%	6.852%
57	11.084	3042	3046	3051	rBV3	233	268	0.04%	0.005%
58	11.261	3096	3101	3102	rBV	257	202	0.03%	0.004%
59	11.325	3117	3121	3126	rBV2	283	286	0.04%	0.005%
60	11.354	3126	3130	3134	rVB2	274	238	0.04%	0.004%
61	11.470	3163	3166	3167	rBV	257	159	0.02%	0.003%
62	11.515	3177	3180	3184	rVV2	199	179	0.03%	0.003%
63	11.643	3217	3220	3225	rVB	259	226	0.03%	0.004%
64	11.669	3225	3228	3230	rBV2	192	151	0.02%	0.003%
65	11.746	3250	3252	3259	rVB4	562	441	0.07%	0.008%
66	11.807	3259	3271	3293	rBV	324922	534986	80.27%	9.950%
67	11.981	3322	3325	3326	rBV	307	196	0.03%	0.004%
68	12.026	3336	3339	3342	rVB2	406	253	0.04%	0.005%
69	12.048	3342	3346	3349	rBV2	199	167	0.03%	0.003%
70	12.084	3353	3357	3358	rBV2	402	244	0.04%	0.005%
71	12.145	3373	3376	3377	rBV2	277	164	0.02%	0.003%
72	12.190	3377	3390	3415	rVV	269039	458789	68.84%	8.533%
73	12.341	3435	3437	3440	rVB	370	180	0.03%	0.003%
74	12.360	3440	3443	3445	rBV	205	170	0.03%	0.003%
75	12.457	3470	3473	3478	rBV	257	245	0.04%	0.005%
76	12.811	3580	3583	3587	rBV	246	236	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062124\
 Data File : VU059403.D
 Acq On : 21 Jun 2024 11:17
 Operator : MD/SY
 Sample : P2964-24
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

77	12.974	3627	3634	3637	rBV2	439	499	0.07%	0.009%
78	13.113	3674	3677	3680	rVB2	235	165	0.02%	0.003%
79	13.132	3680	3683	3685	rBV2	269	209	0.03%	0.004%
80	13.164	3690	3693	3695	rBV	242	180	0.03%	0.003%
81	13.232	3709	3714	3720	rBV4	638	690	0.10%	0.013%
82	13.264	3721	3724	3728	rVB2	214	201	0.03%	0.004%
83	13.392	3760	3764	3767	rBV2	223	219	0.03%	0.004%
84	13.653	3842	3845	3849	rBV	201	171	0.03%	0.003%
85	13.862	3907	3910	3912	rVB2	407	250	0.04%	0.005%
86	13.974	3942	3945	3950	rBV2	465	423	0.06%	0.008%
87	14.010	3951	3956	3960	rVB2	283	250	0.04%	0.005%
88	14.109	3984	3987	3989	rBV	527	331	0.05%	0.006%
89	14.228	4022	4024	4027	rBV2	265	165	0.02%	0.003%
90	14.283	4039	4041	4044	rBV2	241	158	0.02%	0.003%
91	14.331	4052	4056	4060	rBV3	525	448	0.07%	0.008%
92	14.457	4093	4095	4098	rBV	235	157	0.02%	0.003%
93	14.605	4136	4141	4144	rBV3	355	427	0.06%	0.008%
94	14.679	4161	4164	4167	rVB2	331	191	0.03%	0.004%
95	14.791	4196	4199	4203	rBV3	304	226	0.03%	0.004%
96	14.814	4203	4206	4208	rVB	361	205	0.03%	0.004%
97	15.376	4378	4381	4384	rBV3	451	301	0.05%	0.006%
98	15.833	4520	4523	4525	rBV3	447	326	0.05%	0.006%
99	16.460	4716	4718	4719	rBV	645	273	0.04%	0.005%
100	16.582	4753	4756	4759	rBV4	831	766	0.11%	0.014%




Sum of corrected areas: 5376474

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062124\
Data File : VU059403.D
Acq On : 21 Jun 2024 11:17
Operator : MD/SY
Sample : P2964-24
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

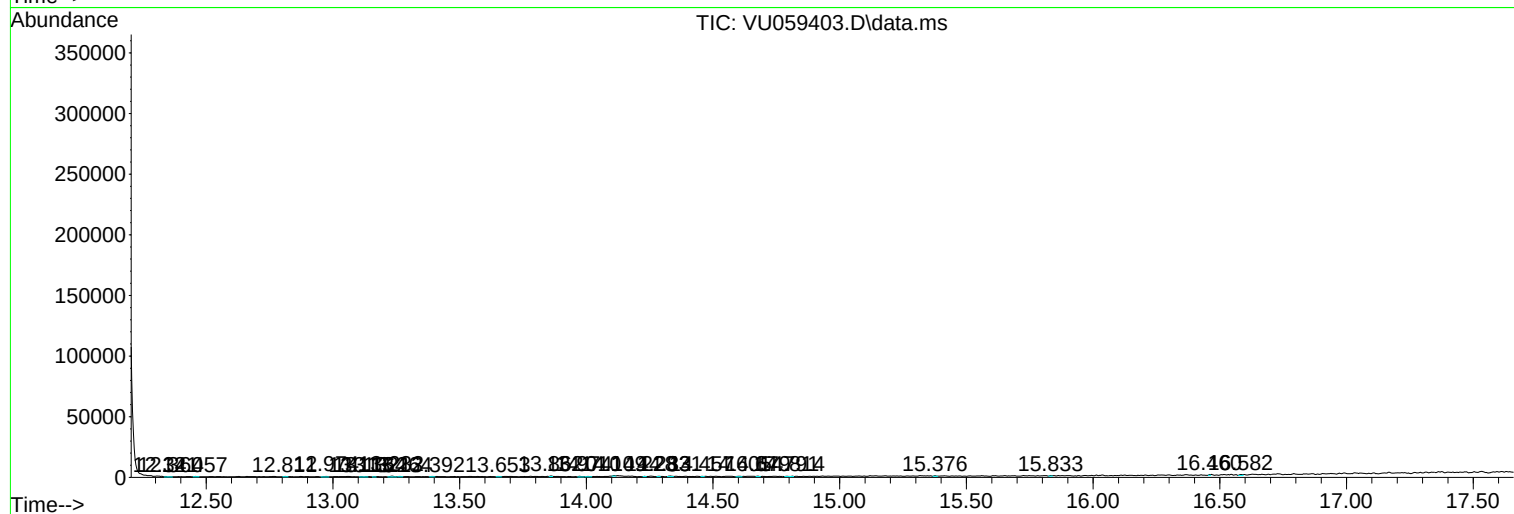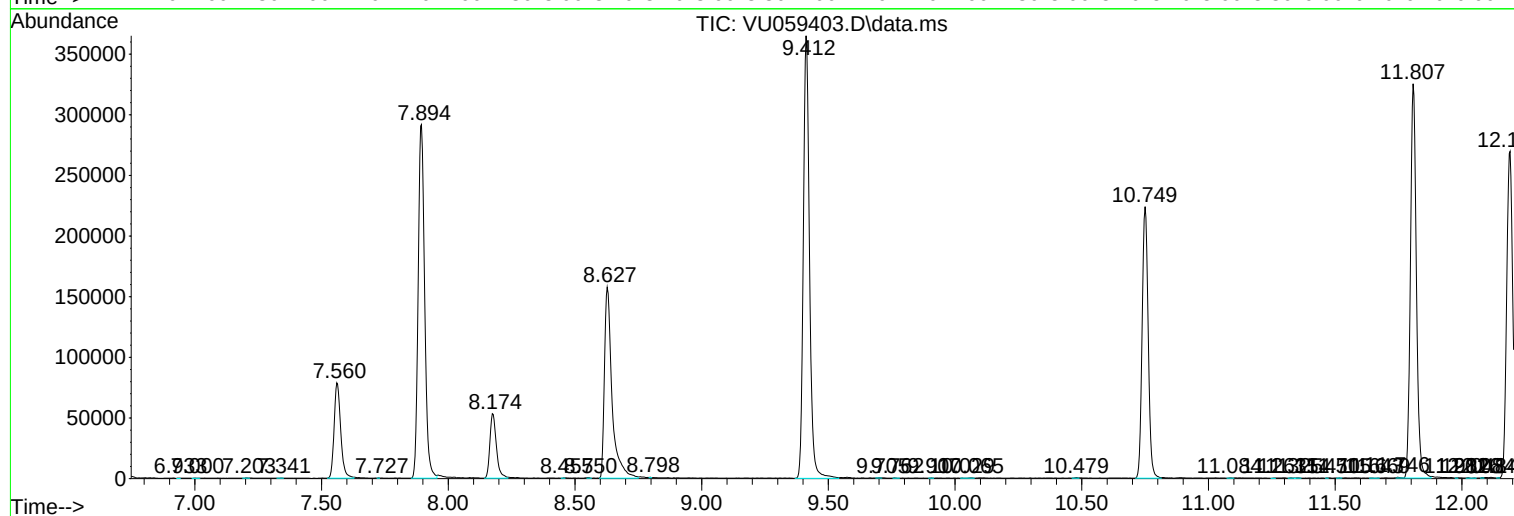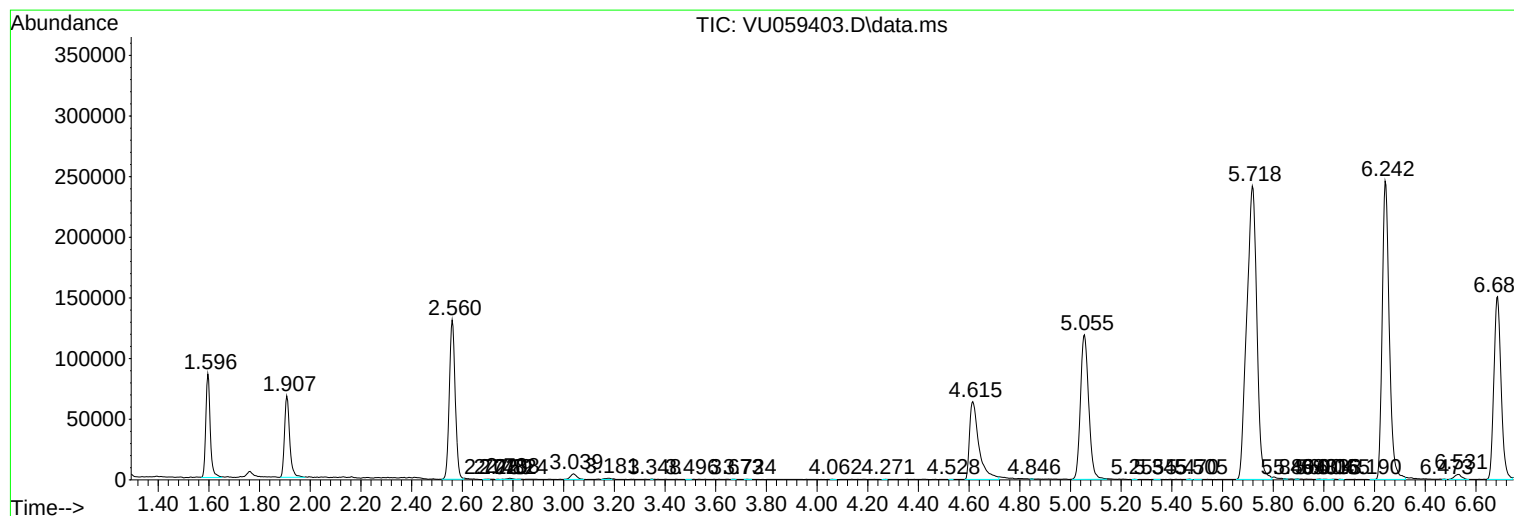

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062124\
Data File : VU059403.D
Acq On : 21 Jun 2024 11:17
Operator : MD/SY
Sample : P2964-24
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062124\
Data File : VU059403.D
Acq On : 21 Jun 2024 11:17
Operator : MD/SY
Sample : P2964-24
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------