


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062124\
Data File : VU059397.D
Acq On : 21 Jun 2024 08:03
Operator : MD/SY
Sample : BFB066
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB066

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Title : VOC Analysis
Last Update : Sat Jun 22 00:01:31 2024

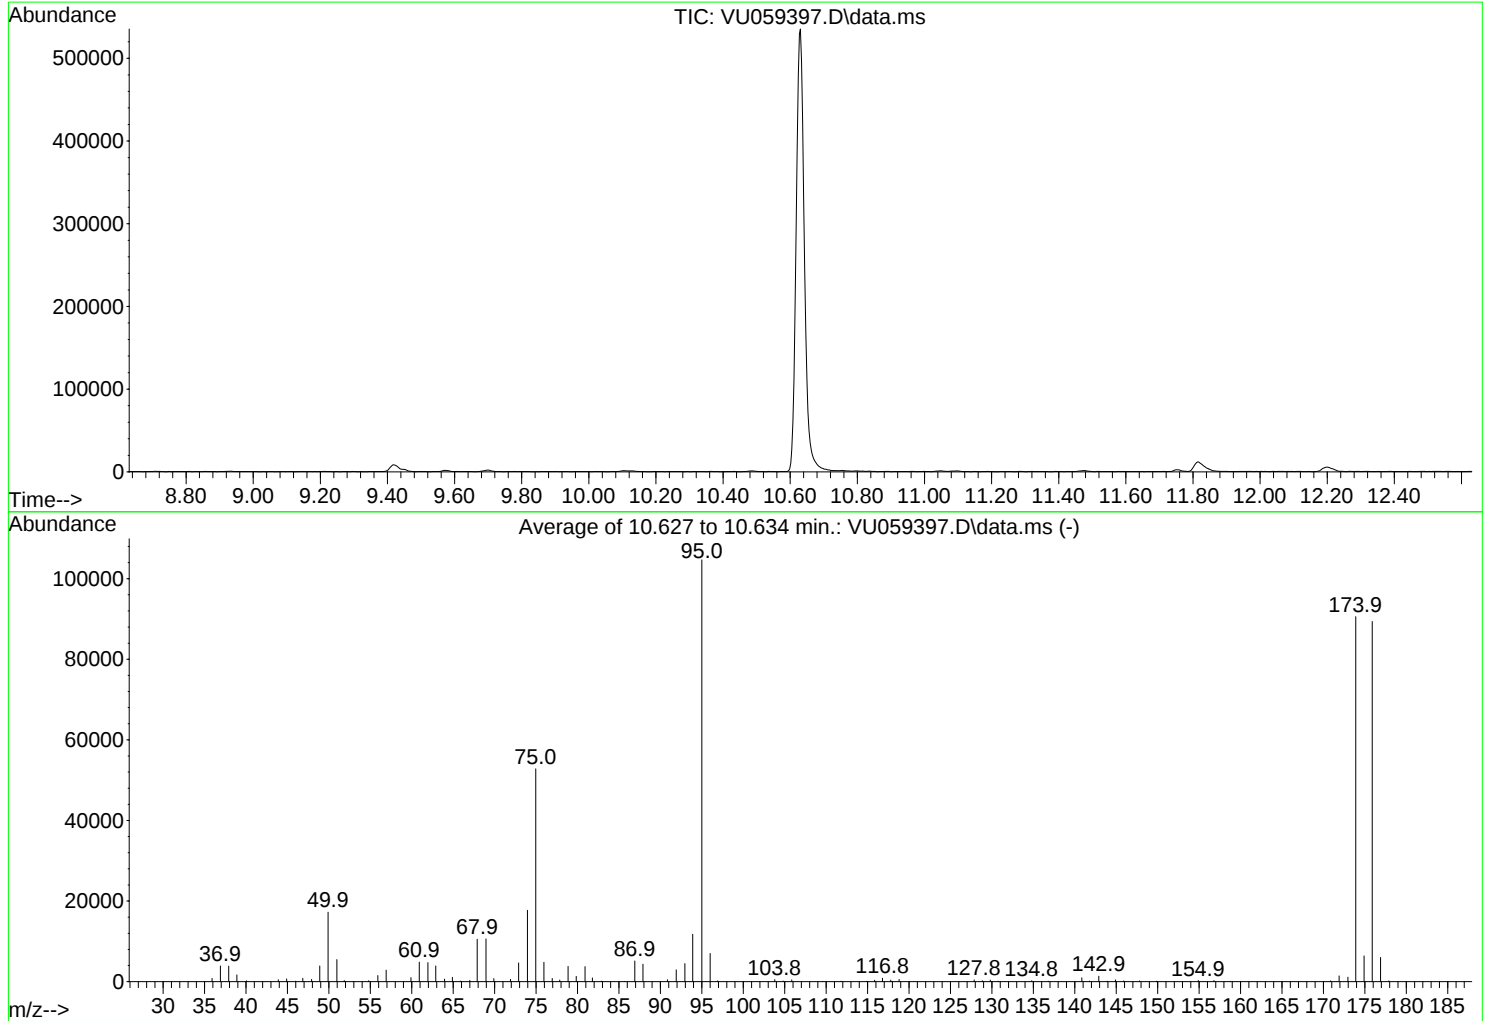

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2892

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.5	17233	PASS
75	95	30	80	50.5	52821	PASS
95	95	100	100	100.0	104675	PASS
96	95	5	9	6.7	6979	PASS
173	174	0.00	2	1.2	1124	PASS
174	95	50	120	86.5	90563	PASS
175	174	5	9	7.1	6405	PASS
176	174	95	101	98.7	89368	PASS
177	176	5	9	6.7	6011	PASS

m/z	Abundance
39.80	148.0
43.90	272.0

Instrument :
MSVOA_U
ClientSampleId :
BFB066

m/z	Abundance
35.90	751.0
36.90	4312.0
37.90	4001.0
38.90	1815.0
40.10	223.0
43.90	748.0
44.90	671.0
46.00	173.0
46.90	864.0
47.90	557.0
48.90	3985.0
49.90	18192.0
50.90	5669.0
51.90	313.0
52.90	106.0
54.80	253.0
55.90	1493.0
56.90	3089.0
59.90	956.0
60.90	4937.0
61.90	4801.0
62.90	4149.0
63.90	751.0
64.90	1075.0
65.90	120.0
67.00	334.0
67.90	10942.0
69.00	10853.0
69.90	819.0
71.90	564.0
72.90	4577.0
74.00	17680.0
74.90	54488.0
75.90	4861.0
76.90	761.0
77.90	426.0
78.90	4020.0
79.90	1370.0
80.90	3852.0
81.80	975.0
82.90	121.0
86.90	5528.0
87.90	4364.0
90.90	438.0
91.90	2846.0
93.00	4833.0
93.90	12193.0
95.00	106120.0
96.00	7258.0
96.90	229.0
103.80	514.0
104.80	157.0
105.80	464.0
111.70	118.0
115.90	395.0
116.80	829.0
117.80	432.0
118.80	613.0
127.90	416.0
128.90	195.0
129.80	457.0
130.80	136.0
134.80	242.0
136.80	120.0
140.80	897.0
141.80	158.0
142.90	1409.0
143.90	101.0
144.90	422.0
145.90	243.0
147.80	223.0
149.80	132.0
154.90	311.0
156.80	245.0
170.90	166.0
171.90	1385.0
173.00	1266.0
173.90	90824.0
174.90	6604.0
175.90	89536.0
176.90	6102.0
177.90	235.0

Instrument :
MSVOA_U
ClientSampleId :
BFB066

m/z	Abundance
35.90	817.0
36.90	3952.0
37.90	3966.0
38.90	1695.0
40.10	213.0
43.90	799.0
44.90	671.0
46.00	168.0
46.90	845.0
47.90	592.0
48.90	3995.0
49.90	17680.0
50.90	5611.0
51.90	269.0
54.80	241.0
55.90	1556.0
56.90	2942.0
59.90	1005.0
60.90	4963.0
61.90	4783.0
62.90	3975.0
63.90	655.0
64.90	1124.0
65.90	161.0
67.00	303.0
67.90	10734.0
69.00	10908.0
69.90	758.0
71.90	554.0
72.90	4845.0
74.00	18216.0
75.00	54432.0
76.00	4914.0
77.00	799.0
77.80	389.0
78.80	3812.0
79.90	1358.0
80.90	3829.0
81.80	953.0
82.90	121.0
86.90	5234.0
87.90	4462.0
90.90	500.0
91.90	3008.0
92.90	4579.0
93.90	12010.0
95.00	107928.0
96.00	7188.0
96.90	201.0
103.80	545.0
104.80	166.0
105.80	468.0
109.60	110.0
111.80	124.0
114.90	127.0
115.80	337.0
116.80	828.0
117.80	429.0
118.80	590.0
127.90	467.0
128.90	233.0
129.80	395.0
130.70	113.0
134.80	244.0
136.80	114.0
140.90	955.0
141.80	151.0
142.90	1386.0
143.90	107.0
144.90	441.0
145.90	219.0
147.80	212.0
149.90	157.0
154.90	314.0
156.80	319.0
158.80	105.0
170.80	205.0
171.90	1458.0
173.00	1167.0
173.90	93264.0
174.90	6621.0
175.90	91912.0
176.90	6199.0
177.90	186.0

Instrument :
MSVOA_U
ClientSampleId :
BFB066

m/z	Abundance
35.90	790.0
36.90	3386.0
37.90	3549.0
38.90	1503.0
39.90	214.0
43.90	751.0
44.90	646.0
46.80	846.0
47.90	570.0
48.90	3714.0
49.90	15828.0
51.00	5209.0
51.80	199.0
54.80	247.0
55.90	1481.0
56.90	2606.0
59.90	1017.0
60.90	4679.0
62.00	4609.0
62.90	3530.0
64.00	539.0
64.90	1047.0
65.90	161.0
67.00	283.0
67.90	9936.0
68.90	10068.0
69.90	637.0
71.90	536.0
72.90	4564.0
73.90	17264.0
75.00	49544.0
76.00	4652.0
77.00	785.0
77.80	338.0
78.80	3451.0
79.80	1196.0
80.90	3491.0
81.80	817.0
82.80	109.0
85.70	104.0
86.90	4626.0
87.90	4204.0
90.80	489.0
91.90	3000.0
92.90	4066.0
93.90	11062.0
95.00	99976.0
96.00	6490.0
96.90	160.0
103.80	516.0
104.80	178.0
105.90	445.0
111.90	116.0
114.90	137.0
115.80	308.0
116.80	814.0
117.80	383.0
118.80	514.0
127.80	445.0
128.80	242.0
129.80	320.0
130.70	105.0
134.80	225.0
136.80	109.0
140.90	959.0
141.80	141.0
142.90	1287.0
143.90	117.0
144.90	439.0
145.80	134.0
147.80	207.0
149.90	136.0
154.90	255.0
156.80	311.0
158.70	155.0
170.80	238.0
171.90	1437.0
172.90	939.0
173.90	87600.0
174.90	5991.0
175.90	86656.0
176.90	5731.0
177.80	134.0

Instrument :
MSVOA_U
ClientSampleId :
BFB066