




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062224\
Data File : VU059418.D
Acq On : 21 Jun 2024 18:48
Operator : MD/SY
Sample : P2898-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GB1

Manual IntegrationsAPPROVED

Quant Time: Jun 22 01:38:39 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 22 01:35:04 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/25/2024
Supervised By :Semsettin Yesilyurt 06/25/2024

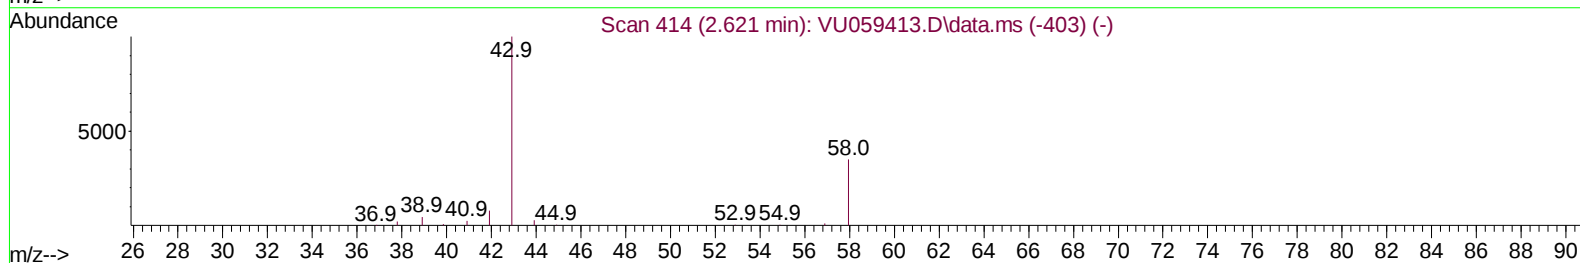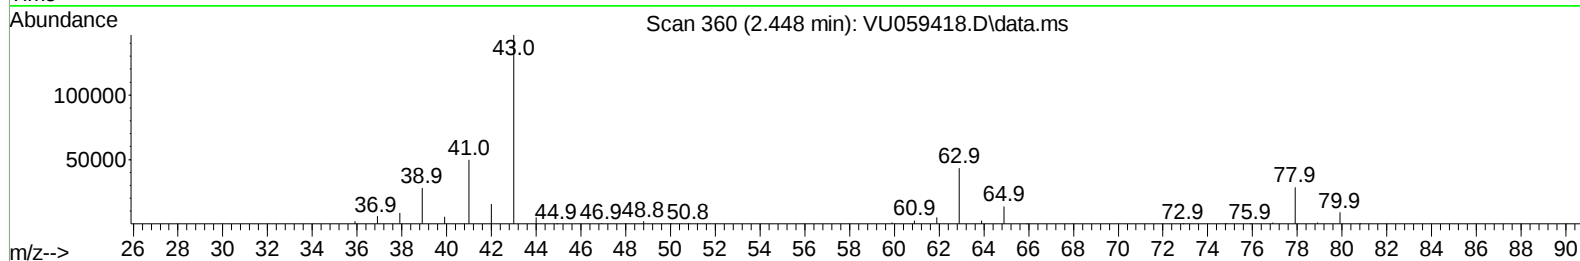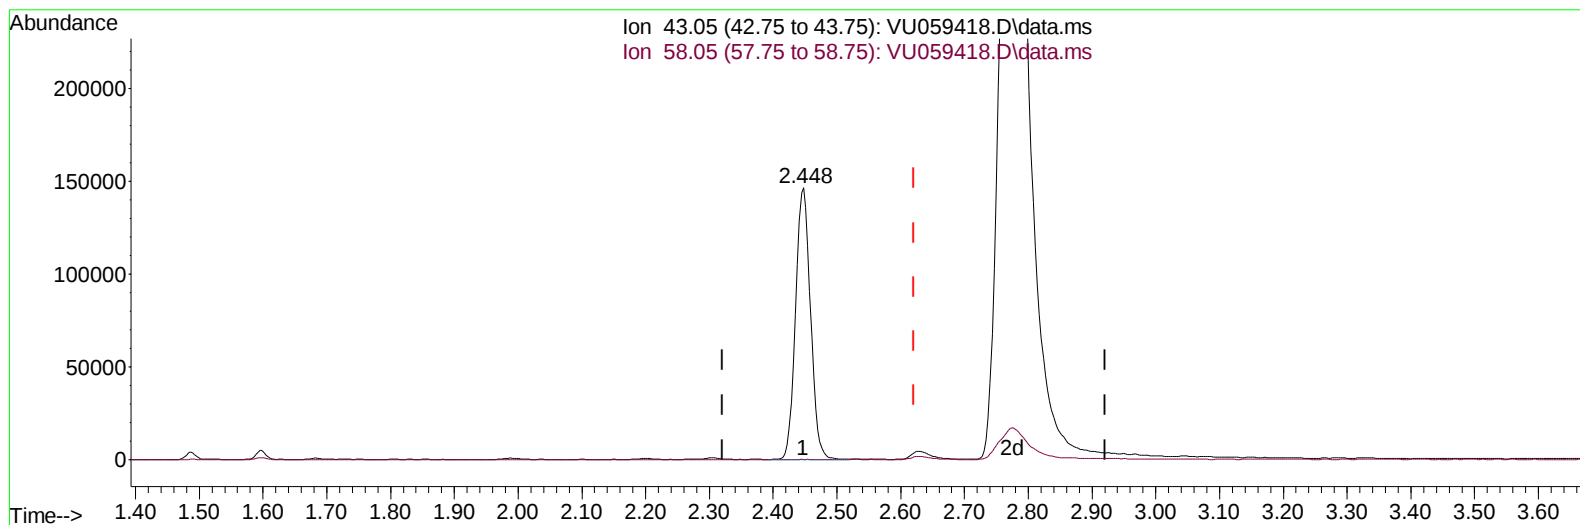

TIC: VU059418.D\data.ms

(13) Acetone (T)

2.448min (-0.174) 156.85 ug/L

response 238485

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	1.46
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062224\
Data File : VU059418.D
Acq On : 21 Jun 2024 18:48
Operator : MD/SY
Sample : P2898-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GB1

Manual IntegrationsAPPROVED

Quant Time: Jun 22 01:38:39 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 22 01:35:04 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/25/2024
Supervised By :Semsettin Yesilyurt 06/25/2024

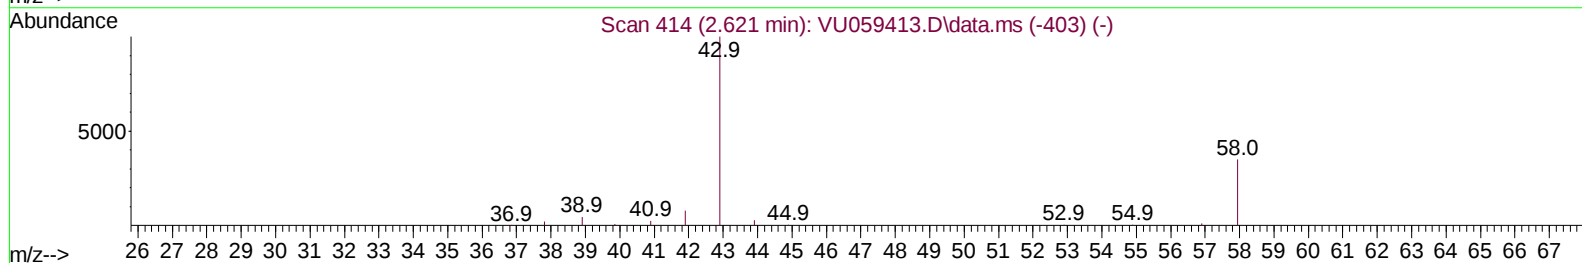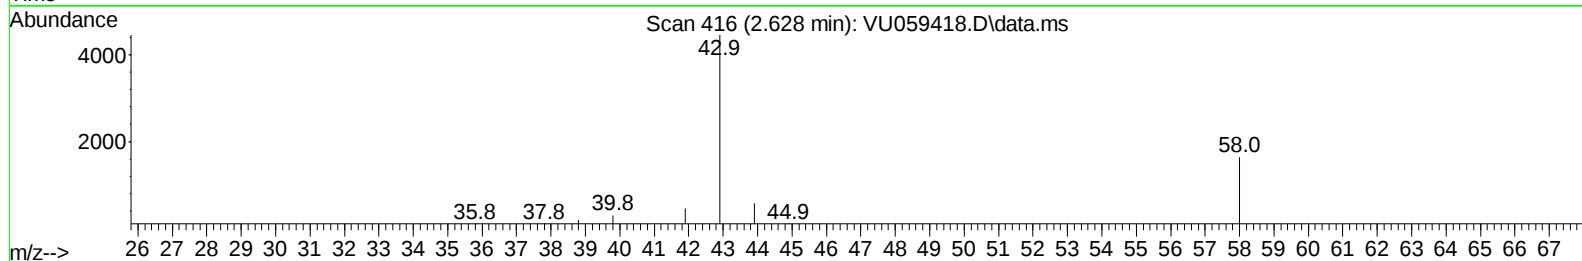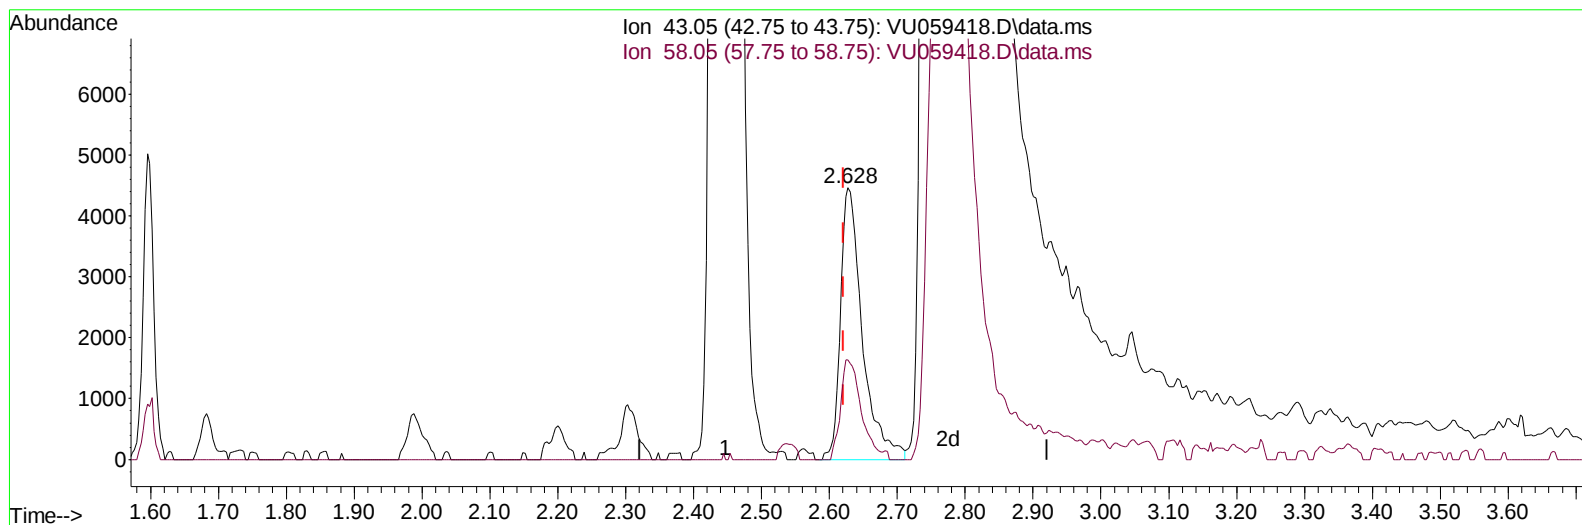

TIC: VU059418.D\data.ms

(13) Acetone (T)

2.628min (+ 0.006) 6.57 ug/L m

response 9984

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	34.98
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062224\
 Data File : VU059418.D
 Acq On : 21 Jun 2024 18:48
 Operator : MD/SY
 Sample : P2898-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GB1

Manual IntegrationsAPPROVED

Quant Time: Jun 22 01:38:39 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 22 01:35:04 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/25/2024
 Supervised By :Semsettin Yesilyurt 06/25/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.245	114		163641	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		164764	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.811	152		77890	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.592	65		42559	3.740	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	74.800%	
7) Chloroethane-d5	1.907	69		46169	4.217	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	84.400%	
11) 1,1-Dichloroethene-d2	2.560	65		18764	3.975	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	79.400%	
20) 2-Butanone-d5	4.618	46		138283	58.998	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery	=	118.000%	
24) Chloroform-d	5.055	84		102710	4.398	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	88.000%	
26) 1,2-Dichloroethane-d4	5.695	65		52960	4.707	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	94.200%	
32) Benzene-d6	5.724	84		197961	4.366	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	87.400%	
36) 1,2-Dichloropropane-d6	6.685	67		64964	4.675	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	93.600%	
41) Toluene-d8	7.894	98		163708	3.883	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	77.600%	
43) trans-1,3-Dichloroprop...	8.177	79		19530	4.489	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	89.800%	
46) 2-Hexanone-d5	8.627	63		104776	57.956	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	115.920%	
56) 1,1,2,2-Tetrachloroeth...	10.749	84		58694	5.112	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	102.200%	
66) 1,2-Dichlorobenzene-d4	12.190	152		65391	4.717	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	94.400%	
Target Compounds							
5) vinyl chloride	1.599	62		14264	0.865	ug/L	98
13) Acetone	2.628	43		9984m	6.567	ug/L	
22) cis-1,2-Dichloroethene	4.660	96		168679	12.679	ug/L	94
34) Trichloroethene	6.537	95		26586	1.962	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062224\
Data File : VU059418.D
Acq On : 21 Jun 2024 18:48
Operator : MD/SY
Sample : P2898-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GB1

Manual IntegrationsAPPROVED

Quant Time: Jun 22 01:38:39 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 22 01:35:04 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/25/2024
Supervised By :Semsettin Yesilyurt 06/25/2024

