

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062224\
 Data File : VU059416.D
 Acq On : 21 Jun 2024 17:59
 Operator : MD/SY
 Sample : P2898-06DL 10X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1G84DL

Quant Time: Jun 22 01:38:04 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 22 01:35:04 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	167875	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	168746	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.811	152	79582	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	46253	3.962	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	79.200%
7) Chloroethane-d5	1.908	69	48705	4.336	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	86.800%
11) 1,1-Dichloroethene-d2	2.560	65	19265	3.978	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	79.600%
20) 2-Butanone-d5	4.621	46	146528	60.939	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	121.880%
24) Chloroform-d	5.055	84	105910	4.420	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.400%
26) 1,2-Dichloroethane-d4	5.698	65	56674	4.910	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.200%
32) Benzene-d6	5.721	84	208659	4.493	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.800%
36) 1,2-Dichloropropane-d6	6.685	67	68983	4.847	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.000%
41) Toluene-d8	7.894	98	174839	4.050	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.000%
43) trans-1,3-Dichloroprop...	8.177	79	21333	4.787	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.800%
46) 2-Hexanone-d5	8.628	63	109812	59.308	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	118.620%
56) 1,1,2,2-Tetrachloroeth...	10.753	84	62780	5.339	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	106.800%
66) 1,2-Dichlorobenzene-d4	12.190	152	68829	4.859	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.200%
Target Compounds						
					Qvalue	
16) Methylene chloride	3.039	84	6455	0.458	ug/L	97
18) trans-1,2-Dichloroethene	3.351	96	2214	0.179	ug/L	99
22) cis-1,2-Dichloroethene	4.660	96	78912	5.782	ug/L	97
34) Trichloroethene	6.541	95	5348	0.385	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062224\
Data File : VU059416.D
Acq On : 21 Jun 2024 17:59
Operator : MD/SY
Sample : P2898-06DL 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G84DL

Quant Time: Jun 22 01:38:04 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 22 01:35:04 2024
Response via : Initial Calibration




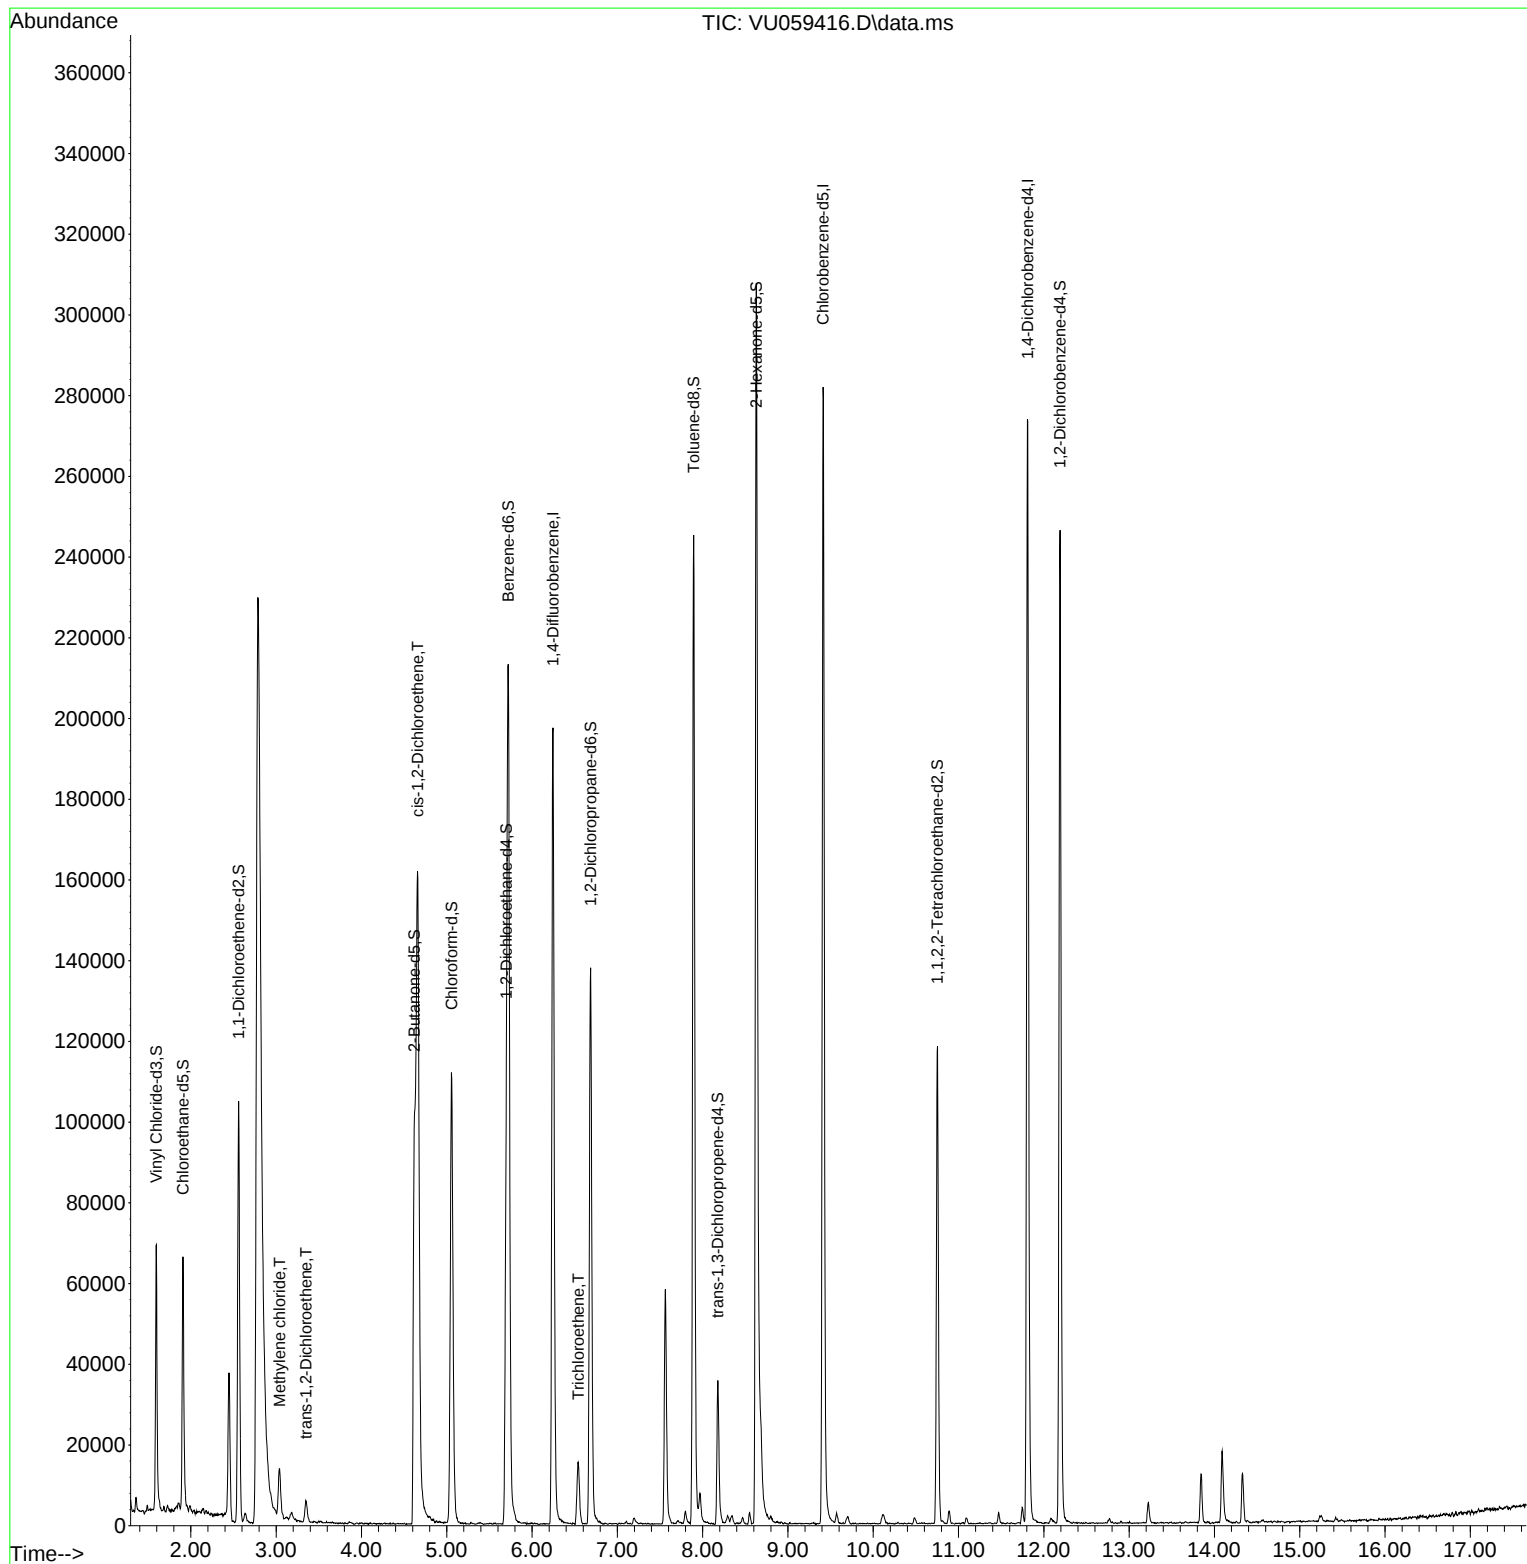


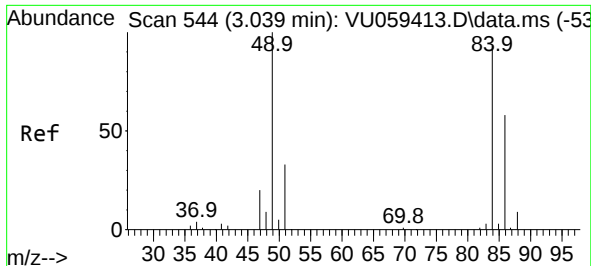

#16
Methylene chloride
Concen: 0.458 ug/L
RT: 3.039 min Scan# 54
Delta R.T. 0.000 min
Lab File: VU059416.D
Acq: 21 Jun 2024 17:59




Instrument :
MSVOA_U
ClientSampleId :
E1G84DL


Tgt Ion: 84 Resp: 6455
Ion Ratio Lower Upper
84 100
86 61.2 42.1 78.1
49 111.6 80.6 149.8

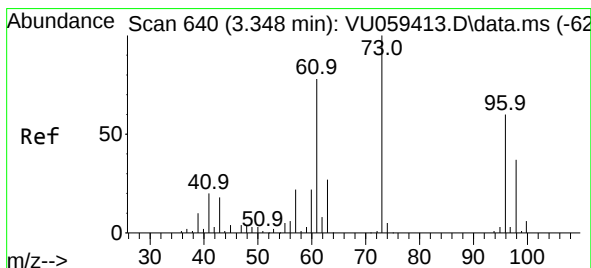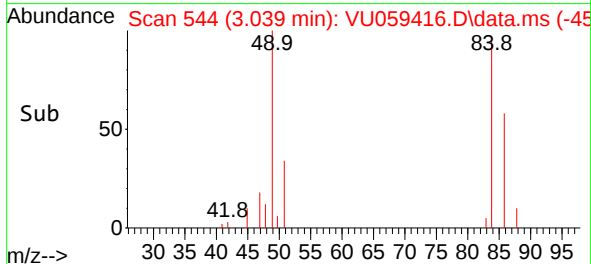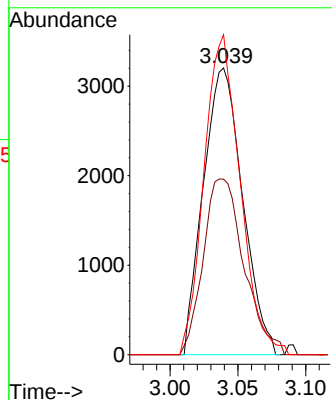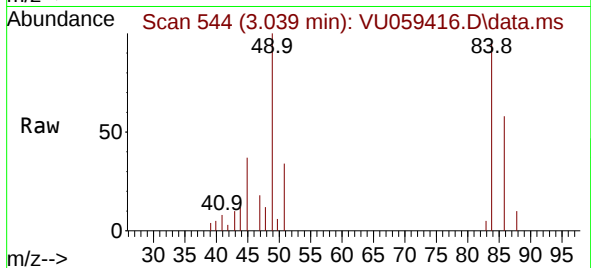

#18
trans-1,2-Dichloroethene
Concen: 0.179 ug/L
RT: 3.351 min Scan# 641
Delta R.T. 0.003 min
Lab File: VU059416.D
Acq: 21 Jun 2024 17:59

Tgt Ion: 96 Resp: 2214
Ion Ratio Lower Upper
96 100
61 147.0 101.8 189.0
98 60.4 43.3 80.5


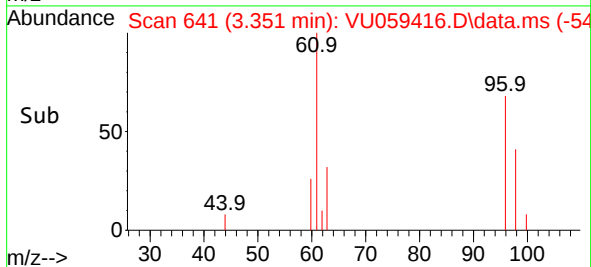
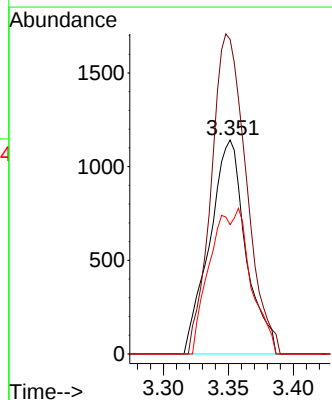
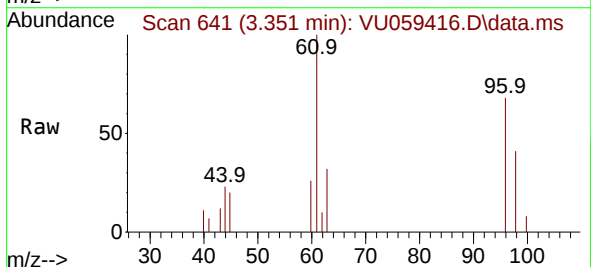


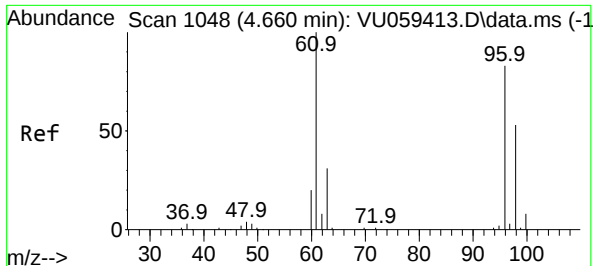

#22
 cis-1,2-Dichloroethene
 Concen: 5.782 ug/L
 RT: 4.660 min Scan# 1048
 Delta R.T. 0.000 min
 Lab File: VU059416.D
 Acq: 21 Jun 2024 17:59

Instrument :
 MSVOA_U
 ClientSampleId :
 E1G84DL

Tgt Ion: 96 Resp: 78912
 Ion Ratio Lower Upper
 96 100
 61 122.5 87.4 162.2
 98 64.7 42.3 78.5

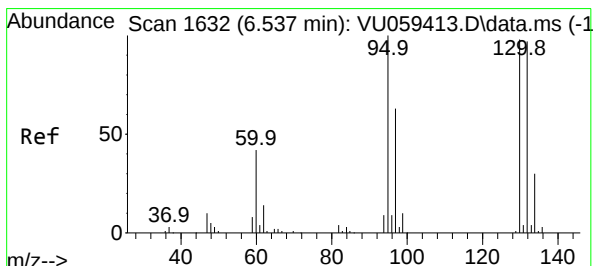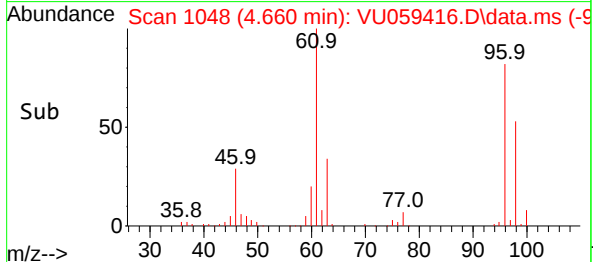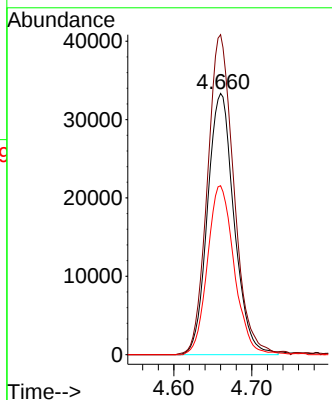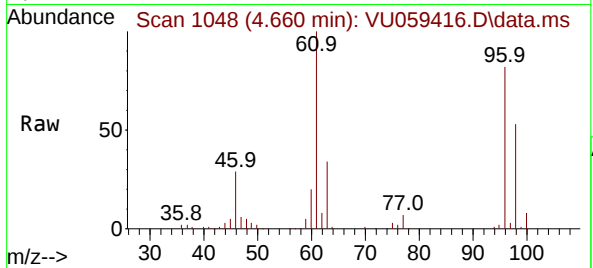

#34
 Trichloroethene
 Concen: 0.385 ug/L
 RT: 6.541 min Scan# 1633
 Delta R.T. 0.003 min
 Lab File: VU059416.D
 Acq: 21 Jun 2024 17:59

Tgt Ion: 95 Resp: 5348
 Ion Ratio Lower Upper
 95 100
 97 63.8 45.3 84.1
 132 101.5 64.0 119.0
 130 100.2 69.1 128.3

