

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062224\
 Data File : VU059426.D
 Acq On : 21 Jun 2024 22:59
 Operator : MD/SY
 Sample : P2936-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B03

Quant Time: Jun 22 01:40:42 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 22 01:35:04 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	148503	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	152886	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	65627	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	39997	3.873	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	77.400%
7) Chloroethane-d5	1.908	69	43709	4.399	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.000%
11) 1,1-Dichloroethene-d2	2.557	65	15925	3.717	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.400%
20) 2-Butanone-d5	4.618	46	124506	58.535	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	117.060%
24) Chloroform-d	5.055	84	94152	4.442	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.800%
26) 1,2-Dichloroethane-d4	5.695	65	49401	4.839	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.800%
32) Benzene-d6	5.721	84	182526	4.338	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.800%
36) 1,2-Dichloropropane-d6	6.685	67	60847	4.719	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.400%
41) Toluene-d8	7.894	98	144855	3.703	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	74.000%
43) trans-1,3-Dichloroprop...	8.177	79	16301	4.038	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.800%
46) 2-Hexanone-d5	8.628	63	88603	52.818	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	105.640%
56) 1,1,2,2-Tetrachloroeth...	10.750	84	54914	5.155	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	103.000%
66) 1,2-Dichlorobenzene-d4	12.190	152	59603	5.103	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.000%
Target Compounds						Qvalue
16) Methylene chloride	3.039	84	3435	0.275	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062224\
Data File : VU059426.D
Acq On : 21 Jun 2024 22:59
Operator : MD/SY
Sample : P2936-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B03


Quant Time: Jun 22 01:40:42 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 22 01:35:04 2024
Response via : Initial Calibration

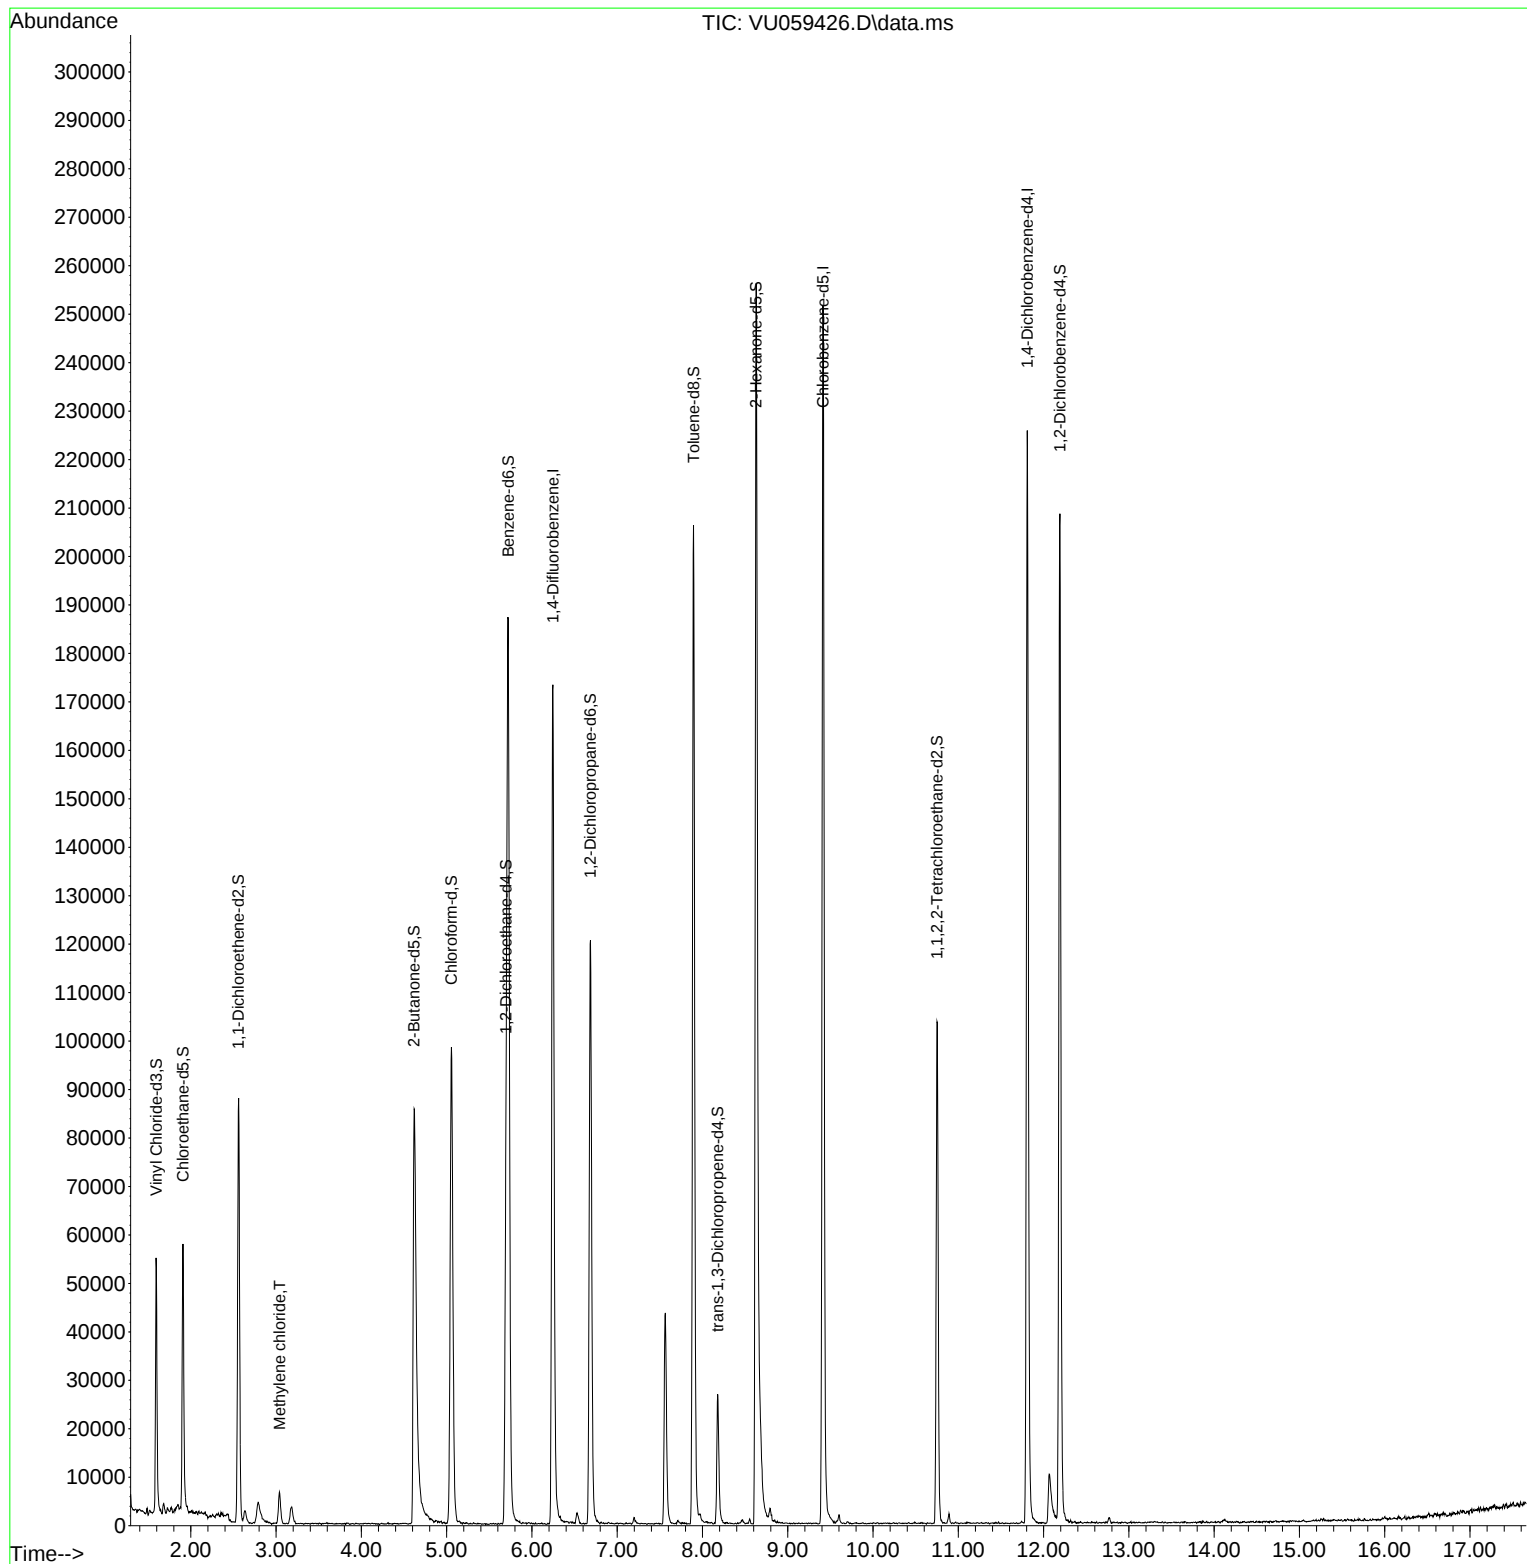

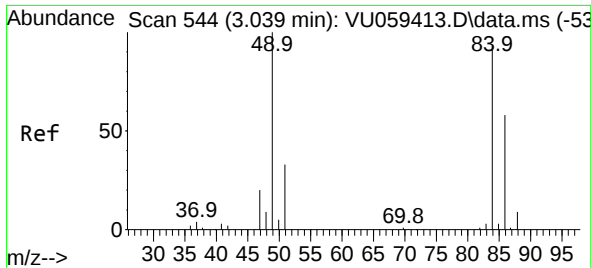

#16
Methylene chloride
Concen: 0.275 ug/L
RT: 3.039 min Scan# 54
Delta R.T. 0.000 min
Lab File: VU059426.D
Acq: 21 Jun 2024 22:59

Instrument :
MSVOA_U
ClientSampleId :
C0B03

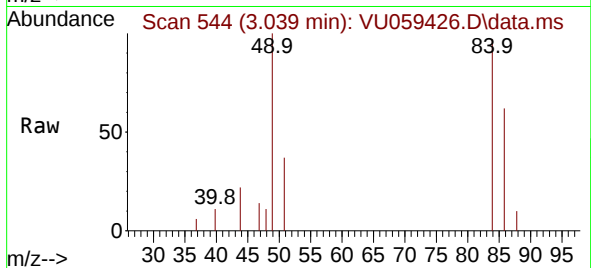

Tgt Ion: 84 Resp: 3435
Ion Ratio Lower Upper
84 100
86 64.7 42.1 78.1
49 103.6 80.6 149.8

