

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062224\
 Data File : VU059417.D
 Acq On : 21 Jun 2024 18:24
 Operator : MD/SY
 Sample : P2898-07DL 10X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1G85DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU059417.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	86	95	116	rVB3	76129	98667	8.57%	1.432%
2	1.907	183	192	206	rBV	59080	78893	6.85%	1.145%
3	2.447	349	360	375	rVB	33290	54497	4.73%	0.791%
4	2.560	384	395	408	rBV	99151	162909	14.15%	2.364%
5	2.775	445	462	513	rBV	388705	1150968	100.00%	16.703%
6	3.036	534	543	561	rVB2	13452	26840	2.33%	0.389%
7	4.660	1021	1048	1082	rBV3	302144	928547	80.68%	13.475%
8	5.055	1156	1171	1194	rBV	106351	237689	20.65%	3.449%
9	5.721	1359	1378	1414	rBV2	204814	548795	47.68%	7.964%
10	6.245	1528	1541	1565	rBV	192990	370376	32.18%	5.375%
11	6.537	1619	1632	1653	rBV	161686	310395	26.97%	4.504%
12	6.685	1666	1678	1703	rBV2	132351	259996	22.59%	3.773%
13	7.563	1937	1951	1967	rBV2	55141	97495	8.47%	1.415%
14	7.894	2041	2054	2071	rBV	237127	412465	35.84%	5.986%
15	8.177	2132	2142	2159	rBV2	33214	58034	5.04%	0.842%
16	8.627	2271	2282	2322	rBV	294308	592228	51.45%	8.594%
17	9.415	2514	2527	2551	rBV	277404	476043	41.36%	6.908%
18	10.753	2928	2943	2962	rBV	115086	186770	16.23%	2.710%
19	11.810	3260	3272	3291	rBV	271079	442134	38.41%	6.416%
20	12.190	3377	3390	3416	rBV	237449	397163	34.51%	5.764%




Sum of corrected areas: 6890904

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062224\
Data File : VU059417.D
Acq On : 21 Jun 2024 18:24
Operator : MD/SY
Sample : P2898-07DL 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G85DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

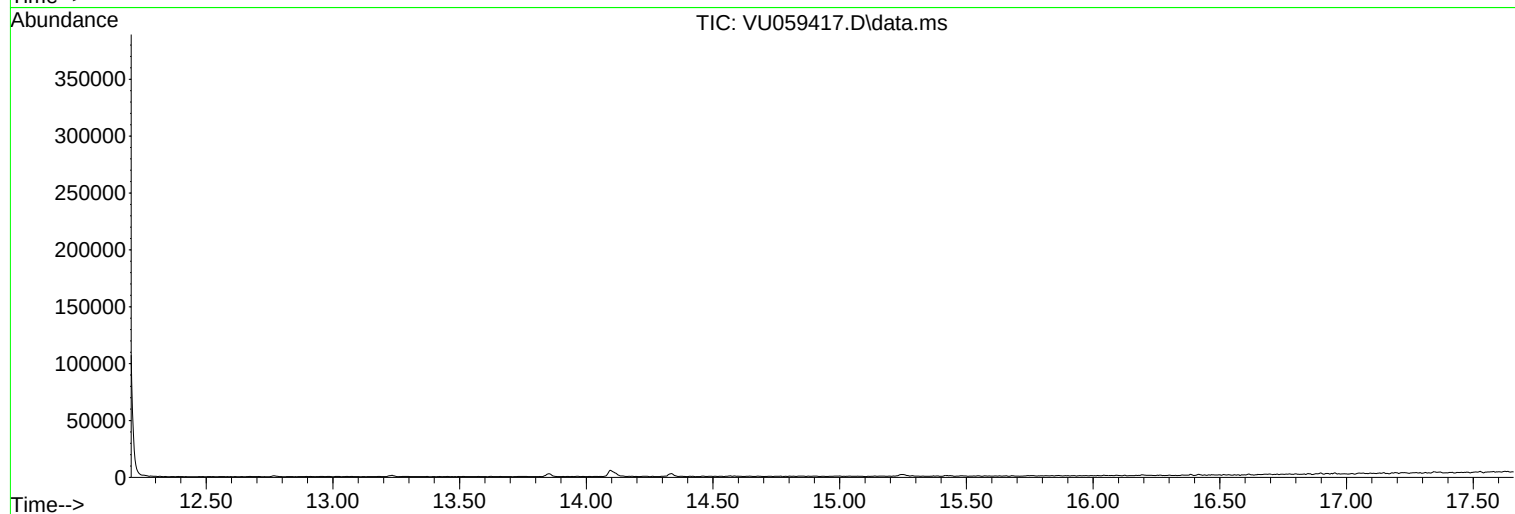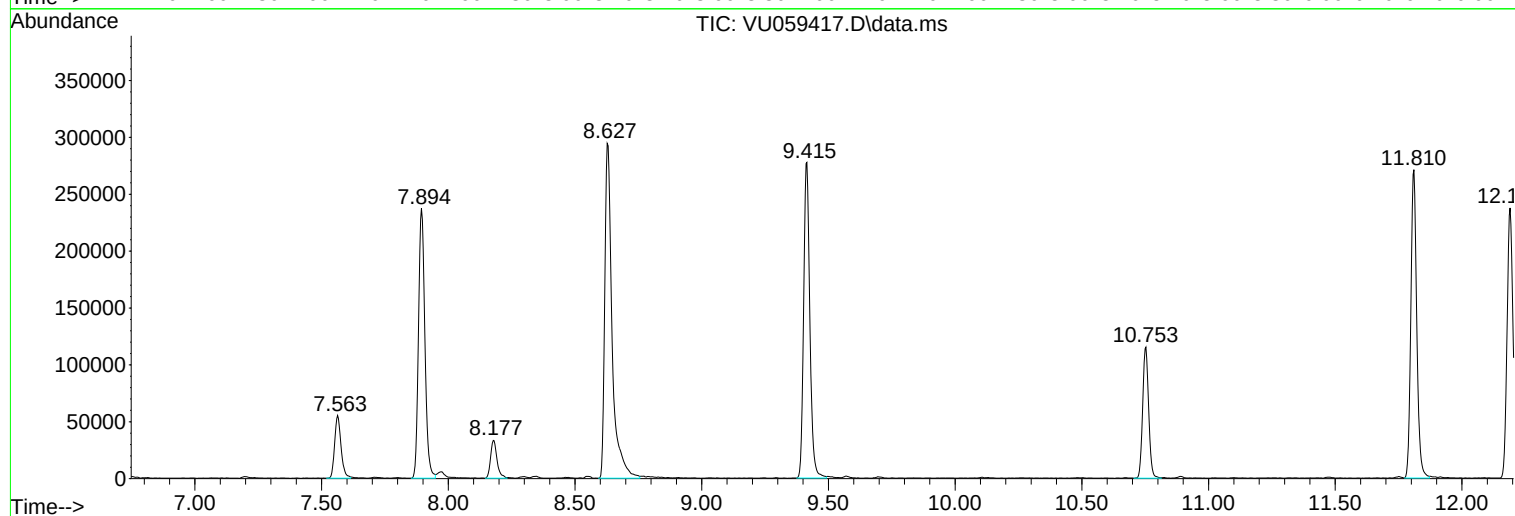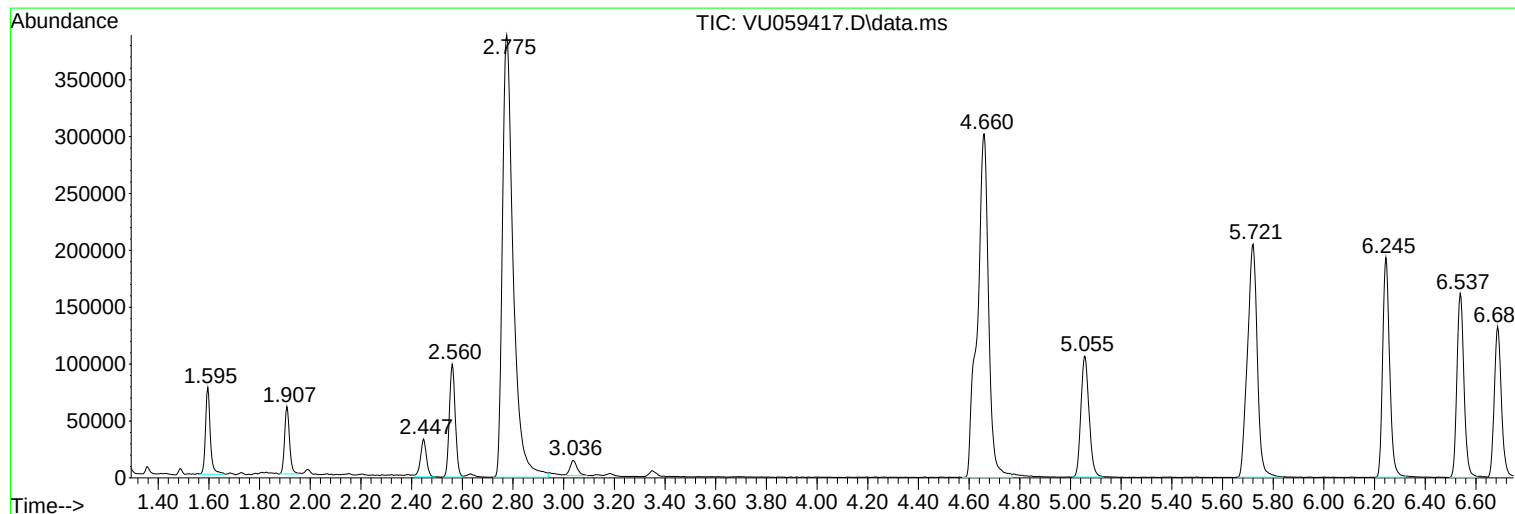

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062224\
Data File : VU059417.D
Acq On : 21 Jun 2024 18:24
Operator : MD/SY
Sample : P2898-07DL 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G85DL










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propane, 2-chloro- Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.447	0.74 ug/L	54497	1,4-Difluorobenzene	6.245

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propane, 2-chloro-	78	C3H7Cl	000075-29-6	90
2			Propane, 2-chloro-	78	C3H7Cl	000075-29-6	64
3			Propane, 2-chloro-	78	C3H7Cl	000075-29-6	38
4			2-Chloroethanol	80	C2H5ClO	000107-07-3	4
5			Acetyl chloride	78	C2H3ClO	000075-36-5	4

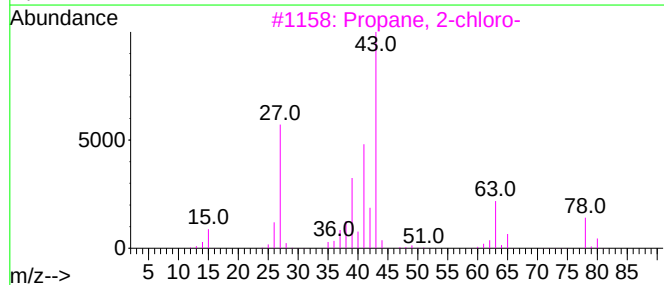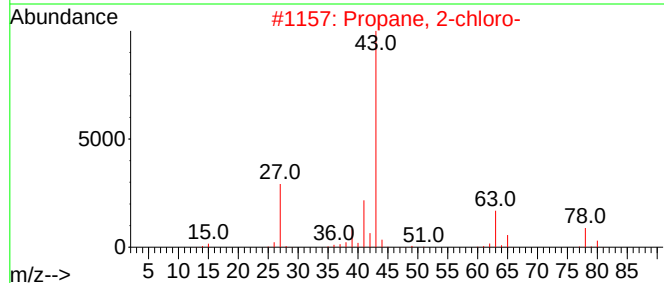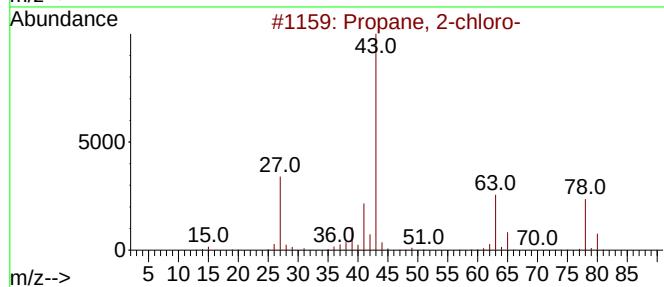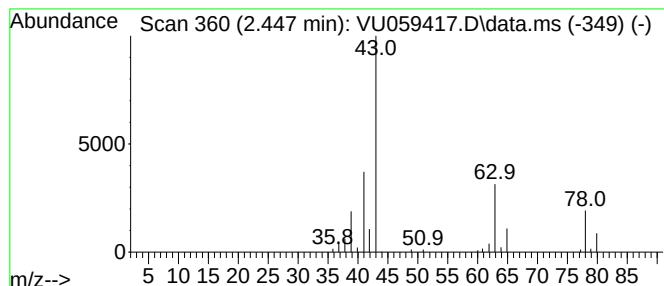

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062224\
Data File : VU059417.D
Acq On : 21 Jun 2024 18:24
Operator : MD/SY
Sample : P2898-07DL 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G85DL










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.775	15.54 ug/L	1150970	1,4-Difluorobenzene	6.245

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Isopropyl Alcohol			60	C3H8O	000067-63-0	86
2	Isopropyl Alcohol			60	C3H8O	000067-63-0	78
3	Isopropyl Alcohol			60	C3H8O	000067-63-0	64
4	Isopropyl Alcohol			60	C3H8O	000067-63-0	56
5	Isopropyl Alcohol			60	C3H8O	000067-63-0	56

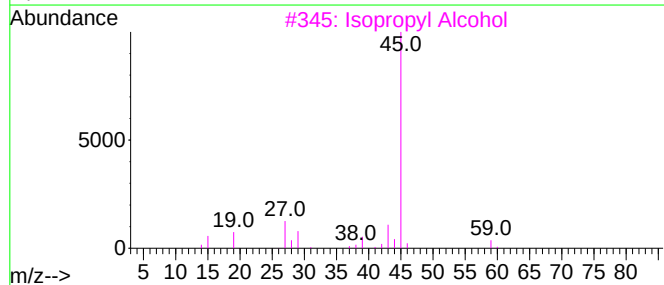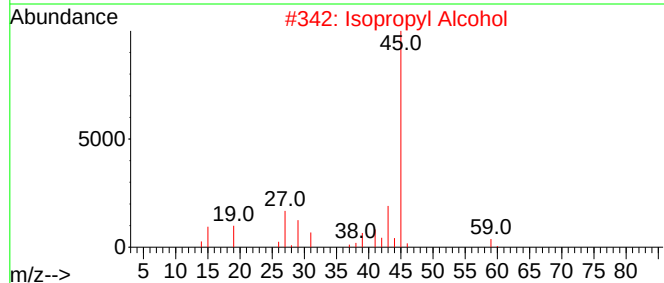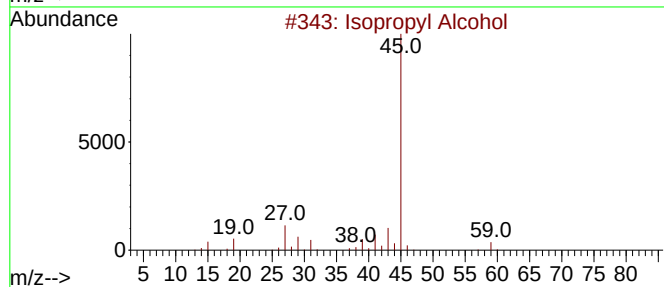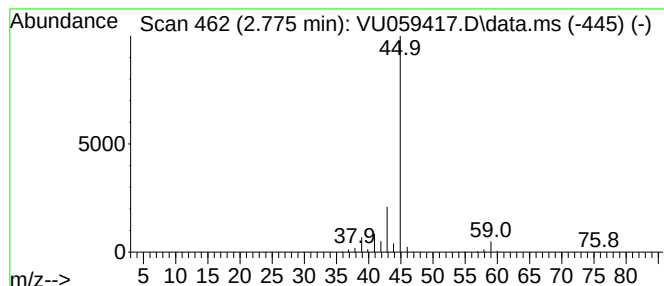

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062224\
Data File : VU059417.D
Acq On : 21 Jun 2024 18:24
Operator : MD/SY
Sample : P2898-07DL 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G85DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propane, 2-chloro-	2.447	0.7	ug/L	54497	1	6.245	370376	5.0
Isopropyl Alcohol	2.775	15.5	ug/L	1150970	1	6.245	370376	5.0