


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062224\
Data File : VU059412.D
Acq On : 21 Jun 2024 14:56
Operator : MD/SY
Sample : BFB164
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB164

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Jun 22 01:35:04 2024

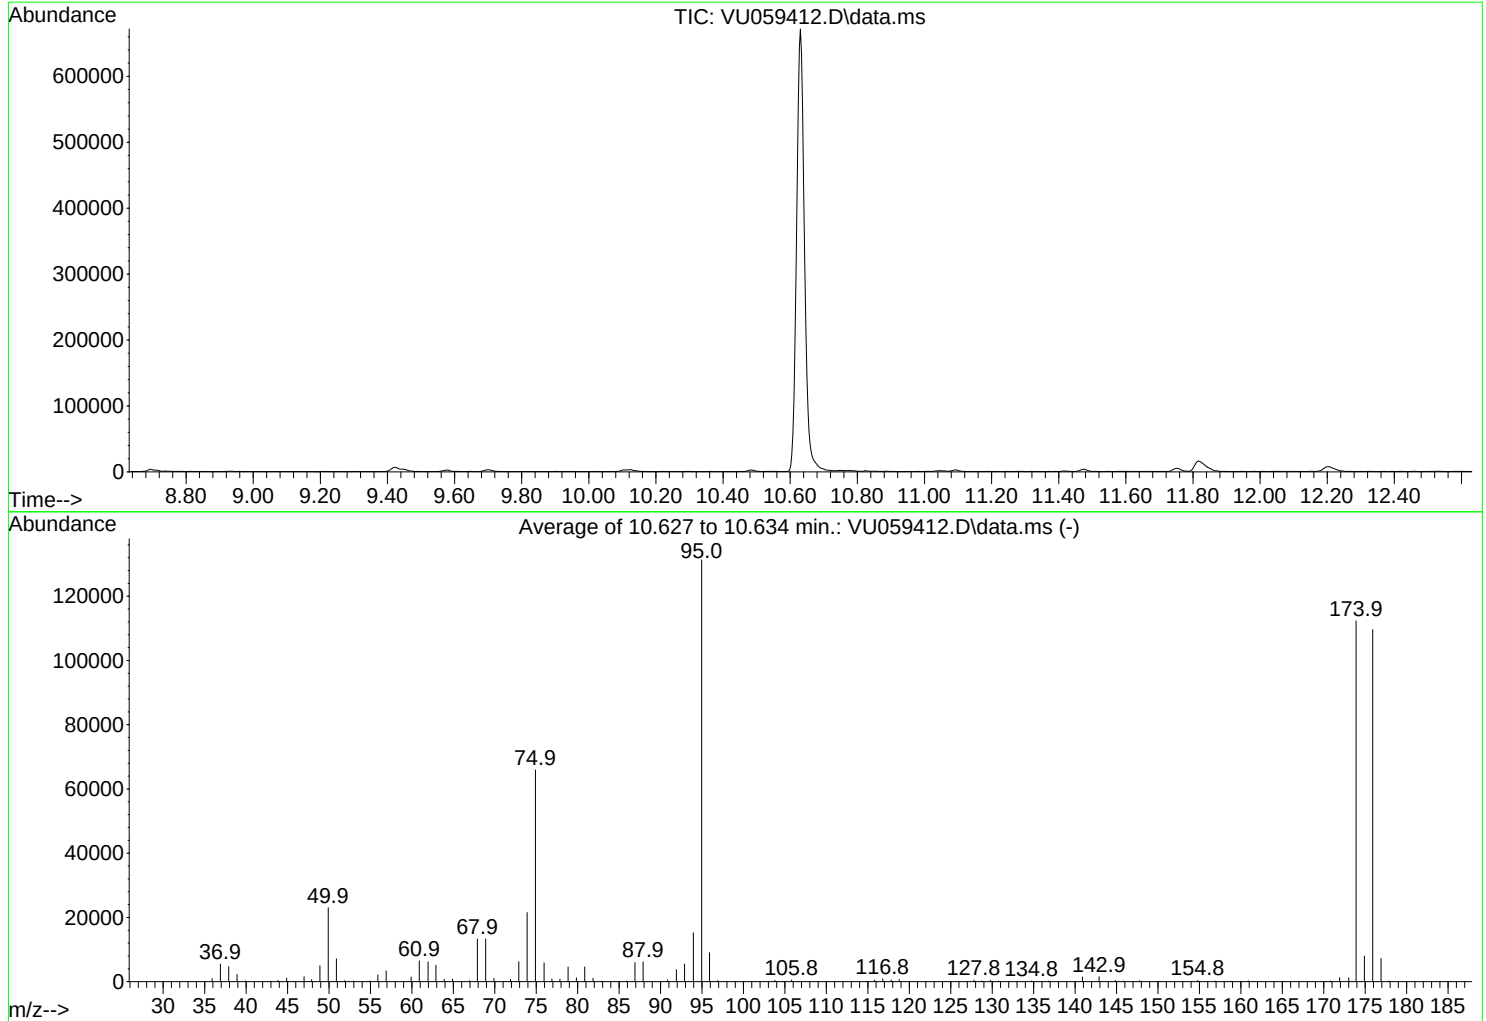

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	23019	PASS
75	95	30	80	50.2	65928	PASS
95	95	100	100	100.0	131325	PASS
96	95	5	9	6.9	9017	PASS
173	174	0.00	2	1.1	1204	PASS
174	95	50	120	85.5	112328	PASS
175	174	5	9	7.1	7994	PASS
176	174	95	101	97.6	109640	PASS
177	176	5	9	6.6	7237	PASS

Scan 2890 (10.582 min): VU059412.D\data.ms
BFB164

m/z	Abundance
39.70	215.0
43.90	426.0

Instrument :
MSVOA_U
ClientSampleId :
BFB164

m/z	Abundance
35.90	1018.0
36.90	5747.0
37.90	4809.0
38.90	2218.0
39.90	274.0
43.00	149.0
43.80	849.0
44.90	1097.0
47.00	1480.0
47.90	665.0
48.90	4942.0
49.90	23264.0
50.90	7284.0
51.90	266.0
52.90	239.0
55.00	382.0
55.90	2015.0
56.90	3293.0
58.00	129.0
59.90	1556.0
60.90	6689.0
62.00	6141.0
62.90	5362.0
63.90	685.0
64.90	811.0
66.90	370.0
67.90	13152.0
68.90	13558.0
69.90	1053.0
71.90	641.0
72.90	6157.0
73.90	21568.0
74.90	66048.0
76.00	6011.0
76.90	986.0
77.80	776.0
78.90	4610.0
79.90	1278.0
80.80	4505.0
81.80	1134.0
82.80	136.0
85.90	256.0
86.90	5934.0
87.90	6409.0
90.90	605.0
91.90	3740.0
92.90	5580.0
94.00	15108.0
95.00	131264.0
95.90	8982.0
96.90	330.0
103.80	435.0
104.70	178.0
105.80	476.0
106.70	130.0
111.00	152.0
114.80	105.0
115.80	489.0
116.80	843.0
117.80	488.0
118.80	591.0
127.80	484.0
128.70	264.0
129.80	460.0
130.80	198.0
134.80	289.0
136.80	261.0
140.90	1348.0
142.90	1599.0
144.90	432.0
145.80	173.0
147.80	282.0
149.70	123.0
154.80	411.0
156.90	162.0
158.80	167.0
160.90	276.0
170.80	177.0
171.90	1156.0
173.00	1102.0
173.90	109240.0
174.90	8144.0
175.90	106152.0
176.90	7089.0
177.90	249.0

Instrument :
MSVOA_U
ClientSampleId :
BFB164

m/z	Abundance
35.90	956.0
36.90	5722.0
37.90	4833.0
38.90	2278.0
39.90	254.0
42.90	152.0
43.90	840.0
44.90	1143.0
47.00	1574.0
47.90	591.0
48.90	5142.0
49.90	23840.0
50.90	7319.0
51.90	307.0
52.90	201.0
54.90	376.0
55.90	2203.0
56.90	3446.0
57.90	127.0
59.90	1502.0
60.90	6692.0
62.00	6270.0
62.90	5265.0
63.90	691.0
64.90	838.0
67.00	325.0
67.90	13816.0
68.90	13692.0
69.90	980.0
71.90	734.0
72.90	6536.0
73.90	22168.0
74.90	68128.0
75.90	6054.0
76.90	865.0
77.90	842.0
78.80	4765.0
79.90	1234.0
80.90	4737.0
81.80	1092.0
82.90	149.0
85.90	228.0
86.90	6138.0
87.90	6484.0
90.80	548.0
91.90	3824.0
92.90	5581.0
93.90	15687.0
94.90	135616.0
95.90	9431.0
96.90	383.0
103.80	405.0
104.70	168.0
105.80	533.0
106.70	119.0
111.00	140.0
114.80	115.0
115.80	498.0
116.80	897.0
117.80	535.0
118.80	704.0
127.80	516.0
128.70	260.0
129.80	436.0
130.80	205.0
134.80	243.0
136.80	239.0
140.90	1429.0
142.90	1591.0
144.80	376.0
145.80	217.0
147.80	282.0
152.90	139.0
154.80	433.0
156.90	165.0
158.80	170.0
160.90	286.0
170.80	188.0
171.90	1295.0
173.00	1262.0
173.90	115688.0
174.90	8168.0
175.90	113776.0
176.90	7435.0
177.80	201.0

Instrument :
MSVOA_U
ClientSampleId :
BFB164

m/z	Abundance
35.90	834.0
36.90	5024.0
37.90	4475.0
38.90	2177.0
40.00	232.0
42.90	143.0
43.90	856.0
44.90	1129.0
45.80	151.0
47.00	1545.0
47.90	524.0
48.90	4735.0
49.90	21952.0
50.90	6761.0
51.90	324.0
53.00	153.0
54.70	363.0
55.90	2098.0
56.90	3243.0
57.90	105.0
59.90	1284.0
60.90	6038.0
61.90	6010.0
62.90	4662.0
63.90	707.0
64.90	790.0
67.00	281.0
67.90	12807.0
68.90	12603.0
69.90	937.0
71.90	753.0
72.90	6051.0
73.90	20840.0
74.90	63608.0
75.90	5381.0
76.90	784.0
77.80	805.0
78.80	4449.0
79.80	1132.0
80.90	4458.0
81.90	986.0
82.90	114.0
85.90	183.0
86.90	5714.0
87.90	5699.0
90.80	433.0
91.90	3606.0
92.90	5278.0
93.90	14819.0
94.90	127096.0
95.90	8638.0
96.90	360.0
103.80	398.0
104.90	173.0
105.80	546.0
110.90	127.0
114.80	107.0
115.80	452.0
116.80	898.0
117.80	505.0
118.80	726.0
127.80	492.0
128.80	230.0
129.80	431.0
130.80	200.0
134.70	209.0
136.80	193.0
140.90	1350.0
142.90	1501.0
144.80	329.0
145.80	248.0
147.80	301.0
152.90	187.0
154.80	406.0
156.90	201.0
158.80	178.0
160.90	234.0
170.80	173.0
171.90	1301.0
173.00	1248.0
173.90	112056.0
174.90	7670.0
175.90	108992.0
176.90	7186.0
177.80	160.0

Instrument :
MSVOA_U
ClientSampleId :
BFB164