

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062424\
 Data File : VU059448.D
 Acq On : 24 Jun 2024 14:31
 Operator : MD/SY
 Sample : P2963-15ME
 Misc : 4.59g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Jun 25 03:16:00 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 22 00:01:31 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	6.238	114	217287	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117	227992	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.811	152	108925	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	33763	25.952	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	51.900%#
7) Chloroethane-d5	1.872	69	22829	20.485	ug/L	-0.04
Spiked Amount	50.000	Range	70 - 130	Recovery	=	40.960%#
11) 1,1-Dichloroethene-d2	2.538	63	46988	18.298	ug/L	-0.03
Spiked Amount	50.000	Range	60 - 125	Recovery	=	36.600%#
21) 2-Butanone-d5	4.621	46	95403	77.800	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	77.800%
24) Chloroform-d	5.052	84	94233	36.385	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	72.760%
26) 1,2-Dichloroethane-d4	5.692	65	61173	38.537	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	77.080%
32) Benzene-d6	5.714	84	176173	33.667	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	67.340%#
36) 1,2-Dichloropropane-d6	6.682	67	62219	34.485	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	68.960%#
41) Toluene-d8	7.891	98	143350	32.270	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	64.540%#
43) trans-1,3-Dichloroprop...	8.177	79	24741	33.924	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	67.840%
47) 2-Hexanone-d5	8.637	63	63924	76.617	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	76.620%
56) 1,1,2,2-Tetrachloroeth...	10.753	84	121856	39.906	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	79.820%
66) 1,2-Dichlorobenzene-d4	12.190	152	69416	42.704	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	85.400%
Target Compounds						
15) Methyl Acetate	2.943	43	26091	11.428	ug/L	96
60) 1,2,3-Trichloropropane	11.807	75	13100	4.325	ug/L #	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062424\
Data File : VU059448.D
Acq On : 24 Jun 2024 14:31
Operator : MD/SY
Sample : P2963-15ME
Misc : 4.59g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Jun 25 03:16:00 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jun 22 00:01:31 2024
Response via : Initial Calibration




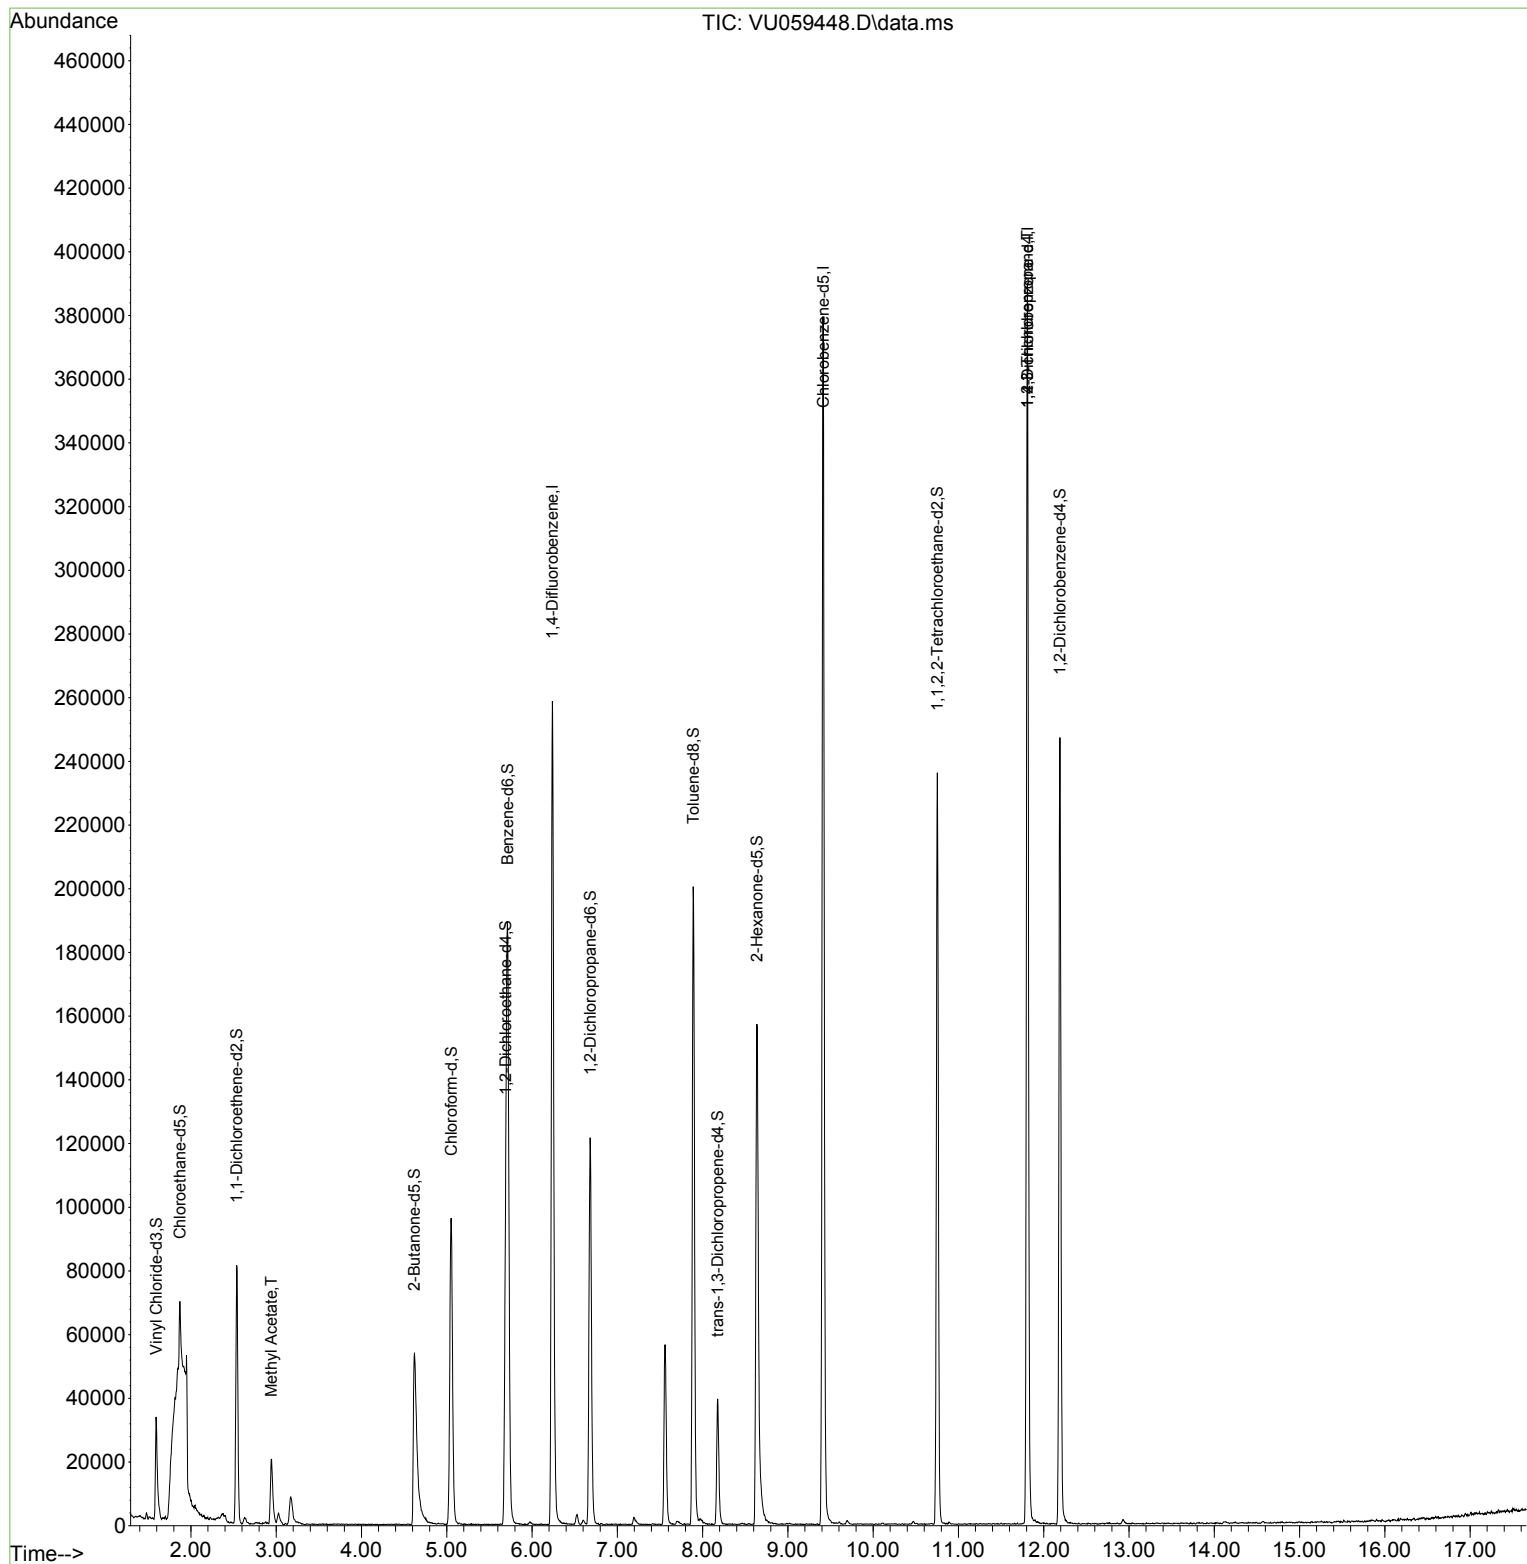


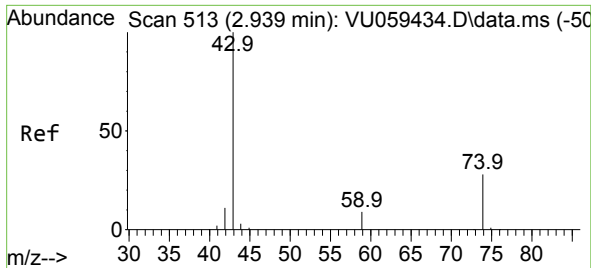

#15
Methyl Acetate
Concen: 11.428 ug/L
RT: 2.943 min Scan# 513
Delta R.T. 0.003 min
Lab File: VU059448.D
Acq: 24 Jun 2024 14:31

Instrument :
MSVOA_U
ClientSampleId :

Tgt Ion: 43 Resp: 26091
Ion Ratio Lower Upper
43 100
74 28.0 20.8 31.2

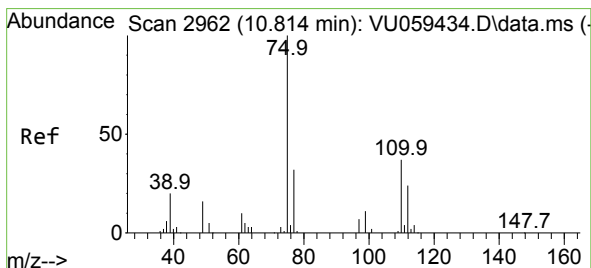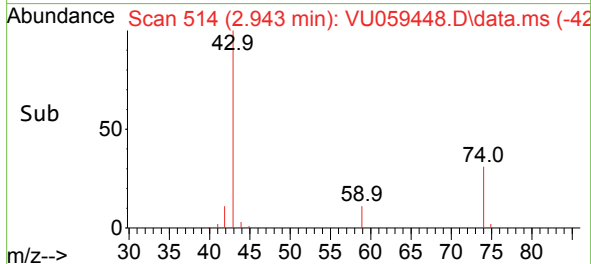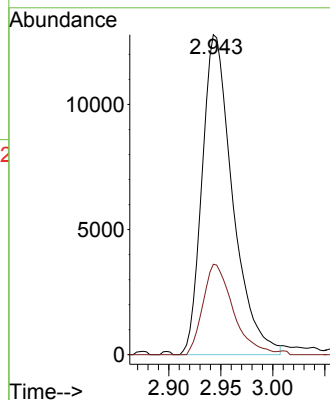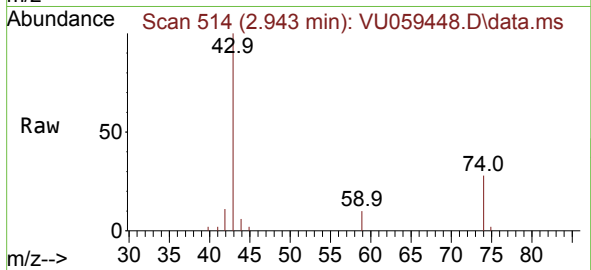

#60
1,2,3-Trichloropropane
Concen: 4.325 ug/L
RT: 11.807 min Scan# 3271
Delta R.T. 0.990 min
Lab File: VU059448.D
Acq: 24 Jun 2024 14:31

Tgt Ion: 75 Resp: 13100
Ion Ratio Lower Upper
75 100
77 31.4 26.2 39.2
110 1.1 28.4 42.6#

