

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062424\
 Data File : VU059444.D
 Acq On : 24 Jun 2024 13:00
 Operator : MD/SY
 Sample : P2909-19ME
 Misc : 4.20g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4B42ME

Quant Time: Jun 25 03:15:10 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 22 00:01:31 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.238	114	213805	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	222960	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	109082	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	32592	25.460	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	50.920%#
7) Chloroethane-d5	1.869	69	22134	20.184	ug/L	-0.04
Spiked Amount	50.000	Range	70 - 130	Recovery	=	40.360%#
11) 1,1-Dichloroethene-d2	2.541	63	47793	18.914	ug/L	-0.02
Spiked Amount	50.000	Range	60 - 125	Recovery	=	37.820%#
21) 2-Butanone-d5	4.618	46	92456	76.624	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	76.620%
24) Chloroform-d	5.052	84	92549	36.316	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	72.640%
26) 1,2-Dichloroethane-d4	5.692	65	59942	38.376	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	76.760%
32) Benzene-d6	5.714	84	174063	34.015	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	68.020%#
36) 1,2-Dichloropropane-d6	6.682	67	61119	34.640	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	69.280%#
41) Toluene-d8	7.891	98	141376	32.544	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	65.080%#
43) trans-1,3-Dichloroprop...	8.174	79	24383	34.188	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	68.380%
47) 2-Hexanone-d5	8.634	63	62711	76.859	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	76.860%
56) 1,1,2,2-Tetrachloroeth...	10.753	84	119131	39.894	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	79.780%
66) 1,2-Dichlorobenzene-d4	12.190	152	68325	41.972	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	83.940%
Target Compounds						
					Qvalue	
15) Methyl Acetate	2.943	43	25359	11.288	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062424\
Data File : VU059444.D
Acq On : 24 Jun 2024 13:00
Operator : MD/SY
Sample : P2909-19ME
Misc : 4.20g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4B42ME

Quant Time: Jun 25 03:15:10 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jun 22 00:01:31 2024
Response via : Initial Calibration

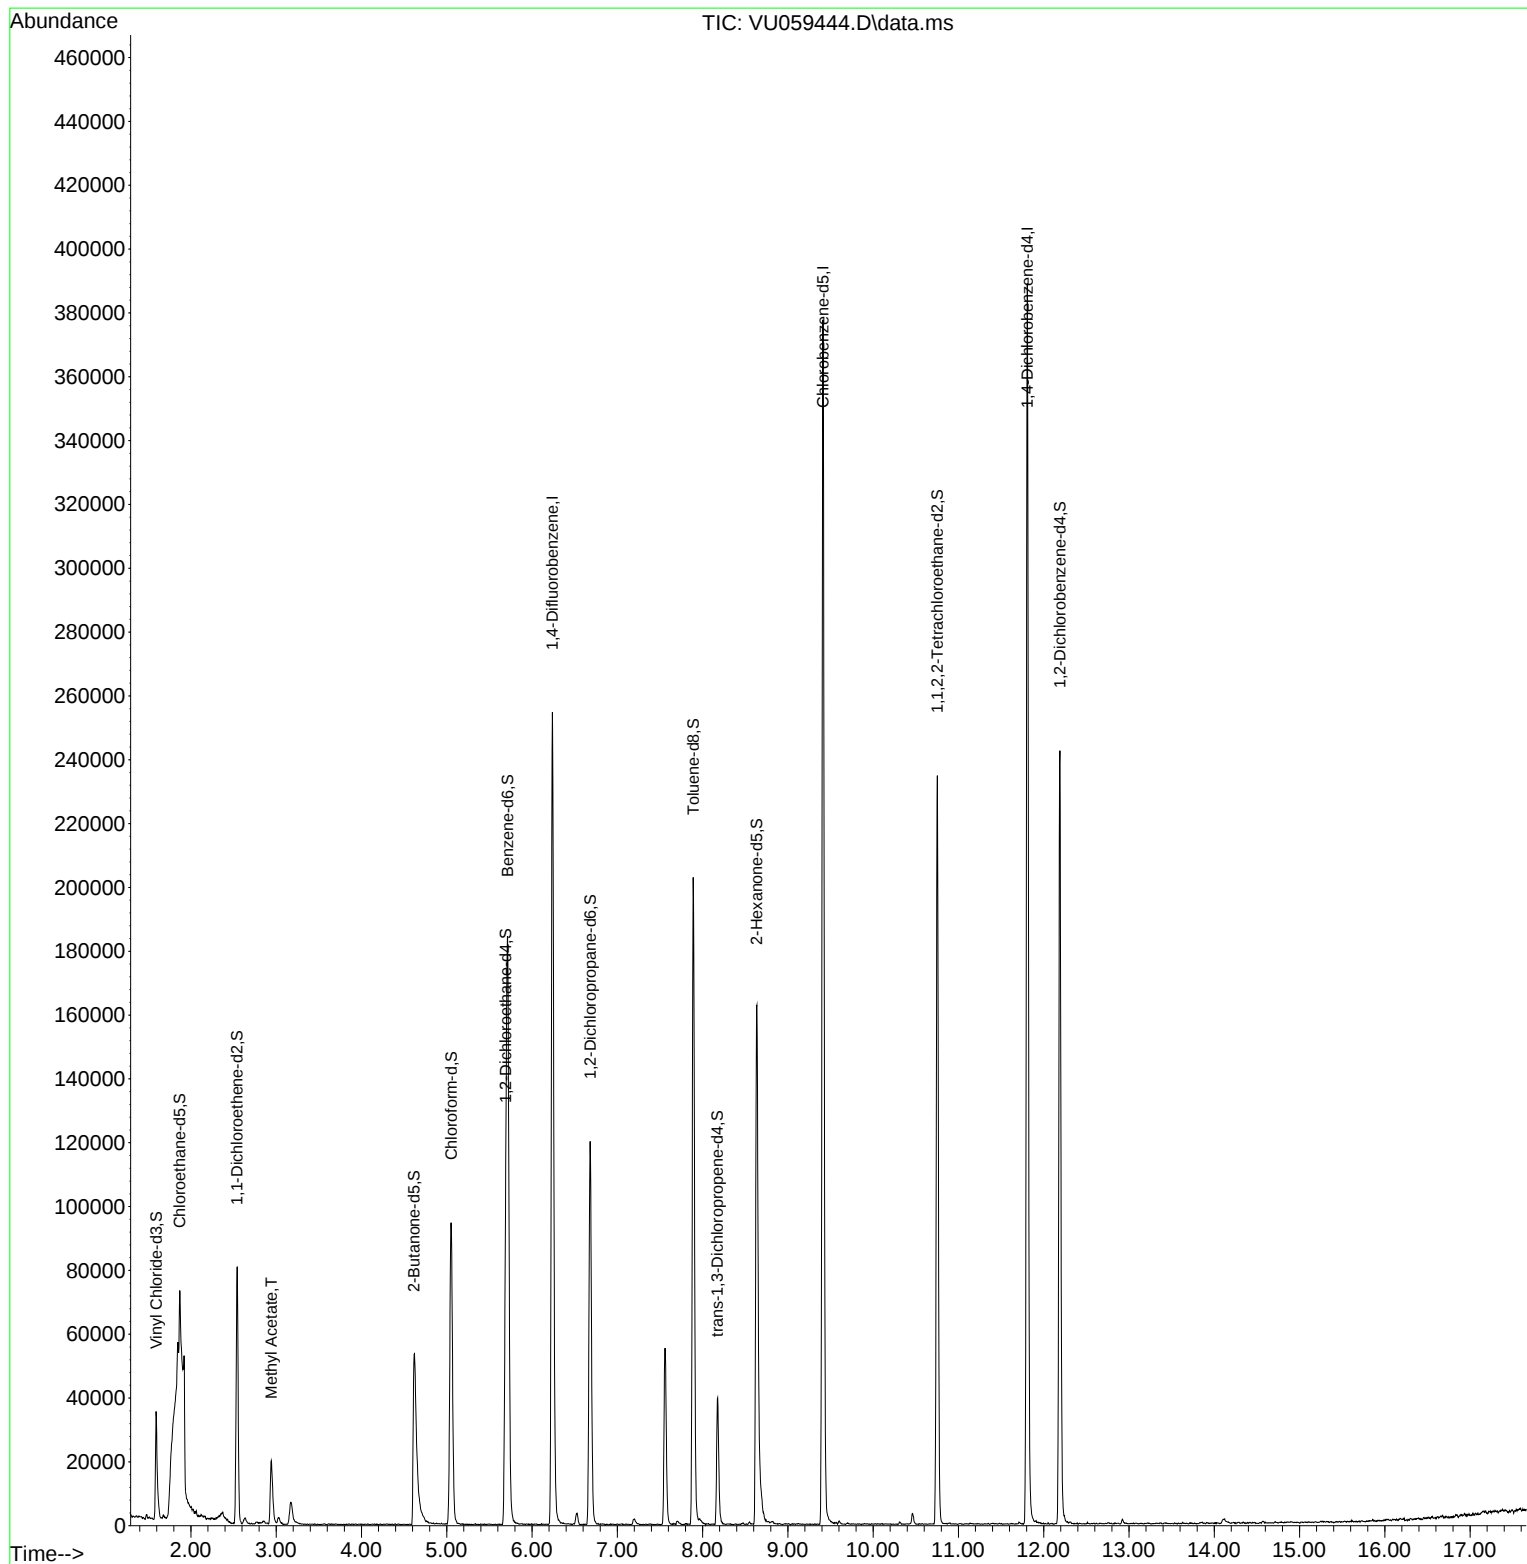

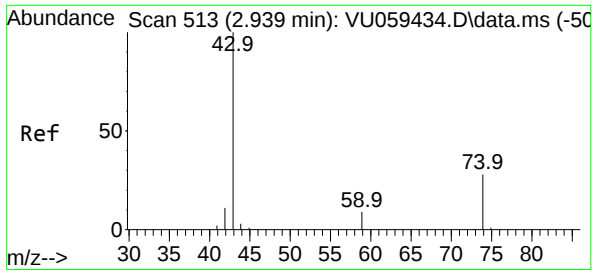

#15
Methyl Acetate
Concen: 11.288 ug/L
RT: 2.943 min Scan# 51
Delta R.T. 0.003 min
Lab File: VU059444.D
Acq: 24 Jun 2024 13:00

Instrument :
MSVOA_U
ClientSampleId :
A4B42ME

Tgt Ion: 43 Resp: 25359
Ion Ratio Lower Upper
43 100
74 28.9 20.8 31.2

