

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062424\
 Data File : VU059436.D
 Acq On : 24 Jun 2024 09:56
 Operator : MD/SY
 Sample : VU0624WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK084

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M

Title : VOC Analysis

Signal : TIC: VU059436.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	114	rBV	89208	105332	15.45%	1.923%
2	1.760	141	146	161	rVB3	3550	5768	0.85%	0.105%
3	1.907	184	192	208	rBV	69506	95410	13.99%	1.742%
4	2.560	383	395	411	rBV	136675	221212	32.45%	4.038%
5	2.785	457	465	474	rBV3	1155	1816	0.27%	0.033%
6	2.904	499	502	505	rBV	205	166	0.02%	0.003%
7	3.039	536	544	555	rVB4	1597	2787	0.41%	0.051%
8	3.171	581	585	588	rBV3	490	385	0.06%	0.007%
9	3.322	625	632	635	rBV2	233	287	0.04%	0.005%
10	3.341	635	638	640	rBV2	433	318	0.05%	0.006%
11	3.403	652	657	661	rVB	167	183	0.03%	0.003%
12	3.483	680	682	687	rVB2	307	249	0.04%	0.005%
13	3.512	687	691	693	rBV2	262	231	0.03%	0.004%
14	3.685	740	745	748	rBV	189	177	0.03%	0.003%
15	3.708	748	752	755	rBV	167	169	0.02%	0.003%
16	3.808	779	783	788	rBV2	195	207	0.03%	0.004%
17	3.949	823	827	833	rVB2	192	215	0.03%	0.004%
18	3.981	833	837	841	rBV	150	155	0.02%	0.003%
19	4.116	875	879	882	rBV2	311	214	0.03%	0.004%
20	4.615	1024	1034	1066	rBV	60768	154442	22.65%	2.819%
21	4.827	1098	1100	1102	rBV	296	182	0.03%	0.003%
22	4.853	1106	1108	1112	rVB3	300	167	0.02%	0.003%
23	4.923	1127	1130	1135	rVB2	261	187	0.03%	0.003%
24	4.984	1145	1149	1153	rBV2	242	196	0.03%	0.004%
25	5.055	1156	1171	1192	rBV	122162	271747	39.86%	4.960%
26	5.187	1210	1212	1217	rVB2	372	176	0.03%	0.003%
27	5.364	1264	1267	1273	rVV2	185	185	0.03%	0.003%
28	5.441	1285	1291	1298	rBV2	284	428	0.06%	0.008%
29	5.615	1342	1345	1349	rBV2	156	153	0.02%	0.003%
30	5.718	1357	1377	1415	rBV2	253364	681779	100.00%	12.444%
31	5.972	1453	1456	1462	rVV2	206	233	0.03%	0.004%
32	6.013	1465	1469	1473	rVB3	229	203	0.03%	0.004%
33	6.242	1527	1540	1572	rBV	252101	488371	71.63%	8.914%
34	6.438	1598	1601	1605	rVB3	340	235	0.03%	0.004%
35	6.473	1610	1612	1618	rVB3	337	342	0.05%	0.006%
36	6.528	1618	1629	1640	rBV7	4452	9380	1.38%	0.171%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062424\
 Data File : VU059436.D
 Acq On : 24 Jun 2024 09:56
 Operator : MD/SY
 Sample : VU0624WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK084

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

37	6.682	1661	1677	1704	rBV	154429	306012	44.88%	5.586%
38	6.856	1728	1731	1733	rBV	265	202	0.03%	0.004%
39	6.885	1737	1740	1744	rVB2	255	194	0.03%	0.004%
40	6.975	1763	1768	1775	rVB2	263	335	0.05%	0.006%
41	7.078	1796	1800	1805	rVB	314	287	0.04%	0.005%
42	7.110	1805	1810	1812	rBV2	354	154	0.02%	0.003%
43	7.158	1821	1825	1829	rBV2	176	182	0.03%	0.003%
44	7.206	1835	1840	1842	rBV2	350	303	0.04%	0.006%
45	7.299	1865	1869	1872	rBV	193	158	0.02%	0.003%
46	7.354	1880	1886	1892	rBV	112	159	0.02%	0.003%
47	7.441	1909	1913	1917	rBV	323	208	0.03%	0.004%
48	7.560	1937	1950	1977	rBV2	77983	144347	21.17%	2.635%
49	7.708	1993	1996	1998	rBV2	321	200	0.03%	0.004%
50	7.804	2019	2026	2027	rBV2	357	353	0.05%	0.006%
51	7.846	2035	2039	2041	rBV	302	267	0.04%	0.005%
52	7.891	2041	2053	2079	rBV	296776	522144	76.59%	9.531%
53	8.174	2130	2141	2166	rBV2	53647	96870	14.21%	1.768%
54	8.354	2193	2197	2201	rBV	182	196	0.03%	0.004%
55	8.550	2251	2258	2264	rVB4	942	1081	0.16%	0.020%
56	8.627	2272	2282	2315	rBV	159164	319390	46.85%	5.830%
57	8.859	2350	2354	2358	rVB	350	272	0.04%	0.005%
58	8.971	2387	2389	2393	rVV	285	159	0.02%	0.003%
59	8.994	2393	2396	2401	rVB2	188	181	0.03%	0.003%
60	9.094	2424	2427	2431	rVB2	302	224	0.03%	0.004%
61	9.135	2431	2440	2445	rBV2	332	675	0.10%	0.012%
62	9.283	2483	2486	2490	rBV2	271	239	0.04%	0.004%
63	9.309	2491	2494	2498	rVV2	197	161	0.02%	0.003%
64	9.412	2514	2526	2549	rBV	374883	628308	92.16%	11.468%
65	9.631	2590	2594	2596	rBV	274	207	0.03%	0.004%
66	10.055	2720	2726	2730	rBV2	199	242	0.04%	0.004%
67	10.094	2736	2738	2741	rBV	223	181	0.03%	0.003%
68	10.132	2747	2750	2753	rBV	198	163	0.02%	0.003%
69	10.303	2799	2803	2806	rBV2	242	234	0.03%	0.004%
70	10.479	2851	2858	2863	rBV3	387	549	0.08%	0.010%
71	10.547	2873	2879	2881	rBV2	223	226	0.03%	0.004%
72	10.749	2929	2942	2961	rBV	227107	372769	54.68%	6.804%
73	11.248	3090	3097	3100	rBV	244	301	0.04%	0.005%
74	11.331	3119	3123	3126	rBV2	243	212	0.03%	0.004%
75	11.470	3163	3166	3167	rBV3	383	258	0.04%	0.005%
76	11.479	3167	3169	3175	rVB4	586	524	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062424\
 Data File : VU059436.D
 Acq On : 24 Jun 2024 09:56
 Operator : MD/SY
 Sample : VU0624WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK084

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

77	11.634	3214	3217	3220	rBV2	196	156	0.02%	0.003%
78	11.688	3230	3234	3236	rBV2	263	205	0.03%	0.004%
79	11.753	3246	3254	3259	rBV2	1305	1635	0.24%	0.030%
80	11.807	3259	3271	3292	rBV	331243	549945	80.66%	10.038%
81	12.055	3346	3348	3355	rVB	253	225	0.03%	0.004%
82	12.135	3371	3373	3377	rBV	211	158	0.02%	0.003%
83	12.187	3377	3389	3412	rBV	277675	466497	68.42%	8.515%
84	12.354	3434	3441	3445	rBV3	422	543	0.08%	0.010%
85	12.431	3462	3465	3471	rBV2	245	215	0.03%	0.004%
86	12.486	3480	3482	3487	rVB2	268	162	0.02%	0.003%
87	12.582	3509	3512	3515	rBV2	345	246	0.04%	0.004%
88	12.717	3551	3554	3557	rBV	308	190	0.03%	0.003%
89	13.232	3708	3714	3723	rVV4	1130	1825	0.27%	0.033%
90	13.483	3789	3792	3795	rBV	237	155	0.02%	0.003%
91	13.685	3853	3855	3858	rVB	357	186	0.03%	0.003%
92	13.852	3899	3907	3916	rBV3	2014	3387	0.50%	0.062%
93	14.103	3976	3985	3998	rBV5	2956	5771	0.85%	0.105%
94	14.331	4050	4056	4059	rBV6	2056	2514	0.37%	0.046%
95	14.389	4072	4074	4078	rVB2	257	160	0.02%	0.003%
96	14.482	4101	4103	4106	rVB	281	156	0.02%	0.003%
97	14.502	4106	4109	4110	rBV2	287	170	0.02%	0.003%
98	14.605	4139	4141	4142	rBV2	385	155	0.02%	0.003%
99	16.187	4630	4633	4637	rBV2	728	622	0.09%	0.011%
100	16.634	4769	4772	4773	rBV2	731	476	0.07%	0.009%




Sum of corrected areas: 5478568

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062424\
Data File : VU059436.D
Acq On : 24 Jun 2024 09:56
Operator : MD/SY
Sample : VU0624WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK084

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

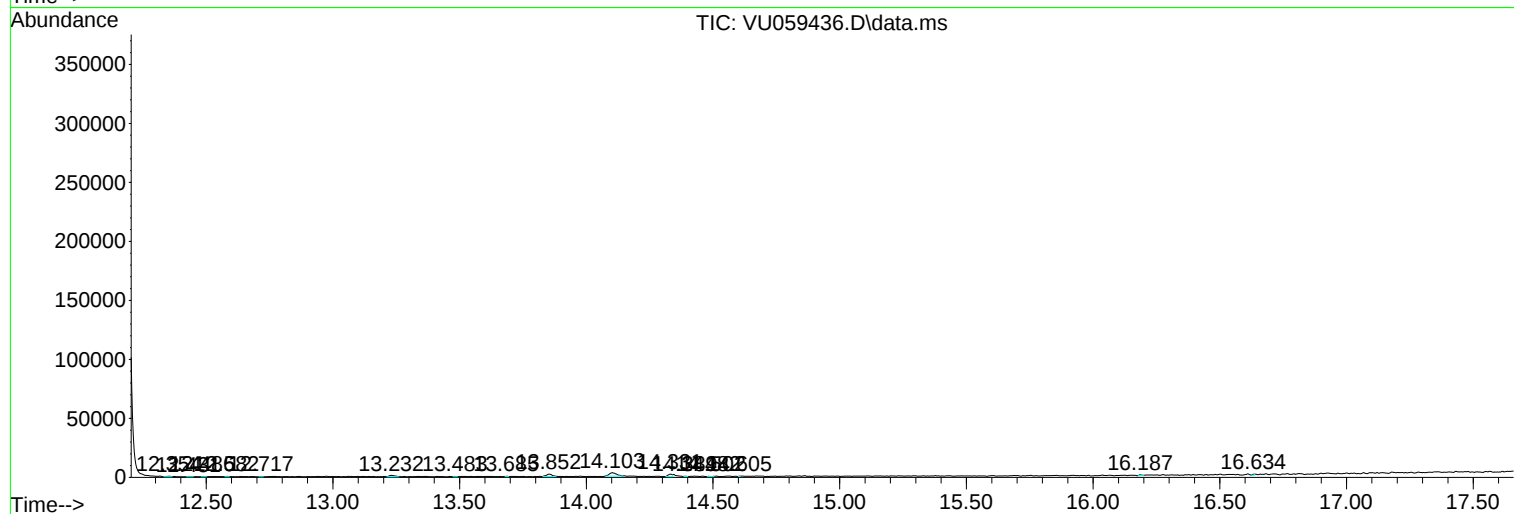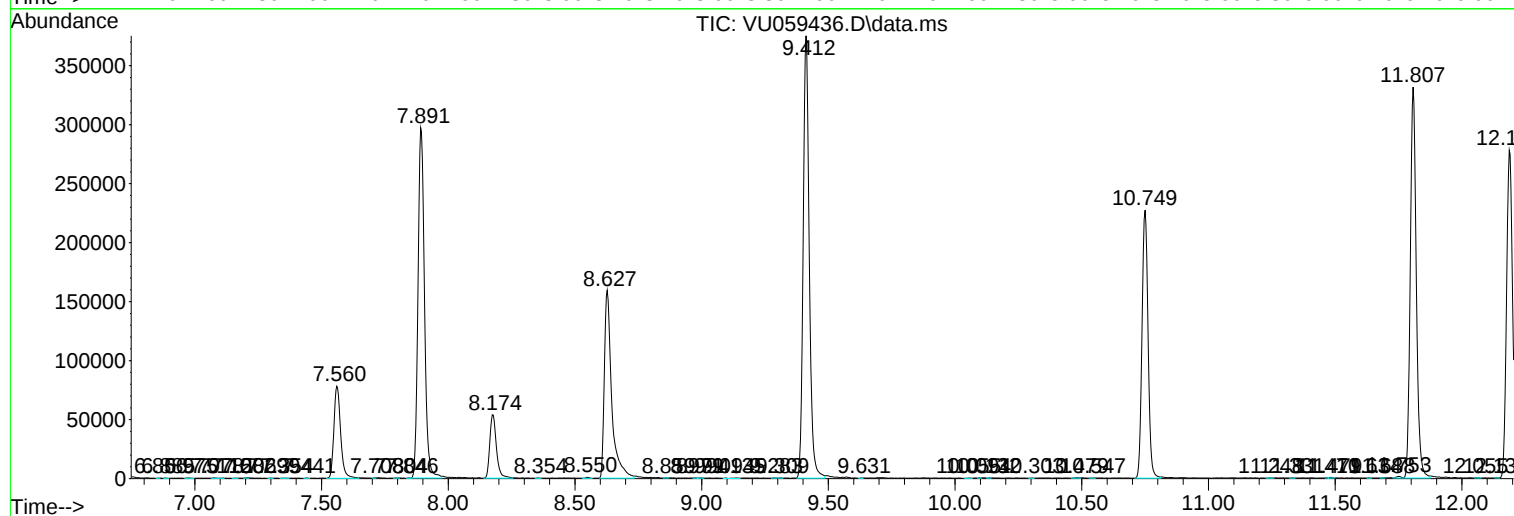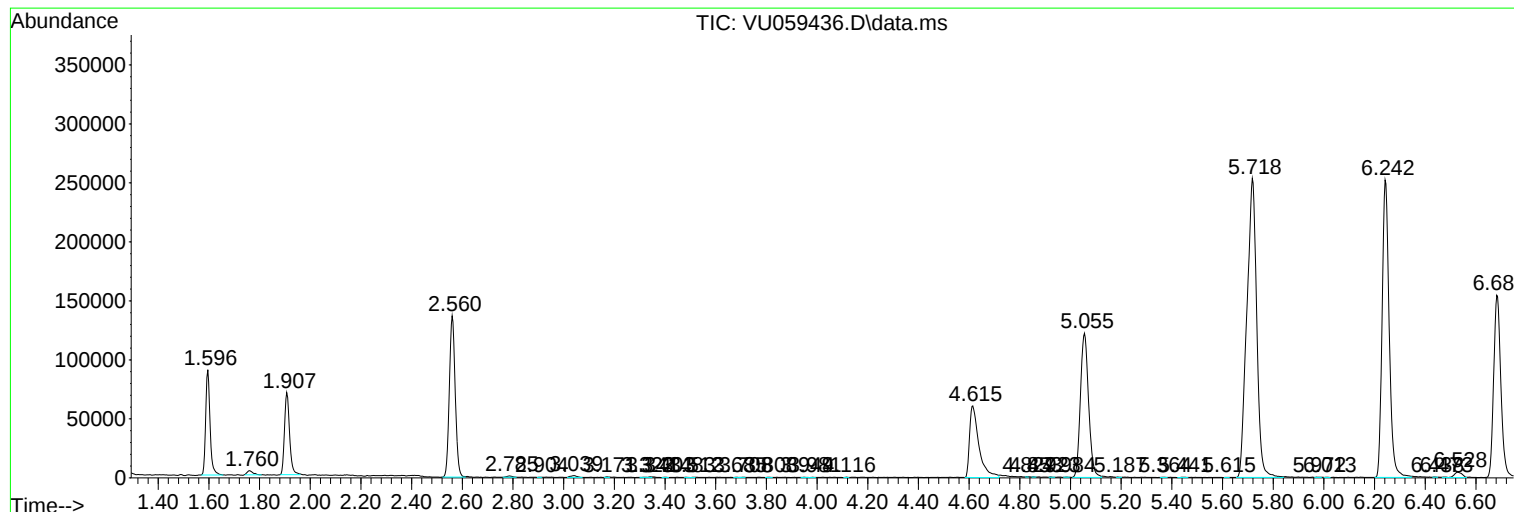

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062424\
Data File : VU059436.D
Acq On : 24 Jun 2024 09:56
Operator : MD/SY
Sample : VU0624WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK084

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062424\
Data File : VU059436.D
Acq On : 24 Jun 2024 09:56
Operator : MD/SY
Sample : VU0624WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK084

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc