

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062424\
 Data File : VU059437.D
 Acq On : 24 Jun 2024 10:19
 Operator : MD/SY
 Sample : P3017-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08C2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

Signal : TIC: VU059437.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.489	57	62	67	rVB2	2260	2220	0.35%	0.043%
2	1.596	85	95	108	rBV	56800	71174	11.18%	1.388%
3	1.679	118	121	131	rVB4	2383	2694	0.42%	0.053%
4	1.763	141	147	155	rVB3	4388	5932	0.93%	0.116%
5	1.907	184	192	206	rBV	54763	73679	11.58%	1.437%
6	2.560	383	395	408	rBV	94419	153883	24.18%	3.001%
7	2.621	408	414	432	rVB2	5163	8850	1.39%	0.173%
8	2.891	495	498	500	rBV2	302	206	0.03%	0.004%
9	2.930	507	510	513	rBV	323	257	0.04%	0.005%
10	2.997	528	531	536	rVB2	196	142	0.02%	0.003%
11	3.033	536	542	543	rBV3	951	911	0.14%	0.018%
12	3.171	575	585	586	rBV3	2729	3098	0.49%	0.060%
13	3.348	633	640	648	rBV5	910	1551	0.24%	0.030%
14	3.763	766	769	773	rBV2	177	152	0.02%	0.003%
15	3.898	808	811	813	rBV	202	127	0.02%	0.002%
16	3.956	826	829	833	rVB2	259	239	0.04%	0.005%
17	3.981	833	837	839	rBV2	321	286	0.04%	0.006%
18	4.087	867	870	875	rVB2	201	196	0.03%	0.004%
19	4.219	908	911	913	rBV2	219	184	0.03%	0.004%
20	4.309	936	939	942	rVB2	244	145	0.02%	0.003%
21	4.383	958	962	967	rBV2	132	149	0.02%	0.003%
22	4.435	967	978	988	rBV5	722	1752	0.28%	0.034%
23	4.480	988	992	996	rBV	204	160	0.03%	0.003%
24	4.611	1021	1033	1076	rBV2	71214	189410	29.76%	3.694%
25	4.865	1109	1112	1115	rBV	294	234	0.04%	0.005%
26	5.055	1156	1171	1202	rBV2	116027	287938	45.25%	5.616%
27	5.197	1212	1215	1217	rVB3	458	285	0.04%	0.006%
28	5.216	1218	1221	1222	rBV	264	126	0.02%	0.002%
29	5.393	1273	1276	1280	rVB2	203	162	0.03%	0.003%
30	5.428	1284	1287	1290	rVB	214	126	0.02%	0.002%
31	5.515	1310	1314	1317	rBV2	182	144	0.02%	0.003%
32	5.579	1332	1334	1341	rBV2	261	201	0.03%	0.004%
33	5.718	1357	1377	1400	rBV3	208502	575039	90.36%	11.216%
34	5.965	1450	1454	1456	rBV2	266	230	0.04%	0.004%
35	6.004	1462	1466	1470	rVB2	417	375	0.06%	0.007%
36	6.033	1470	1475	1482	rVB3	412	584	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062424\
 Data File : VU059437.D
 Acq On : 24 Jun 2024 10:19
 Operator : MD/SY
 Sample : P3017-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08C2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

37	6.071	1482	1487	1489	rBV	420	392	0.06%	0.008%
38	6.190	1519	1524	1526	rBV2	278	248	0.04%	0.005%
39	6.242	1527	1540	1562	rBV	256251	497739	78.22%	9.708%
40	6.531	1619	1630	1641	rVB5	5092	10078	1.58%	0.197%
41	6.631	1658	1661	1664	rVV2	211	157	0.02%	0.003%
42	6.685	1664	1678	1708	rVV2	138161	270481	42.50%	5.275%
43	6.795	1709	1712	1714	rBV2	341	212	0.03%	0.004%
44	6.859	1727	1732	1736	rBV2	243	258	0.04%	0.005%
45	7.103	1798	1808	1823	rBV5	3675	7821	1.23%	0.153%
46	7.193	1829	1836	1838	rBV2	1426	1637	0.26%	0.032%
47	7.303	1864	1870	1871	rBV	194	164	0.03%	0.003%
48	7.496	1927	1930	1933	rBV	197	148	0.02%	0.003%
49	7.560	1938	1950	1969	rBV	61850	114985	18.07%	2.243%
50	7.705	1989	1995	2000	rBV4	1042	1357	0.21%	0.026%
51	7.750	2007	2009	2012	rVB	302	179	0.03%	0.003%
52	7.785	2016	2020	2021	rBV2	185	128	0.02%	0.002%
53	7.808	2024	2027	2032	rVB2	305	280	0.04%	0.005%
54	7.846	2036	2039	2041	rBV2	231	149	0.02%	0.003%
55	7.894	2041	2054	2072	rBV	225546	397285	62.43%	7.749%
56	8.126	2123	2126	2129	rBV3	359	194	0.03%	0.004%
57	8.177	2131	2142	2164	rVV	43408	76476	12.02%	1.492%
58	8.287	2174	2176	2182	rVB3	403	349	0.05%	0.007%
59	8.316	2182	2185	2190	rBV2	173	145	0.02%	0.003%
60	8.467	2223	2232	2247	rVB4	2432	4157	0.65%	0.081%
61	8.544	2253	2256	2257	rBV	465	264	0.04%	0.005%
62	8.627	2272	2282	2312	rBV	175101	351565	55.25%	6.857%
63	8.788	2327	2332	2342	rVV8	2082	3480	0.55%	0.068%
64	8.840	2346	2348	2353	rVB2	295	161	0.03%	0.003%
65	8.975	2385	2390	2392	rBV2	251	232	0.04%	0.005%
66	9.132	2435	2439	2443	rVB2	202	164	0.03%	0.003%
67	9.155	2443	2446	2448	rBV2	234	151	0.02%	0.003%
68	9.232	2465	2470	2472	rBV2	170	162	0.03%	0.003%
69	9.412	2513	2526	2555	rBV	376168	636363	100.00%	12.412%
70	9.557	2568	2571	2572	rBV2	495	292	0.05%	0.006%
71	9.608	2585	2587	2589	rVB2	367	143	0.02%	0.003%
72	9.692	2606	2613	2624	rBV3	1942	3298	0.52%	0.064%
73	10.106	2734	2742	2745	rBV4	884	1103	0.17%	0.022%
74	10.248	2782	2786	2790	rBV	276	242	0.04%	0.005%
75	10.476	2855	2857	2858	rBV	250	135	0.02%	0.003%
76	10.750	2929	2942	2965	rBV	231484	377077	59.26%	7.355%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062424\
 Data File : VU059437.D
 Acq On : 24 Jun 2024 10:19
 Operator : MD/SY
 Sample : P3017-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08C2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

77	10.888	2977	2985	2996	rVB3	2882	4835	0.76%	0.094%
78	11.196	3078	3081	3084	rBV	193	149	0.02%	0.003%
79	11.296	3109	3112	3115	rBV2	233	167	0.03%	0.003%
80	11.409	3144	3147	3150	rBV2	239	164	0.03%	0.003%
81	11.428	3150	3153	3158	rBV2	184	175	0.03%	0.003%
82	11.486	3161	3171	3188	rBV5	4291	10814	1.70%	0.211%
83	11.743	3246	3251	3258	rBV3	1223	1678	0.26%	0.033%
84	11.807	3259	3271	3294	rBV	336491	552640	86.84%	10.779%
85	12.187	3377	3389	3409	rVV	239012	403227	63.36%	7.865%
86	12.341	3434	3437	3441	rBV2	256	180	0.03%	0.004%
87	12.364	3441	3444	3446	rBV	244	168	0.03%	0.003%
88	12.579	3509	3511	3516	rBV2	386	315	0.05%	0.006%
89	12.762	3563	3568	3569	rBV2	712	577	0.09%	0.011%
90	12.804	3578	3581	3589	rVB2	246	252	0.04%	0.005%
91	12.865	3593	3600	3605	rBV2	390	613	0.10%	0.012%
92	13.232	3708	3714	3717	rBV	819	797	0.13%	0.016%
93	13.701	3857	3860	3865	rBV2	256	289	0.05%	0.006%
94	13.849	3901	3906	3908	rBV2	1294	1259	0.20%	0.025%
95	13.917	3924	3927	3929	rBV2	177	141	0.02%	0.003%
96	14.103	3977	3985	3993	rBV3	2435	3380	0.53%	0.066%
97	14.290	4040	4043	4048	rBV2	435	437	0.07%	0.009%
98	14.335	4051	4057	4063	rVV4	1452	1685	0.26%	0.033%
99	14.502	4107	4109	4111	rBV	297	206	0.03%	0.004%
100	16.045	4587	4589	4594	rVB2	535	278	0.04%	0.005%




Sum of corrected areas: 5127118

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062424\
Data File : VU059437.D
Acq On : 24 Jun 2024 10:19
Operator : MD/SY
Sample : P3017-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08C2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

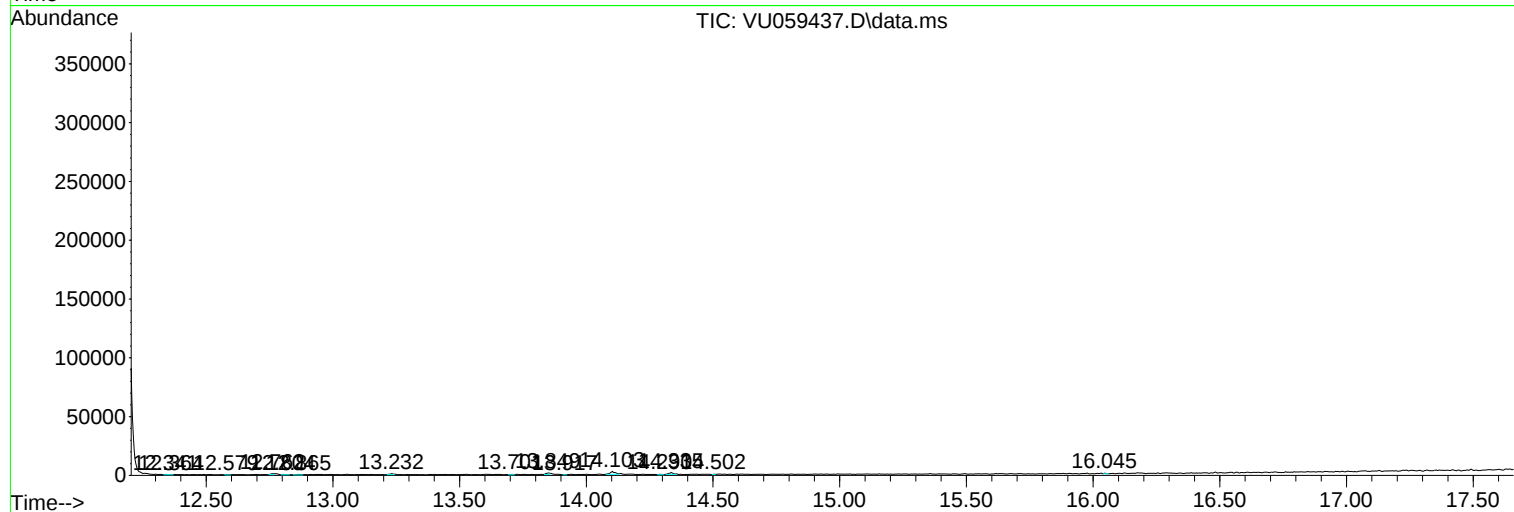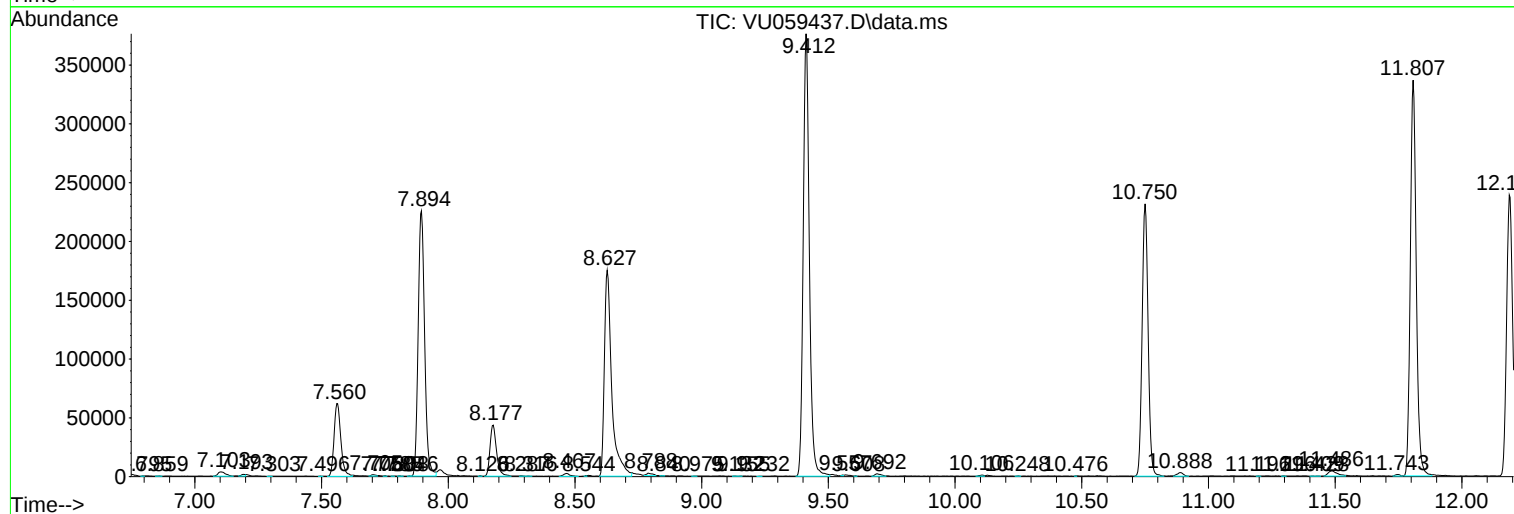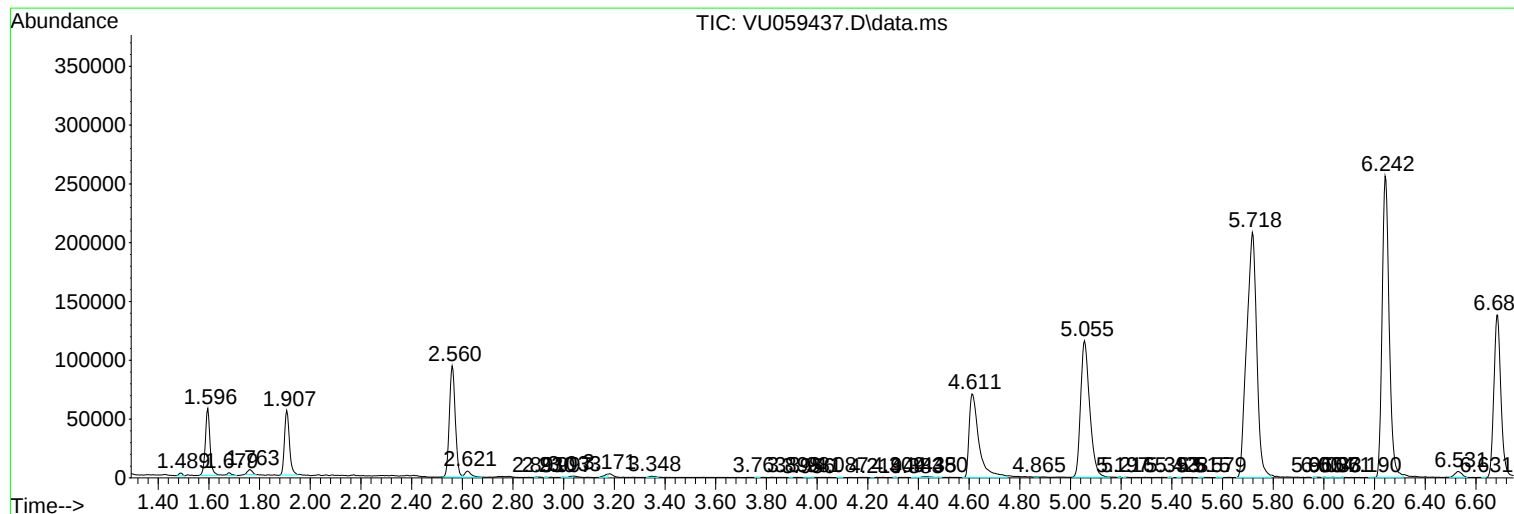

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062424\
Data File : VU059437.D
Acq On : 24 Jun 2024 10:19
Operator : MD/SY
Sample : P3017-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08C2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062424\
Data File : VU059437.D
Acq On : 24 Jun 2024 10:19
Operator : MD/SY
Sample : P3017-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08C2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------