

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062424\
 Data File : VU059438.D
 Acq On : 24 Jun 2024 10:42
 Operator : MD/SY
 Sample : P3037-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08C6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M

Title : VOC Analysis

Signal : TIC: VU059438.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.486	58	61	67	rVB2	1557	1368	0.22%	0.027%
2	1.596	85	95	109	rBV	55044	68344	11.01%	1.359%
3	1.760	140	146	160	rVB4	4510	7383	1.19%	0.147%
4	1.907	184	192	210	rVB	52972	73504	11.85%	1.462%
5	2.560	383	395	408	rBV	93255	151844	24.47%	3.019%
6	2.621	409	414	427	rVB	4736	6755	1.09%	0.134%
7	2.753	450	455	459	rVV	541	611	0.10%	0.012%
8	2.856	484	487	496	rVB2	188	199	0.03%	0.004%
9	2.901	497	501	504	rVB2	309	224	0.04%	0.004%
10	3.036	534	543	553	rBV3	1111	2177	0.35%	0.043%
11	3.178	574	587	602	rBV5	2162	5282	0.85%	0.105%
12	3.348	634	640	649	rVV5	953	1402	0.23%	0.028%
13	3.438	665	668	672	rVB	311	259	0.04%	0.005%
14	3.473	672	679	682	rBV2	282	350	0.06%	0.007%
15	3.570	706	709	713	rVV	245	192	0.03%	0.004%
16	3.631	720	728	733	rBV2	400	661	0.11%	0.013%
17	3.872	800	803	807	rVV	272	199	0.03%	0.004%
18	4.020	846	849	854	rVB	197	163	0.03%	0.003%
19	4.059	855	861	867	rBV2	244	308	0.05%	0.006%
20	4.200	901	905	908	rBV2	219	184	0.03%	0.004%
21	4.219	908	911	913	rVV2	247	175	0.03%	0.003%
22	4.425	971	975	986	rVB4	544	962	0.16%	0.019%
23	4.612	1023	1033	1061	rBV	69168	173933	28.03%	3.459%
24	5.055	1155	1171	1200	rBV3	111339	282383	45.51%	5.615%
25	5.354	1260	1264	1266	rBV2	288	243	0.04%	0.005%
26	5.579	1330	1334	1338	rVB2	227	182	0.03%	0.004%
27	5.718	1356	1377	1410	rBV2	200684	568014	91.54%	11.295%
28	5.914	1435	1438	1442	rBV2	251	160	0.03%	0.003%
29	5.981	1455	1459	1460	rVB2	267	160	0.03%	0.003%
30	6.001	1460	1465	1468	rBV2	330	306	0.05%	0.006%
31	6.052	1478	1481	1482	rBV	372	211	0.03%	0.004%
32	6.116	1498	1501	1507	rVB	256	191	0.03%	0.004%
33	6.242	1527	1540	1563	rBV	247600	481749	77.64%	9.579%
34	6.380	1581	1583	1586	rVB3	369	175	0.03%	0.003%
35	6.492	1614	1618	1620	rBV3	214	203	0.03%	0.004%
36	6.528	1620	1629	1641	rVV5	4403	9129	1.47%	0.182%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062424\
 Data File : VU059438.D
 Acq On : 24 Jun 2024 10:42
 Operator : MD/SY
 Sample : P3037-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08C6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

37	6.611	1651	1655	1658	rBV2	245	175	0.03%	0.003%
38	6.682	1664	1677	1700	rBV	136430	267359	43.09%	5.316%
39	6.782	1706	1708	1711	rVB	300	180	0.03%	0.004%
40	6.804	1712	1715	1719	rVB2	553	349	0.06%	0.007%
41	6.872	1729	1736	1737	rBV2	149	168	0.03%	0.003%
42	7.100	1798	1807	1816	rBV6	3428	7232	1.17%	0.144%
43	7.193	1830	1836	1845	rVV6	1444	2611	0.42%	0.052%
44	7.309	1867	1872	1878	rBV	219	242	0.04%	0.005%
45	7.373	1888	1892	1897	rBV2	159	170	0.03%	0.003%
46	7.431	1905	1910	1914	rBV2	187	165	0.03%	0.003%
47	7.560	1938	1950	1975	rBV2	62486	114797	18.50%	2.283%
48	7.701	1989	1994	1995	rBV2	1037	709	0.11%	0.014%
49	7.891	2041	2053	2071	rBV	220061	390813	62.98%	7.771%
50	8.174	2130	2141	2157	rBV	43814	75501	12.17%	1.501%
51	8.470	2224	2233	2240	rBV2	1438	1997	0.32%	0.040%
52	8.550	2254	2258	2265	rVB3	560	571	0.09%	0.011%
53	8.627	2272	2282	2317	rBV	168815	346955	55.92%	6.899%
54	8.791	2327	2333	2346	rVB9	2664	4511	0.73%	0.090%
55	9.264	2476	2480	2484	rBV2	274	238	0.04%	0.005%
56	9.412	2514	2526	2552	rBV	368351	620490	100.00%	12.338%
57	9.563	2571	2573	2575	rBV2	406	215	0.03%	0.004%
58	9.605	2583	2586	2589	rBV	274	197	0.03%	0.004%
59	9.624	2590	2592	2596	rVV2	261	166	0.03%	0.003%
60	9.692	2607	2613	2614	rBV	1631	1251	0.20%	0.025%
61	9.846	2657	2661	2665	rVV	318	269	0.04%	0.005%
62	9.894	2672	2676	2679	rVB	376	309	0.05%	0.006%
63	9.917	2679	2683	2690	rBV2	424	656	0.11%	0.013%
64	10.023	2714	2716	2724	rVB2	236	222	0.04%	0.004%
65	10.100	2734	2740	2747	rBV4	733	1055	0.17%	0.021%
66	10.467	2849	2854	2857	rBV	276	222	0.04%	0.004%
67	10.489	2857	2861	2862	rVV2	267	222	0.04%	0.004%
68	10.515	2866	2869	2872	rVV2	268	230	0.04%	0.005%
69	10.550	2876	2880	2882	rBV2	195	167	0.03%	0.003%
70	10.563	2882	2884	2889	rVV	293	260	0.04%	0.005%
71	10.586	2889	2891	2896	rVB	216	176	0.03%	0.003%
72	10.750	2929	2942	2963	rBV	232013	375570	60.53%	7.468%
73	10.843	2969	2971	2974	rVB2	393	215	0.03%	0.004%
74	10.888	2977	2985	2993	rVV3	3046	3408	0.55%	0.068%
75	11.010	3019	3023	3025	rBV2	257	190	0.03%	0.004%
76	11.049	3031	3035	3041	rVB	253	237	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062424\
 Data File : VU059438.D
 Acq On : 24 Jun 2024 10:42
 Operator : MD/SY
 Sample : P3037-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08C6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

77	11.100	3041	3051	3053	rBV3	450	537	0.09%	0.011%
78	11.232	3087	3092	3095	rBV	272	262	0.04%	0.005%
79	11.486	3160	3171	3191	rBV4	5167	11988	1.93%	0.238%
80	11.756	3246	3255	3259	rBV3	629	842	0.14%	0.017%
81	11.807	3259	3271	3298	rBV	325463	544766	87.80%	10.833%
82	11.955	3315	3317	3320	rVB	357	195	0.03%	0.004%
83	12.077	3352	3355	3359	rBV2	205	189	0.03%	0.004%
84	12.097	3359	3361	3364	rVV	389	229	0.04%	0.005%
85	12.116	3364	3367	3371	rVB2	270	203	0.03%	0.004%
86	12.187	3376	3389	3415	rBV	236611	401812	64.76%	7.990%
87	12.309	3424	3427	3431	rBV2	412	323	0.05%	0.006%
88	12.611	3518	3521	3526	rBV2	238	217	0.03%	0.004%
89	12.766	3564	3569	3577	rVB3	1210	1471	0.24%	0.029%
90	12.933	3617	3621	3625	rVB2	520	380	0.06%	0.008%
91	13.219	3707	3710	3712	rBV	493	293	0.05%	0.006%
92	13.235	3712	3715	3717	rVB2	583	329	0.05%	0.007%
93	13.595	3824	3827	3832	rVB2	261	175	0.03%	0.003%
94	13.846	3902	3905	3907	rBV2	747	482	0.08%	0.010%
95	13.897	3918	3921	3924	rBV2	457	370	0.06%	0.007%
96	14.106	3980	3986	3995	rBV4	1289	2173	0.35%	0.043%
97	14.331	4051	4056	4057	rBV2	746	560	0.09%	0.011%
98	14.704	4169	4172	4174	rBV2	401	262	0.04%	0.005%
99	14.955	4245	4250	4253	rBV3	392	447	0.07%	0.009%
100	15.119	4296	4301	4304	rBV2	363	425	0.07%	0.008%




Sum of corrected areas: 5028985

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062424\
Data File : VU059438.D
Acq On : 24 Jun 2024 10:42
Operator : MD/SY
Sample : P3037-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08C6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

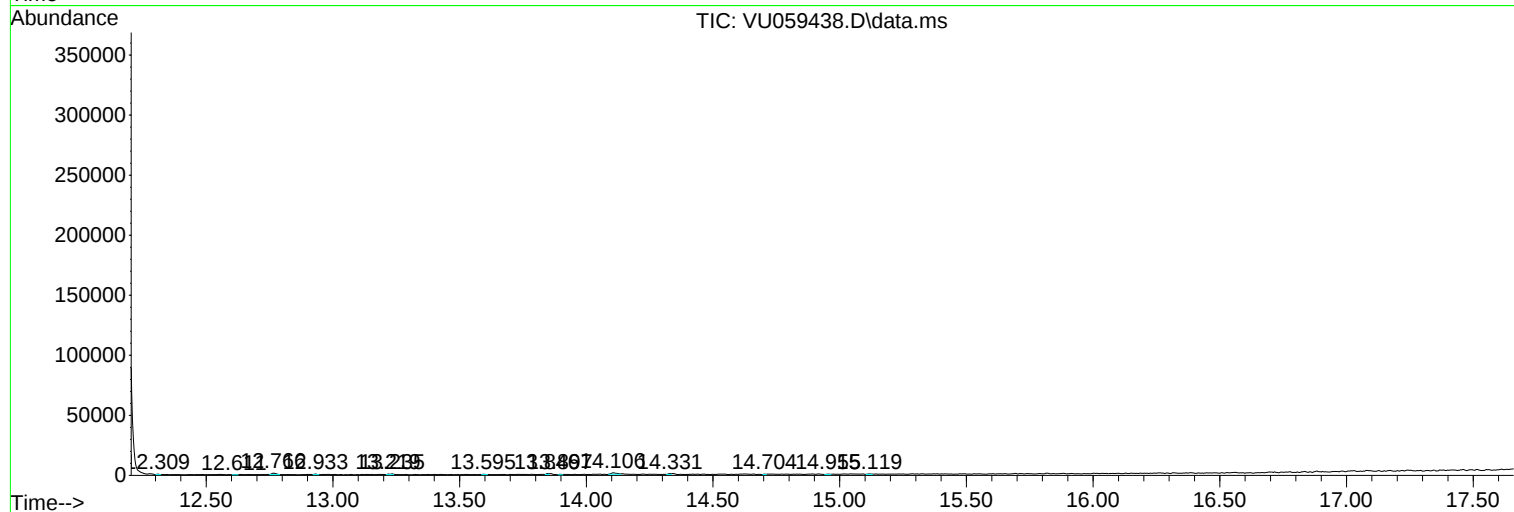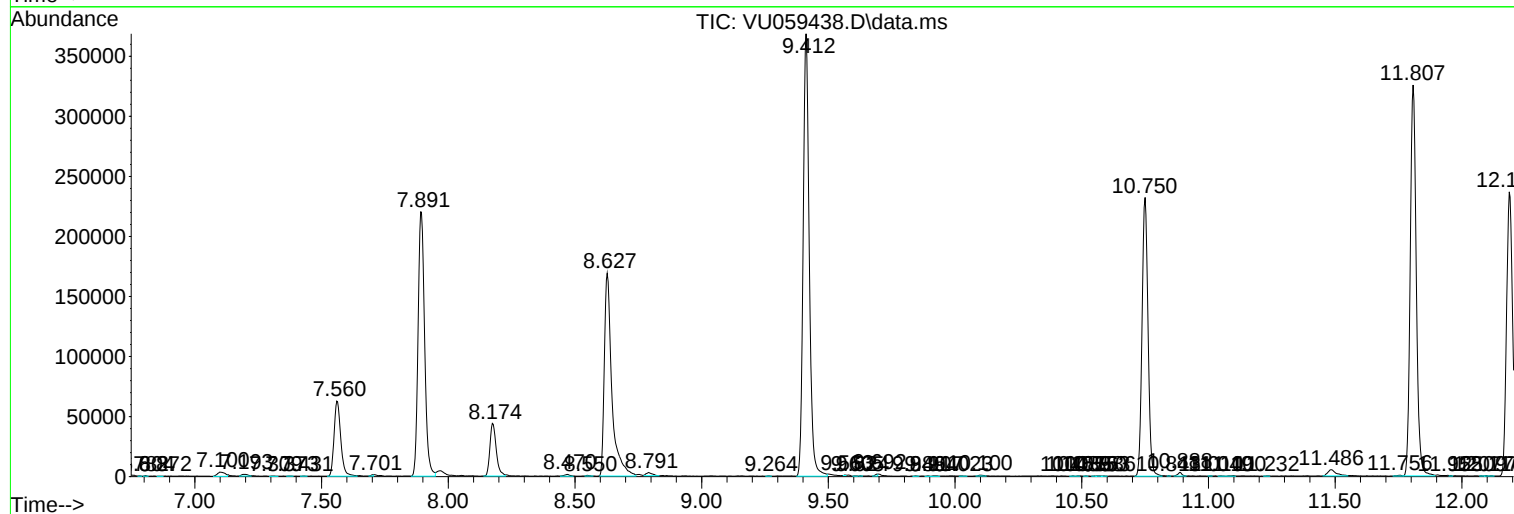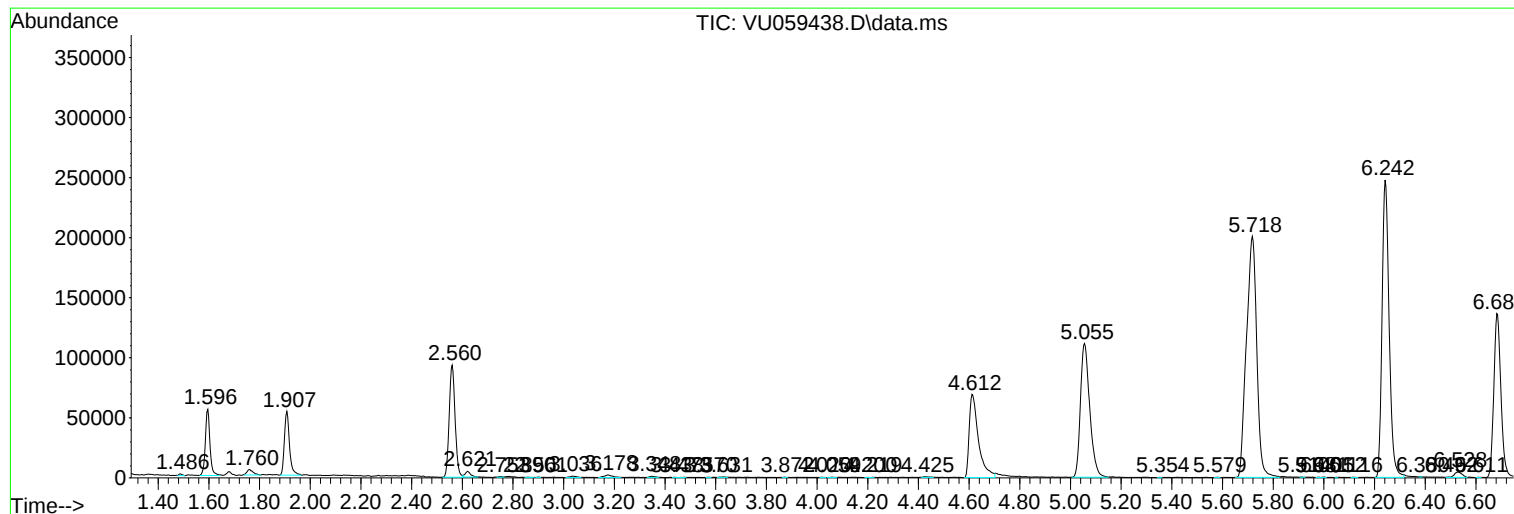

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062424\
Data File : VU059438.D
Acq On : 24 Jun 2024 10:42
Operator : MD/SY
Sample : P3037-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08C6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062424\
Data File : VU059438.D
Acq On : 24 Jun 2024 10:42
Operator : MD/SY
Sample : P3037-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08C6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------