

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062424\
 Data File : VU059454.D
 Acq On : 24 Jun 2024 16:50
 Operator : MD/SY
 Sample : P3037-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M

Title : VOC Analysis

Signal : TIC: VU059454.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.592	87	94	109	rBV	97319	116114	14.84%	1.778%
2	1.895	181	188	213	rVB	70619	104347	13.33%	1.598%
3	2.554	382	393	411	rBV	153477	253027	32.34%	3.875%
4	3.158	577	581	582	rBV2	661	475	0.06%	0.007%
5	3.274	613	617	620	rBV	186	176	0.02%	0.003%
6	3.338	635	637	643	rBV3	457	435	0.06%	0.007%
7	3.689	743	746	749	rBV	222	169	0.02%	0.003%
8	3.975	832	835	838	rBV	246	210	0.03%	0.003%
9	4.087	867	870	871	rBV	108	66	0.01%	0.001%
10	4.158	889	892	898	rVB2	281	287	0.04%	0.004%
11	4.187	898	901	904	rBV2	141	93	0.01%	0.001%
12	4.206	904	907	913	rBV	240	260	0.03%	0.004%
13	4.370	955	958	962	rBV2	156	116	0.01%	0.002%
14	4.390	962	964	966	rVB	227	60	0.01%	0.001%
15	4.464	984	987	993	rBV	216	252	0.03%	0.004%
16	4.612	1015	1033	1065	rBV	76895	191710	24.50%	2.936%
17	5.052	1154	1170	1191	rBV	136612	301788	38.57%	4.622%
18	5.293	1241	1245	1249	rBV2	489	373	0.05%	0.006%
19	5.313	1249	1251	1255	rVB2	372	204	0.03%	0.003%
20	5.364	1266	1267	1270	rVB	167	90	0.01%	0.001%
21	5.380	1270	1272	1278	rBV3	218	185	0.02%	0.003%
22	5.422	1284	1285	1286	rVB	125	24	0.00%	0.000%
23	5.435	1286	1289	1292	rVB	186	125	0.02%	0.002%
24	5.454	1292	1295	1298	rBV2	129	113	0.01%	0.002%
25	5.531	1315	1319	1324	rBV2	304	277	0.04%	0.004%
26	5.573	1328	1332	1335	rBV	112	96	0.01%	0.001%
27	5.592	1335	1338	1342	rBV2	171	168	0.02%	0.003%
28	5.644	1351	1354	1356	rBV	189	131	0.02%	0.002%
29	5.718	1356	1377	1410	rVV2	285636	782506	100.00%	11.984%
30	6.039	1474	1477	1478	rBV	259	126	0.02%	0.002%
31	6.100	1494	1496	1498	rBV	98	48	0.01%	0.001%
32	6.116	1498	1501	1502	rBV	206	121	0.02%	0.002%
33	6.242	1525	1540	1558	rBV	286448	543739	69.49%	8.327%
34	6.402	1586	1590	1593	rBV3	342	338	0.04%	0.005%
35	6.496	1617	1619	1620	rBV2	191	59	0.01%	0.001%
36	6.531	1620	1630	1641	rVB9	4182	8320	1.06%	0.127%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062424\
 Data File : VU059454.D
 Acq On : 24 Jun 2024 16:50
 Operator : MD/SY
 Sample : P3037-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

37	6.605	1650	1653	1656	rVB2	195	115	0.01%	0.002%
38	6.621	1656	1658	1660	rBV	233	93	0.01%	0.001%
39	6.640	1660	1664	1665	rBV2	348	174	0.02%	0.003%
40	6.682	1665	1677	1702	rBV	172530	342979	43.83%	5.253%
41	6.891	1738	1742	1745	rBV2	183	141	0.02%	0.002%
42	7.033	1782	1786	1790	rBV	253	214	0.03%	0.003%
43	7.068	1794	1797	1799	rBV2	183	119	0.02%	0.002%
44	7.107	1804	1809	1813	rBV	316	391	0.05%	0.006%
45	7.174	1828	1830	1831	rBV	138	55	0.01%	0.001%
46	7.435	1908	1911	1920	rBV2	163	263	0.03%	0.004%
47	7.560	1938	1950	1968	rBV	90381	161093	20.59%	2.467%
48	7.801	2019	2025	2029	rBV4	621	673	0.09%	0.010%
49	7.843	2034	2038	2040	rBV	202	158	0.02%	0.002%
50	7.891	2040	2053	2072	rBV	350654	608068	77.71%	9.312%
51	8.174	2131	2141	2160	rBV	61714	105467	13.48%	1.615%
52	8.348	2192	2195	2197	rBV	194	114	0.01%	0.002%
53	8.399	2209	2211	2215	rVB	287	156	0.02%	0.002%
54	8.454	2226	2228	2231	rBV3	259	201	0.03%	0.003%
55	8.554	2254	2259	2265	rVB4	1037	1169	0.15%	0.018%
56	8.627	2271	2282	2319	rBV	204844	392885	50.21%	6.017%
57	8.949	2380	2382	2384	rBV2	146	46	0.01%	0.001%
58	8.959	2384	2385	2386	rVB	185	36	0.00%	0.001%
59	9.023	2403	2405	2407	rBV2	147	43	0.01%	0.001%
60	9.039	2407	2410	2412	rBV	199	134	0.02%	0.002%
61	9.222	2464	2467	2475	rBV2	197	224	0.03%	0.003%
62	9.412	2514	2526	2554	rBV	411225	686924	87.79%	10.520%
63	9.698	2607	2615	2624	rBV5	1746	3074	0.39%	0.047%
64	9.843	2657	2660	2663	rBV	191	156	0.02%	0.002%
65	10.004	2707	2710	2715	rBV2	185	196	0.03%	0.003%
66	10.180	2762	2765	2767	rBV2	240	130	0.02%	0.002%
67	10.193	2767	2769	2772	rBV	143	98	0.01%	0.002%
68	10.264	2788	2791	2793	rBV	211	136	0.02%	0.002%
69	10.316	2805	2807	2813	rBV	239	159	0.02%	0.002%
70	10.750	2930	2942	2960	rBV	259165	418066	53.43%	6.402%
71	11.746	3248	3252	3259	rBV2	791	723	0.09%	0.011%
72	11.807	3259	3271	3294	rBV	385459	625495	79.93%	9.579%
73	12.187	3376	3389	3417	rBV	327824	545775	69.75%	8.358%
74	13.843	3902	3904	3906	rBV	616	394	0.05%	0.006%
75	14.087	3969	3980	4001	rBV	64345	116023	14.83%	1.777%
76	15.219	4322	4332	4356	rBV	70551	120135	15.35%	1.840%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062424\
Data File : VU059454.D
Acq On : 24 Jun 2024 16:50
Operator : MD/SY
Sample : P3037-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Title : VOC Analysis

77	15.409	4382	4391	4410	rVB	28592	48403	6.19%	0.741%
78	15.952	4553	4560	4571	rBV	13136	19871	2.54%	0.304%
79	16.261	4649	4656	4664	rBV3	14240	22398	2.86%	0.343%




Sum of corrected areas: 6529795

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062424\
Data File : VU059454.D
Acq On : 24 Jun 2024 16:50
Operator : MD/SY
Sample : P3037-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

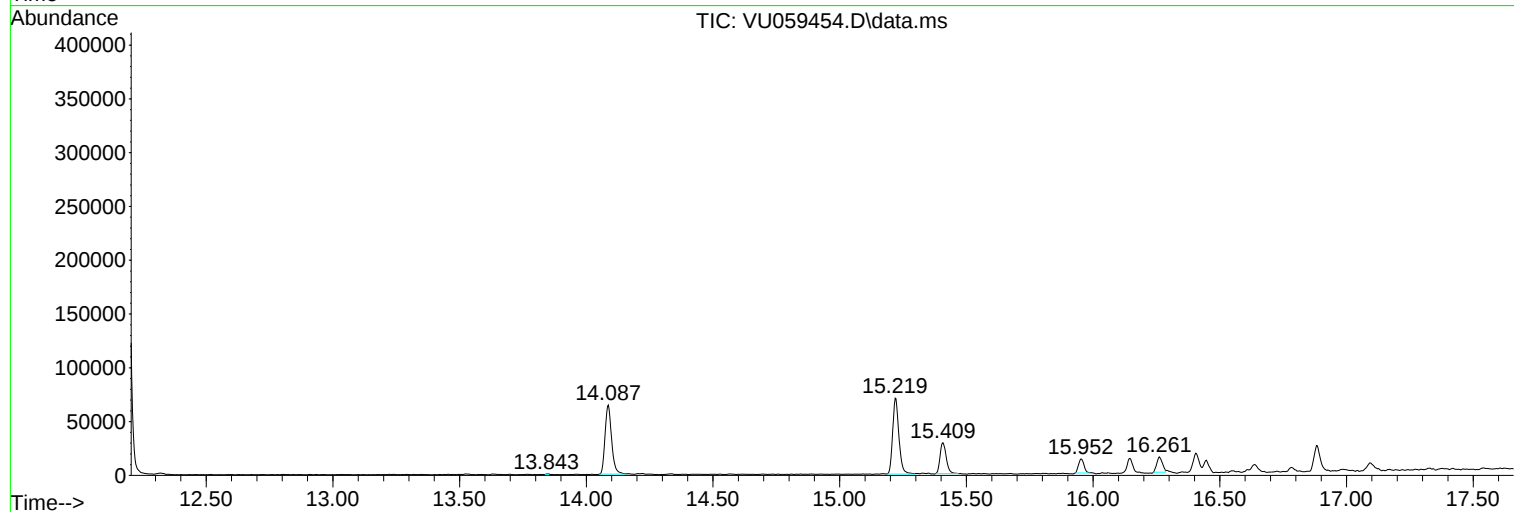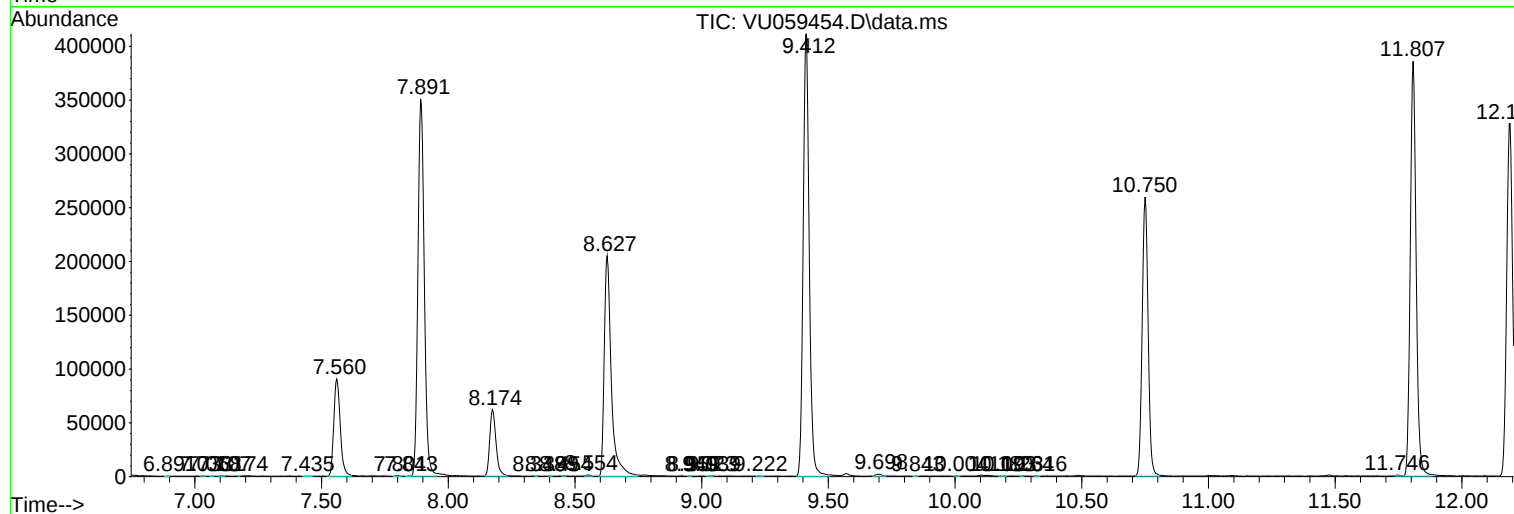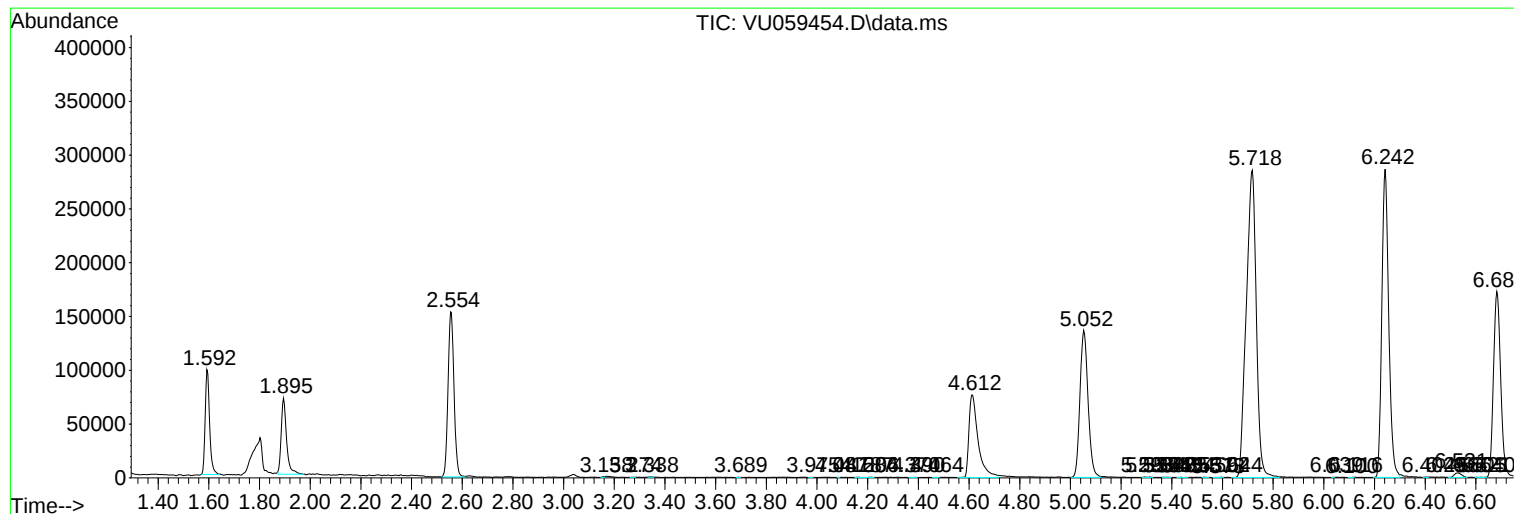

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062424\
Data File : VU059454.D
Acq On : 24 Jun 2024 16:50
Operator : MD/SY
Sample : P3037-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062424\
Data File : VU059454.D
Acq On : 24 Jun 2024 16:50
Operator : MD/SY
Sample : P3037-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------