


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062424\
Data File : VU059433.D
Acq On : 24 Jun 2024 07:50
Operator : MD/SY
Sample : BFB067
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB067

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Title : VOC Analysis
Last Update : Thu Jun 27 04:10:00 2024

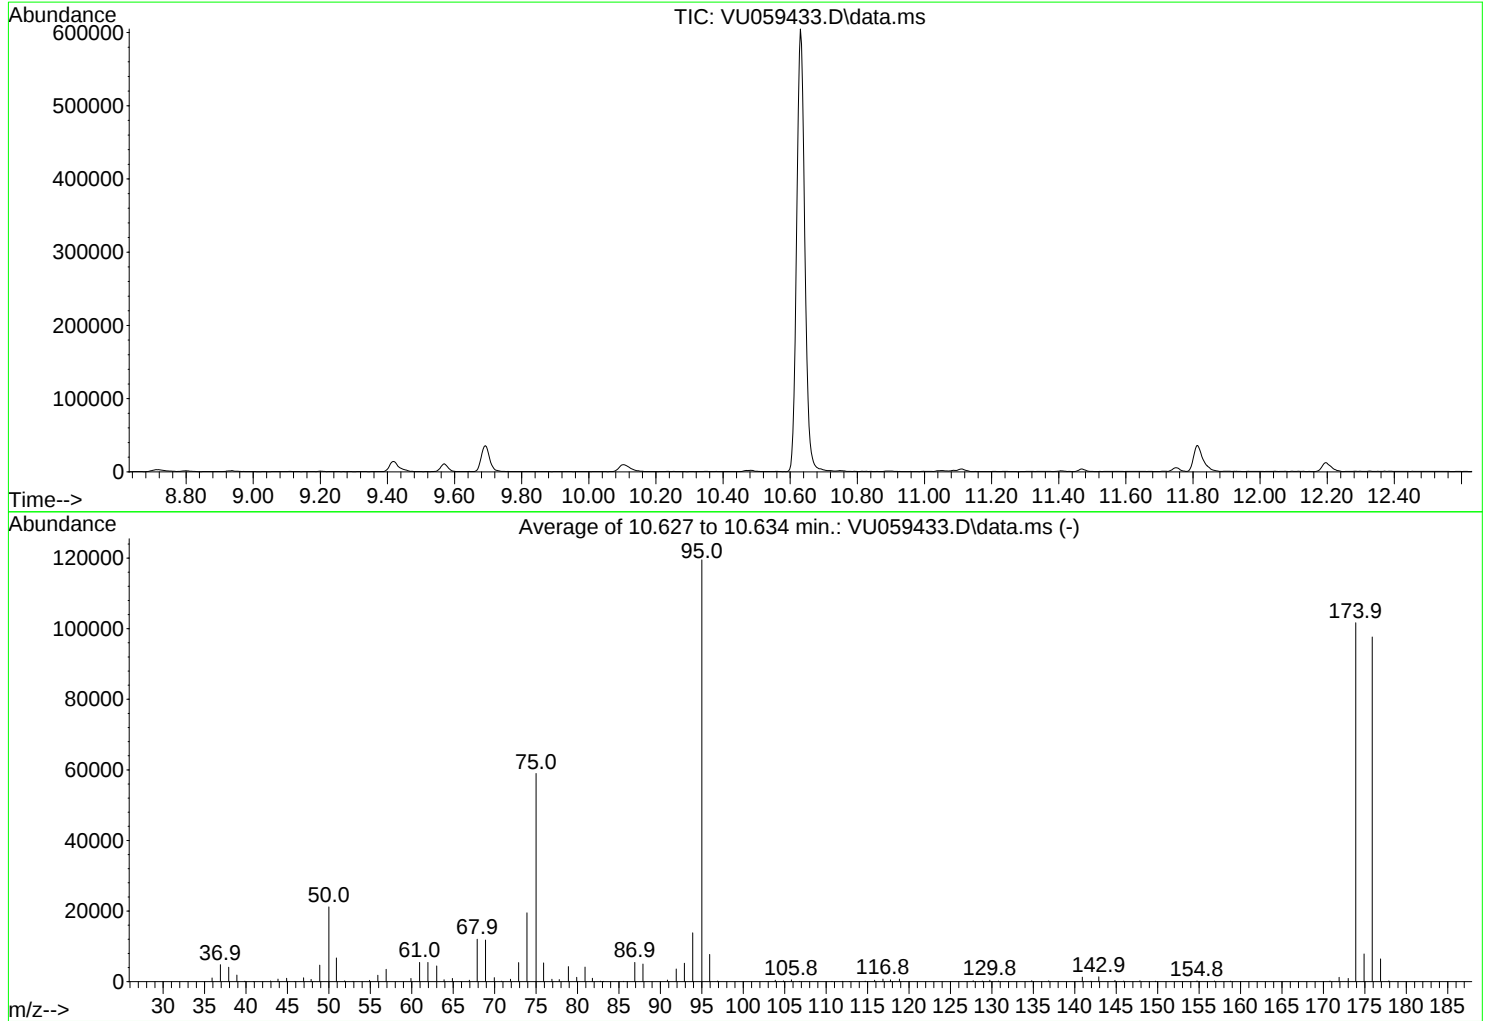

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2892

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	21192	PASS
75	95	30	80	49.4	58997	PASS
95	95	100	100	100.0	119509	PASS
96	95	5	9	6.4	7701	PASS
173	174	0.00	2	0.9	889	PASS
174	95	50	120	85.1	101699	PASS
175	174	5	9	7.7	7844	PASS
176	174	95	101	96.0	97653	PASS
177	176	5	9	6.6	6432	PASS

m/z	Abundance
39.90	129.0
43.80	208.0

Instrument :
MSVOA_U
ClientSampleId :
BFB067

m/z	Abundance
35.90	1025.0
36.90	4692.0
37.90	3991.0
38.90	2063.0
40.00	242.0
40.90	111.0
42.90	216.0
43.90	894.0
44.90	957.0
45.90	162.0
46.90	1101.0
47.80	770.0
48.90	4526.0
50.00	20640.0
50.90	6658.0
51.90	278.0
52.90	120.0
54.90	376.0
55.90	1792.0
56.90	3340.0
59.90	888.0
60.90	5165.0
61.90	5194.0
63.00	4340.0
63.90	604.0
64.90	958.0
65.90	110.0
67.00	414.0
67.90	11778.0
68.90	11565.0
69.90	1262.0
70.80	170.0
71.90	704.0
72.90	5688.0
73.90	19336.0
75.00	58432.0
75.90	5146.0
76.90	683.0
77.80	499.0
78.90	4142.0
79.90	1044.0
80.90	4176.0
81.80	928.0
82.80	113.0
86.90	5245.0
87.90	4968.0
90.80	506.0
91.90	3400.0
92.90	5049.0
93.90	13552.0
95.00	116520.0
96.00	7878.0
96.90	219.0
103.80	368.0
104.80	172.0
105.80	491.0
112.00	121.0
112.80	115.0
114.80	105.0
115.80	400.0
116.80	775.0
117.80	509.0
118.80	739.0
127.80	285.0
128.90	194.0
129.70	380.0
130.80	175.0
134.80	256.0
136.80	195.0
140.90	1201.0
141.90	123.0
142.90	1292.0
144.80	428.0
145.90	183.0
147.90	230.0
149.70	137.0
154.80	205.0
156.80	187.0
158.80	114.0
170.80	192.0
171.90	1151.0
173.00	1288.0
173.90	97888.0
174.90	7681.0
175.90	93200.0
176.90	6104.0
177.90	199.0

Instrument :
MSVOA_U
ClientSampleId :
BFB067

m/z	Abundance
35.90	1098.0
36.90	4944.0
37.90	4176.0
38.90	1898.0
39.80	261.0
43.00	205.0
43.90	971.0
44.90	996.0
45.90	120.0
47.00	1079.0
47.90	637.0
48.90	4784.0
50.00	21984.0
50.90	7020.0
51.90	238.0
52.90	112.0
54.90	381.0
55.90	1915.0
56.90	3632.0
59.90	911.0
60.90	5588.0
61.90	5637.0
63.00	4549.0
63.90	560.0
64.90	940.0
66.90	421.0
67.90	12418.0
68.90	12039.0
70.00	1186.0
70.80	163.0
71.90	735.0
72.90	5577.0
73.90	20128.0
75.00	60856.0
75.90	5448.0
76.90	684.0
77.80	593.0
78.90	4412.0
79.90	1280.0
80.90	4305.0
81.80	997.0
82.80	126.0
83.10	126.0
85.50	119.0
86.90	5586.0
87.90	5105.0
90.80	490.0
91.90	3787.0
92.90	5445.0
93.90	14117.0
95.00	123160.0
96.00	7845.0
96.90	203.0
103.80	404.0
104.80	214.0
105.80	488.0
106.80	112.0
110.70	119.0
111.90	111.0
114.70	136.0
115.90	422.0
116.90	737.0
117.70	507.0
118.80	741.0
127.80	304.0
128.80	185.0
129.80	422.0
130.80	178.0
134.80	291.0
136.90	233.0
140.90	1335.0
141.90	146.0
142.90	1383.0
144.80	394.0
145.90	199.0
147.90	258.0
149.80	130.0
154.80	243.0
156.90	202.0
158.80	129.0
170.80	199.0
171.90	1303.0
173.00	1379.0
173.90	104656.0
174.90	8141.0
175.90	100184.0
176.90	6656.0
177.90	211.0

Instrument :
MSVOA_U
ClientSampleId :
BFB067

m/z	Abundance
35.90	1048.0
36.90	4789.0
37.90	4020.0
38.90	1618.0
39.80	285.0
43.00	186.0
43.90	939.0
44.90	914.0
47.00	1064.0
47.90	528.0
48.90	4665.0
50.00	20952.0
50.90	6488.0
51.90	221.0
52.90	104.0
54.90	359.0
55.90	1803.0
56.90	3522.0
59.90	954.0
61.00	5614.0
62.00	5544.0
63.00	4412.0
63.90	537.0
64.90	806.0
66.90	365.0
67.90	11798.0
68.90	11723.0
69.90	988.0
70.80	111.0
71.90	665.0
72.90	4967.0
73.90	19048.0
75.00	57704.0
75.90	5351.0
76.90	670.0
77.80	653.0
78.90	4259.0
79.90	1342.0
80.90	3971.0
81.80	924.0
82.80	111.0
83.10	115.0
85.60	121.0
86.00	159.0
86.90	5542.0
87.90	4830.0
90.90	412.0
91.90	3598.0
92.90	5194.0
93.90	13811.0
95.00	118848.0
95.90	7380.0
96.90	183.0
103.90	408.0
104.90	243.0
105.80	469.0
106.80	128.0
110.70	125.0
114.60	151.0
115.90	435.0
116.90	682.0
117.70	449.0
118.90	691.0
127.70	308.0
128.80	185.0
129.80	423.0
130.80	166.0
134.80	289.0
136.90	234.0
140.90	1300.0
142.00	179.0
142.90	1425.0
144.90	322.0
145.90	202.0
147.80	305.0
149.80	130.0
154.70	274.0
156.90	204.0
158.80	112.0
170.80	188.0
171.90	1188.0
173.90	102552.0
174.90	7711.0
175.90	99576.0
176.90	6536.0
177.90	244.0

Instrument :
MSVOA_U
ClientSampleId :
BFB067