




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062524\
Data File : VU059470.D
Acq On : 25 Jun 2024 14:42
Operator : MD/SY
Sample : P2961-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GC5

Manual IntegrationsAPPROVED

Quant Time: Jun 26 04:29:50 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 26 04:26:20 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/26/2024
Supervised By :Semsettin Yesilyurt 06/26/2024

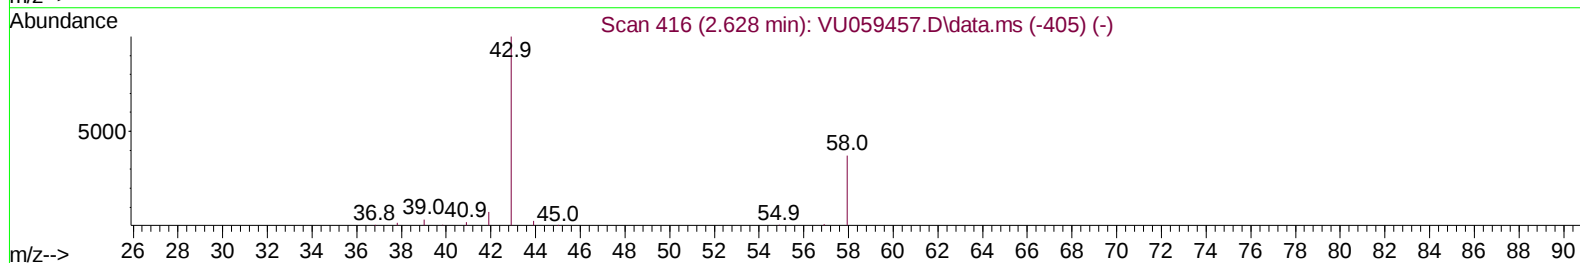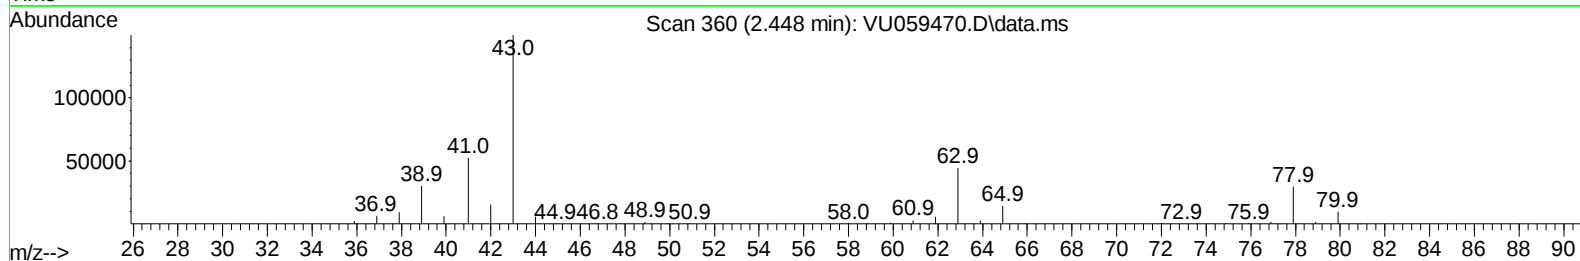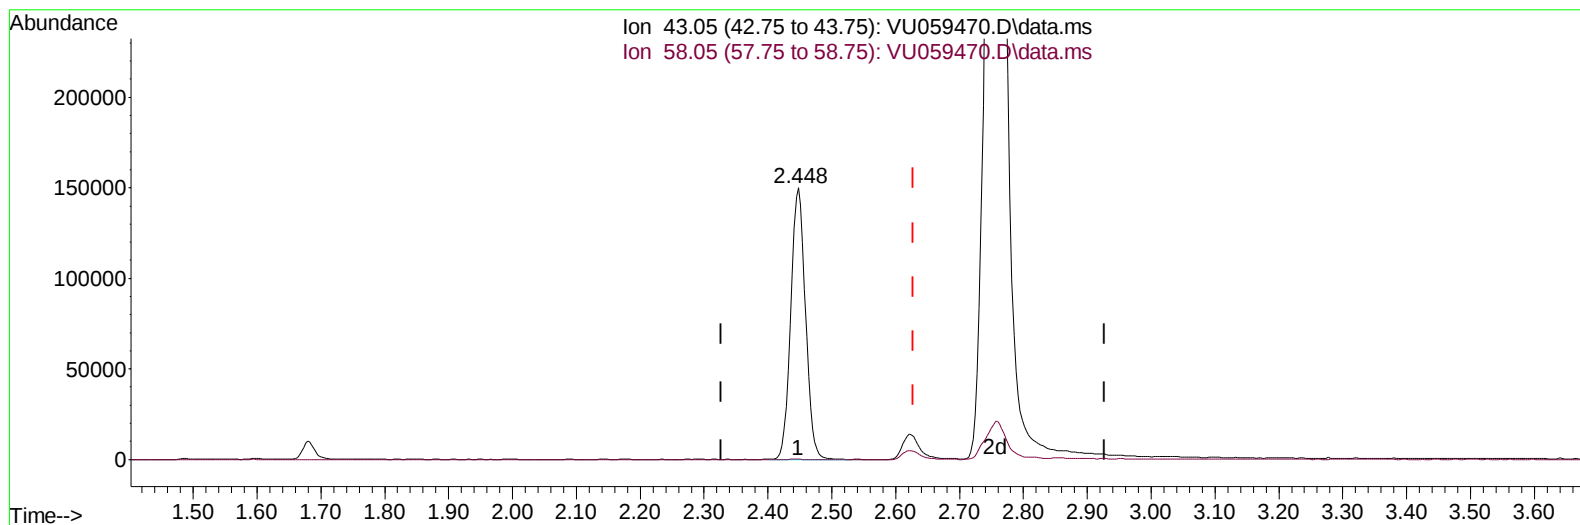

TIC: VU059470.D\data.ms

(13) Acetone (T)

2.448min (-0.180) 188.36 ug/L

response 240422

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	4.03
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062524\
Data File : VU059470.D
Acq On : 25 Jun 2024 14:42
Operator : MD/SY
Sample : P2961-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GC5

Manual IntegrationsAPPROVED

Quant Time: Jun 26 04:29:50 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 26 04:26:20 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/26/2024
Supervised By :Semsettin Yesilyurt 06/26/2024

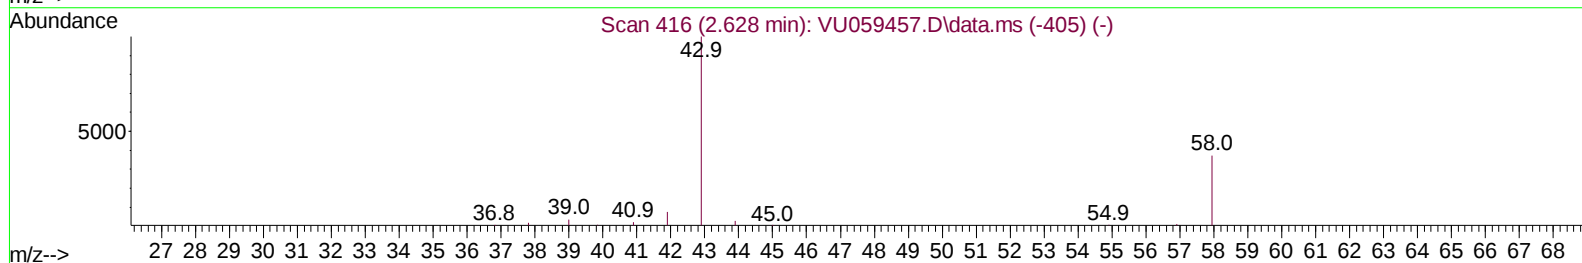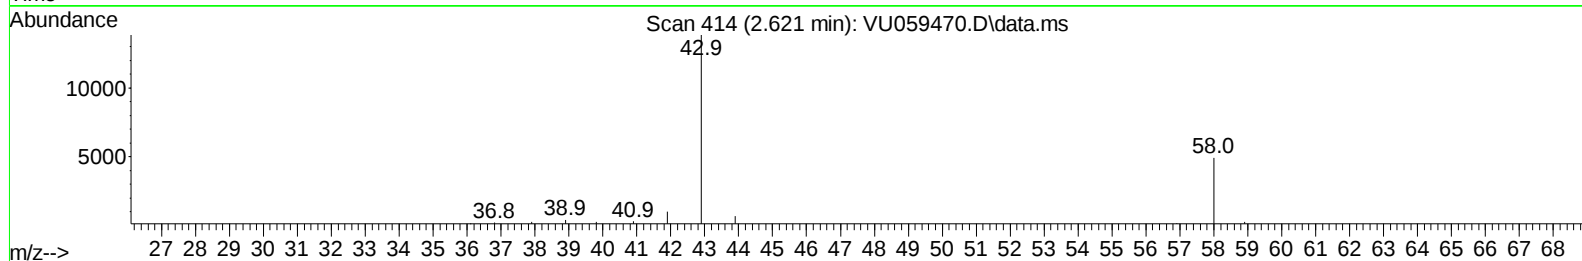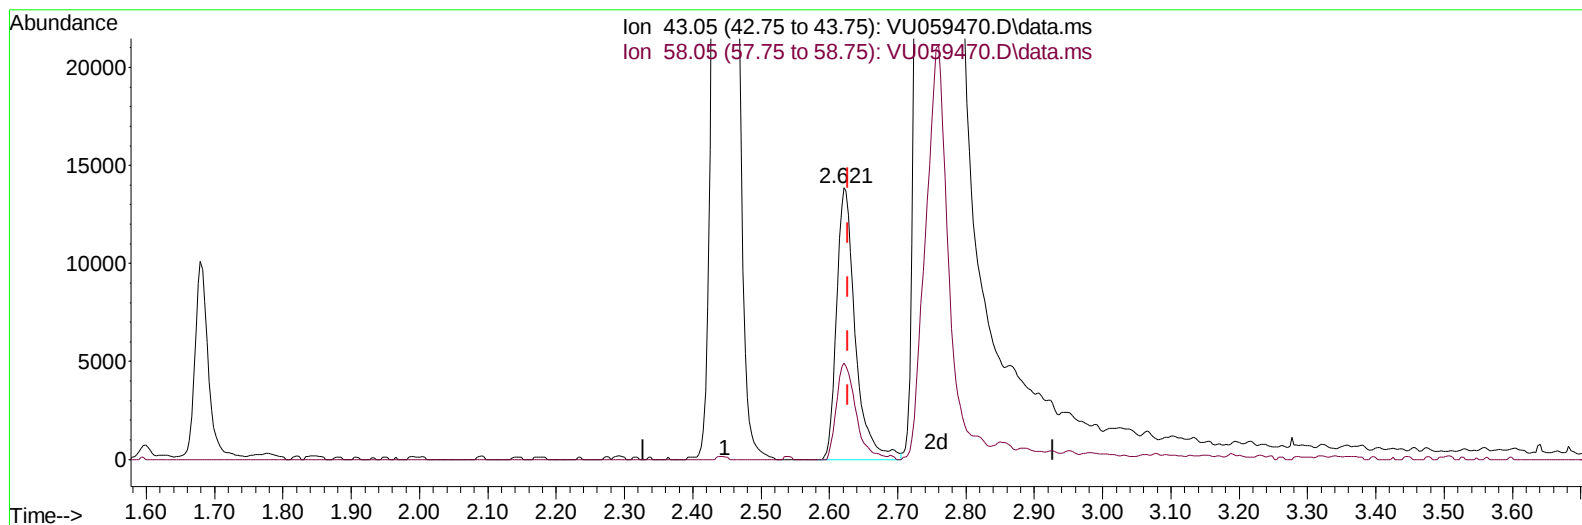

TIC: VU059470.D\data.ms

(13) Acetone (T)

2.621min (-0.006) 20.68 ug/L m

response 26399

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	36.69
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062524\
 Data File : VU059470.D
 Acq On : 25 Jun 2024 14:42
 Operator : MD/SY
 Sample : P2961-13
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GC5

Manual IntegrationsAPPROVED

Quant Time: Jun 26 04:29:50 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 26 04:26:20 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/26/2024
 Supervised By :Semsettin Yesilyurt 06/26/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.245	114		137377	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		141983	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		63439	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.596	65		29117	3.048	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	61.000%	
7) Chloroethane-d5	1.907	69		35429	3.855	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	77.000%	
11) 1,1-Dichloroethene-d2	2.560	65		11792	2.975	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	59.600%#	
20) 2-Butanone-d5	4.615	46		139514	70.903	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	141.800%#	
24) Chloroform-d	5.058	84		88579	4.518	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.400%	
26) 1,2-Dichloroethane-d4	5.695	65		47936	5.075	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.600%	
32) Benzene-d6	5.721	84		150744	3.858	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	77.200%	
36) 1,2-Dichloropropane-d6	6.682	67		56256	4.698	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.000%	
41) Toluene-d8	7.894	98		114623	3.155	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	63.200%#	
43) trans-1,3-Dichloroprop...	8.177	79		16351	4.361	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.200%	
46) 2-Hexanone-d5	8.627	63		98038	62.930	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	125.860%	
56) 1,1,2,2-Tetrachloroeth...	10.750	84		58451	5.908	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	118.200%	
66) 1,2-Dichlorobenzene-d4	12.190	152		59748	5.292	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.800%	
Target Compounds							
13) Acetone	2.621	43		26399m	20.682	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062524\
Data File : VU059470.D
Acq On : 25 Jun 2024 14:42
Operator : MD/SY
Sample : P2961-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GC5

Manual IntegrationsAPPROVED

Quant Time: Jun 26 04:29:50 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 26 04:26:20 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/26/2024
Supervised By :Semsettin Yesilyurt 06/26/2024

