




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062524\
Data File : VU059471.D
Acq On : 25 Jun 2024 15:06
Operator : MD/SY
Sample : P2961-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GC6

Manual IntegrationsAPPROVED

Quant Time: Jun 26 04:30:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 26 04:26:20 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/26/2024
Supervised By :Semsettin Yesilyurt 06/26/2024

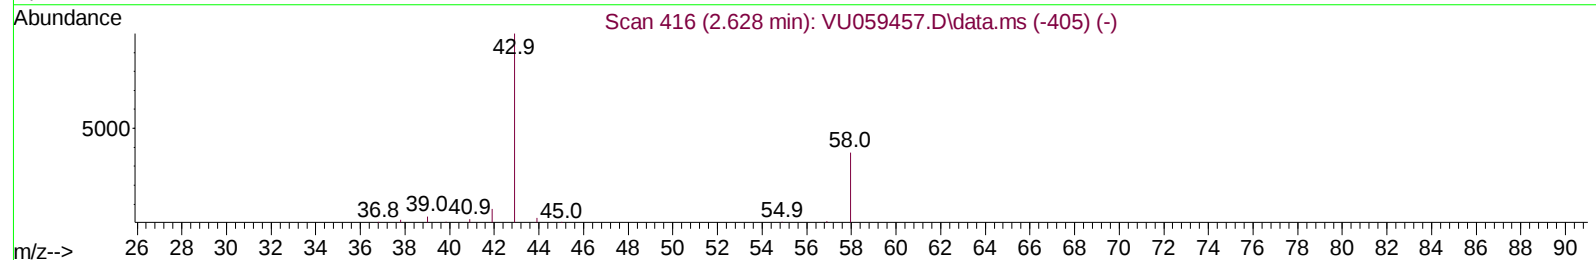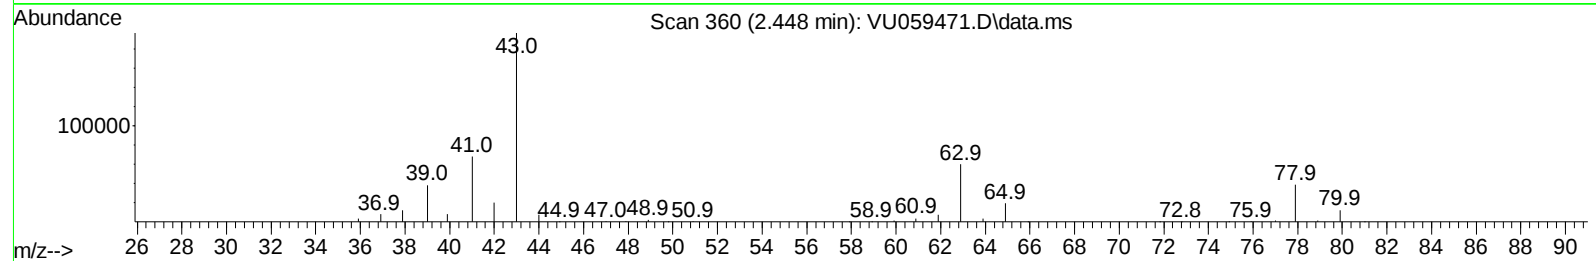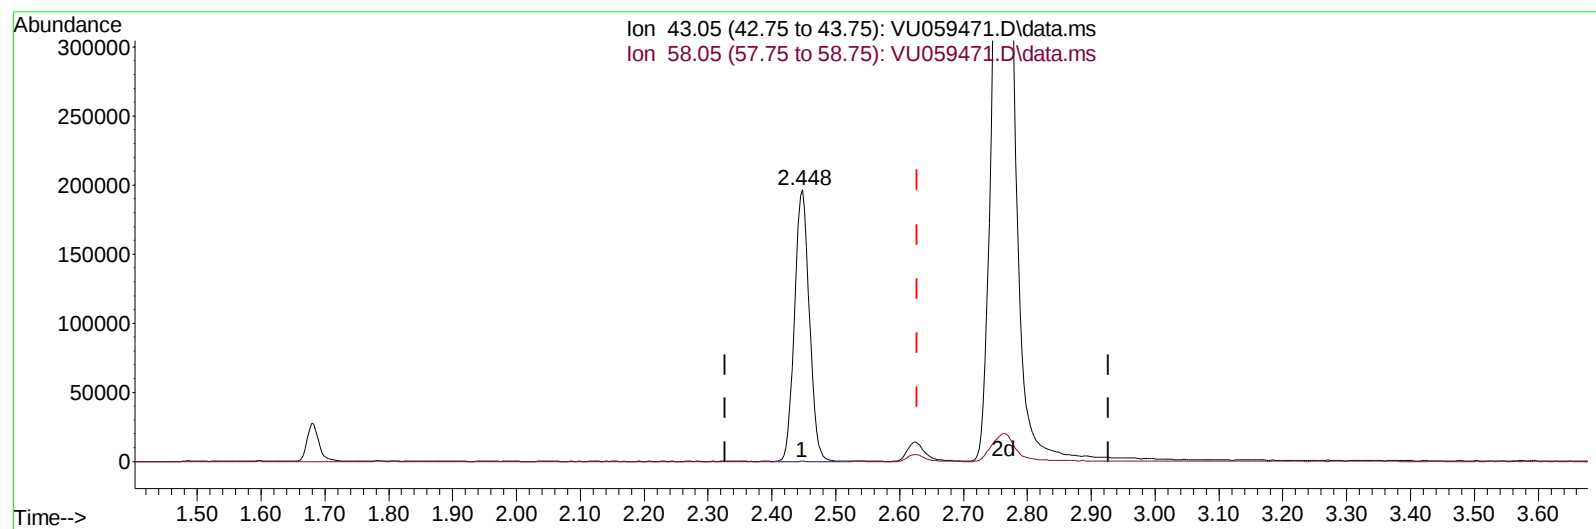

TIC: VU059471.D\data.ms

(13) Acetone (T)

2.448min (-0.180) 246.51 ug/L

response 316746

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	3.01
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062524\
Data File : VU059471.D
Acq On : 25 Jun 2024 15:06
Operator : MD/SY
Sample : P2961-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GC6

Manual IntegrationsAPPROVED

Quant Time: Jun 26 04:30:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 26 04:26:20 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/26/2024
Supervised By :Semsettin Yesilyurt 06/26/2024

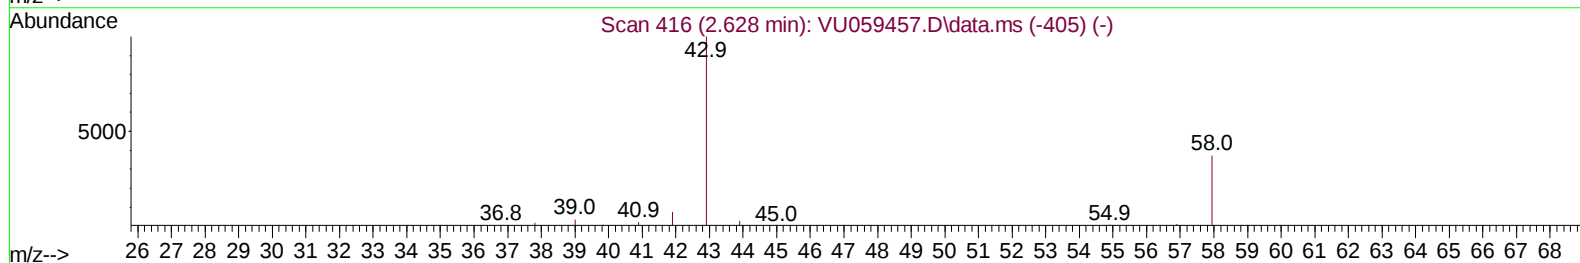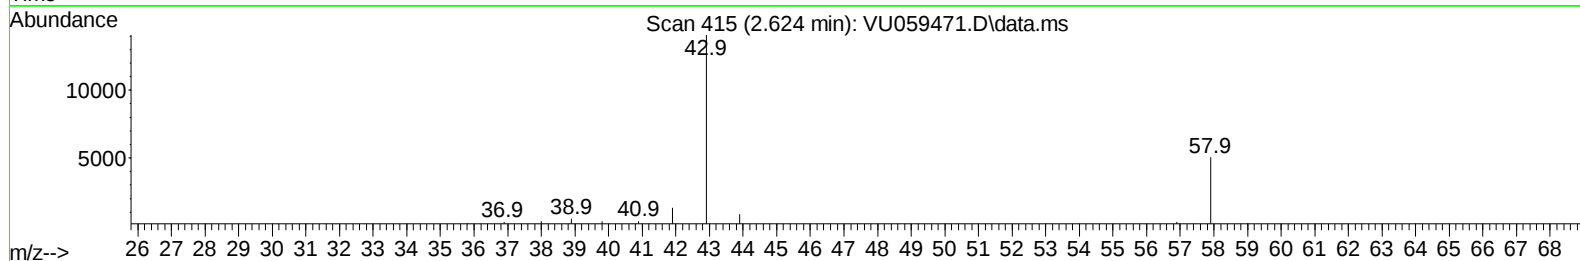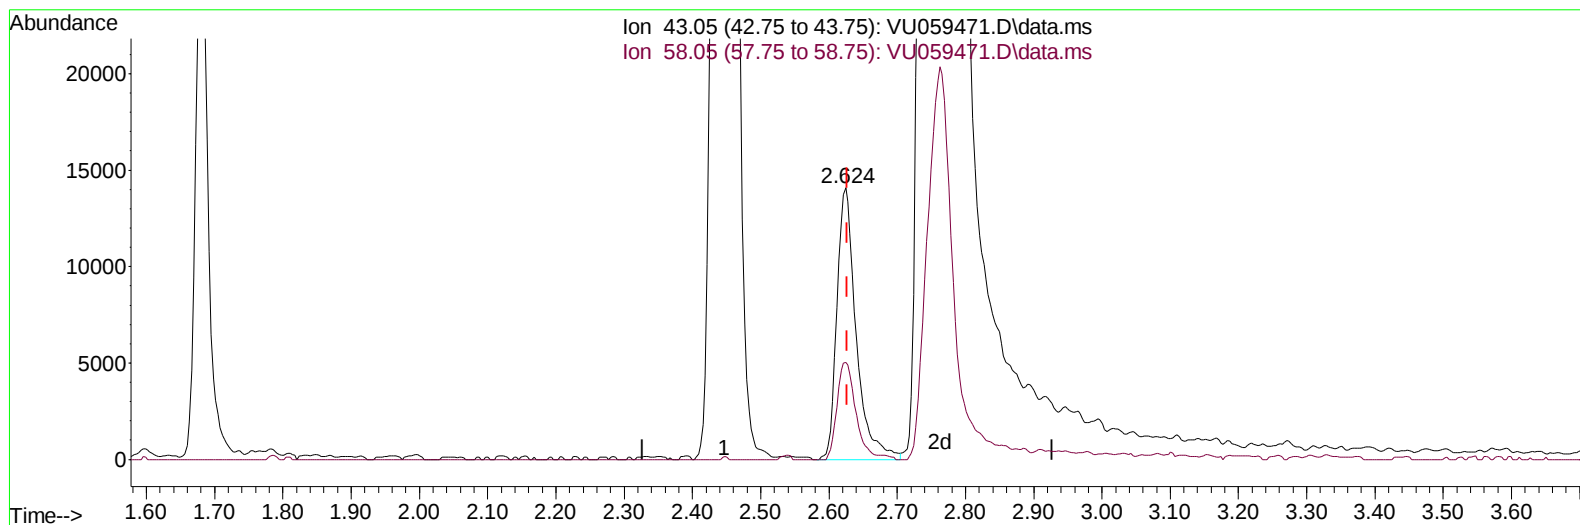

TIC: VU059471.D\data.ms

(13) Acetone (T)

2.624min (-0.003) 21.45 ug/L m

response 27557

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	34.58
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062524\
 Data File : VU059471.D
 Acq On : 25 Jun 2024 15:06
 Operator : MD/SY
 Sample : P2961-14
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GC6

Manual IntegrationsAPPROVED

Quant Time: Jun 26 04:30:03 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 26 04:26:20 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/26/2024
 Supervised By :Semsettin Yesilyurt 06/26/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.245	114		138295	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		148028	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		67292	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.595	65		30126	3.133	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	62.600%	
7) Chloroethane-d5	1.907	69		35726	3.861	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	77.200%	
11) 1,1-Dichloroethene-d2	2.560	65		11964	2.999	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	60.000%	
20) 2-Butanone-d5	4.615	46		138814	70.079	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery	=	140.160%#	
24) Chloroform-d	5.055	84		88402	4.479	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	89.600%	
26) 1,2-Dichloroethane-d4	5.695	65		46889	4.932	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	98.600%	
32) Benzene-d6	5.721	84		151251	3.713	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	74.200%	
36) 1,2-Dichloropropane-d6	6.682	67		56587	4.533	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	90.600%	
41) Toluene-d8	7.894	98		115953	3.062	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	61.200%#	
43) trans-1,3-Dichloroprop...	8.177	79		17260	4.415	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	88.400%	
46) 2-Hexanone-d5	8.627	63		101371	62.412	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	124.820%	
56) 1,1,2,2-Tetrachloroeth...	10.749	84		58590	5.680	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	113.600%	
66) 1,2-Dichlorobenzene-d4	12.190	152		59894	5.001	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	100.000%	
Target Compounds							
13) Acetone	2.624	43		27557m	21.446	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062524\
Data File : VU059471.D
Acq On : 25 Jun 2024 15:06
Operator : MD/SY
Sample : P2961-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GC6

Manual IntegrationsAPPROVED

Quant Time: Jun 26 04:30:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 26 04:26:20 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/26/2024
Supervised By :Semsettin Yesilyurt 06/26/2024

