




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062524\
Data File : VU059472.D
Acq On : 25 Jun 2024 15:30
Operator : MD/SY
Sample : P2961-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GE0

Manual IntegrationsAPPROVED

Quant Time: Jun 26 04:30:17 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 26 04:26:20 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/26/2024
Supervised By :Semsettin Yesilyurt 06/26/2024

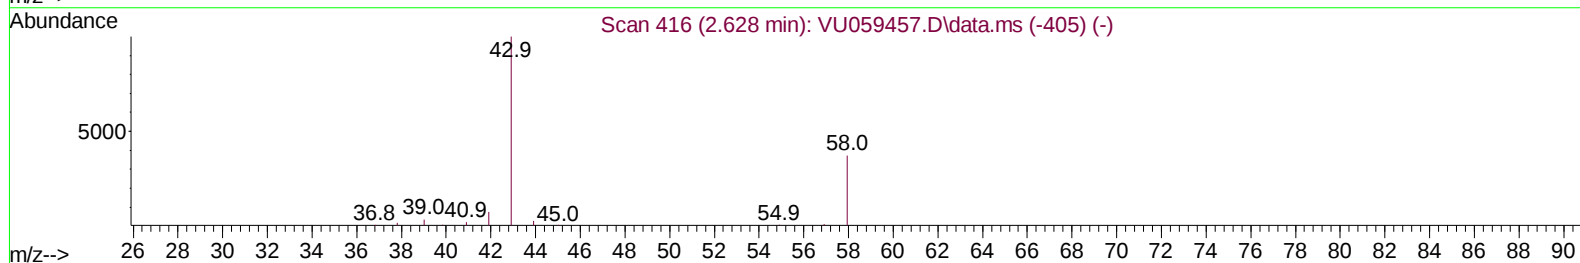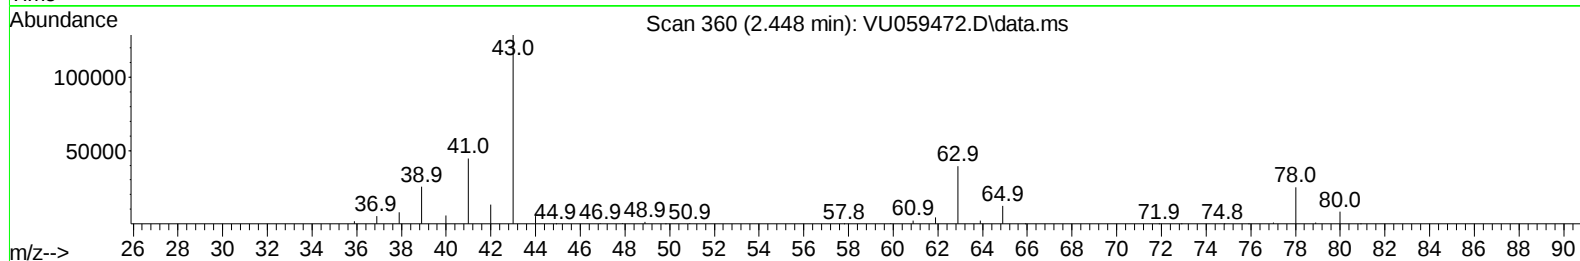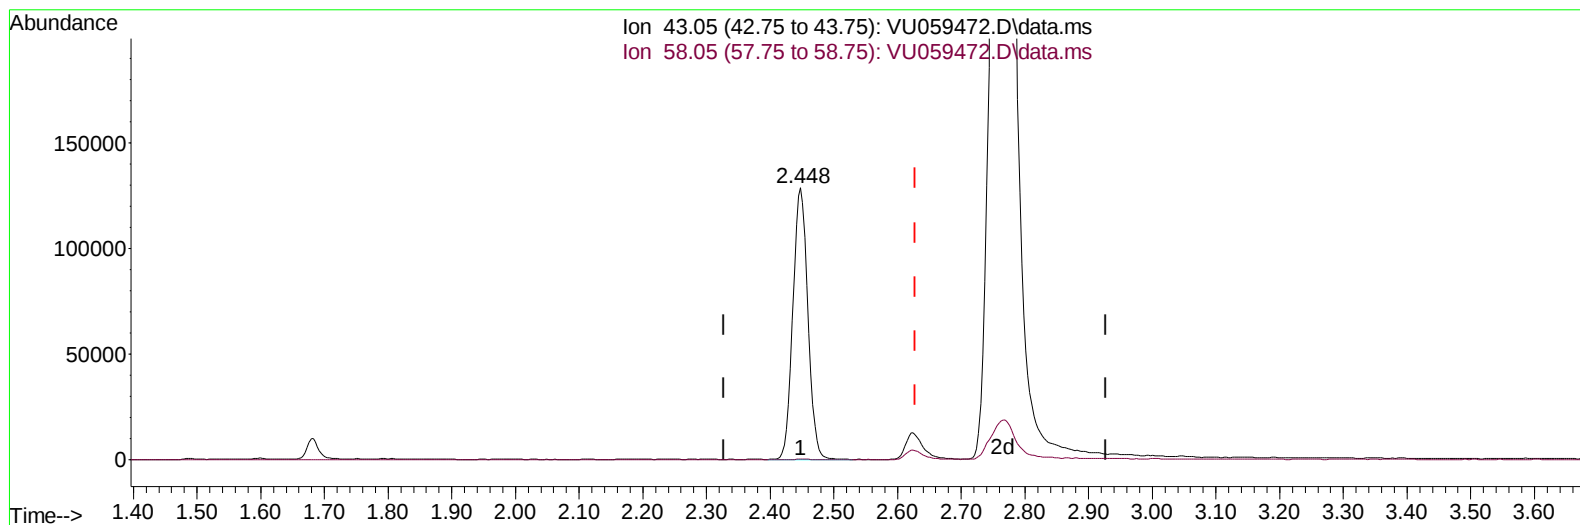

TIC: VU059472.D\data.ms

(13) Acetone (T)

2.448min (-0.180) 158.41 ug/L

response 210281

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	4.08
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062524\
Data File : VU059472.D
Acq On : 25 Jun 2024 15:30
Operator : MD/SY
Sample : P2961-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GE0

Manual IntegrationsAPPROVED

Quant Time: Jun 26 04:30:17 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 26 04:26:20 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/26/2024
Supervised By :Semsettin Yesilyurt 06/26/2024

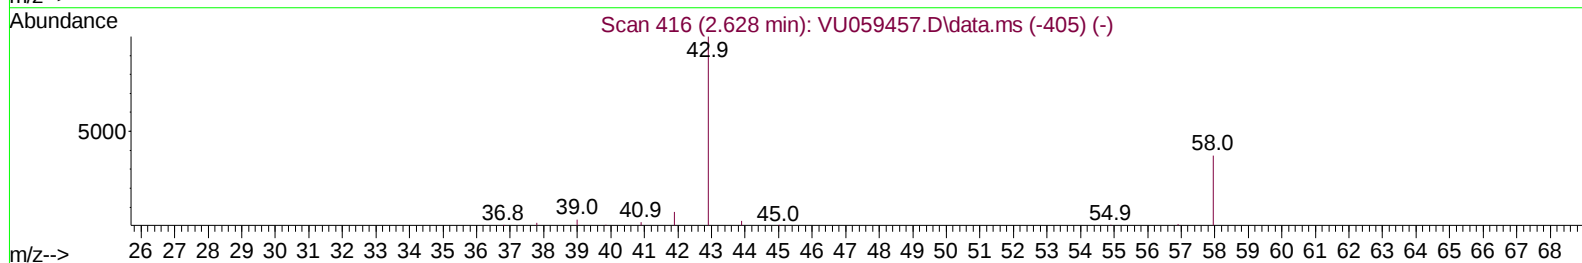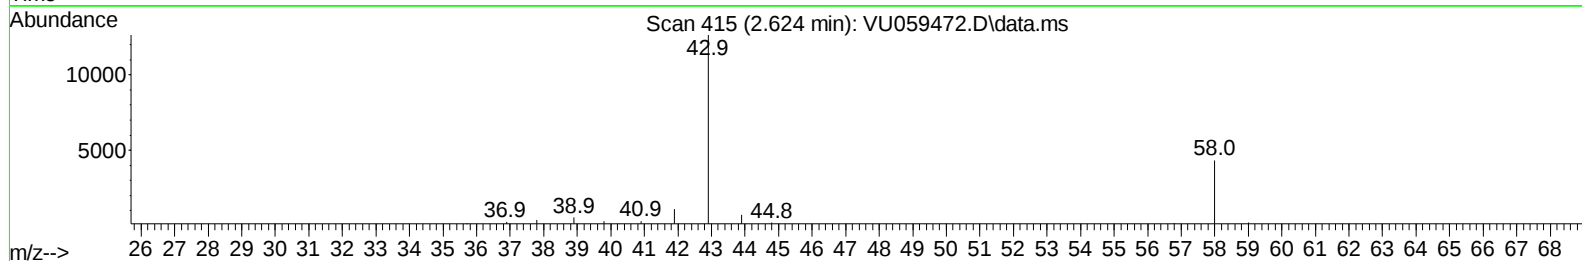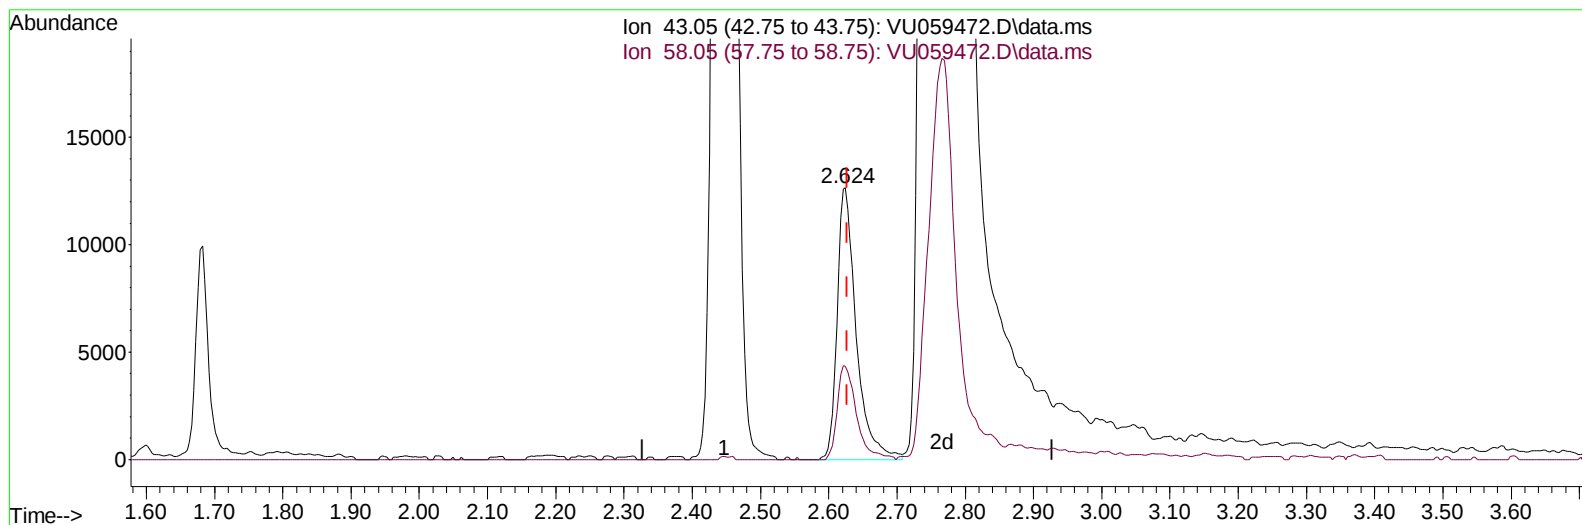

TIC: VU059472.D\data.ms

(13) Acetone (T)

2.624min (-0.003) 18.44 ug/L m

response 24482

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	35.02
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062524\
 Data File : VU059472.D
 Acq On : 25 Jun 2024 15:30
 Operator : MD/SY
 Sample : P2961-15
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GE0

Manual IntegrationsAPPROVED

Quant Time: Jun 26 04:30:17 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 26 04:26:20 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/26/2024
 Supervised By :Semsettin Yesilyurt 06/26/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.245	114		142870	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		150015	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		66401	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.596	65		28701	2.889	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery =	57.800%		
7) Chloroethane-d5	1.907	69		34704	3.631	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery =	72.600%		
11) 1,1-Dichloroethene-d2	2.560	65		11658	2.829	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery =	56.600%#		
20) 2-Butanone-d5	4.615	46		138819	67.837	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery =	135.680%#		
24) Chloroform-d	5.055	84		88263	4.328	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	86.600%		
26) 1,2-Dichloroethane-d4	5.695	65		47065	4.792	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	95.800%		
32) Benzene-d6	5.721	84		150729	3.651	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	73.000%		
36) 1,2-Dichloropropane-d6	6.685	67		55985	4.425	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery =	88.600%		
41) Toluene-d8	7.894	98		112209	2.924	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	58.400%#		
43) trans-1,3-Dichloroprop...	8.177	79		16136	4.073	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery =	81.400%		
46) 2-Hexanone-d5	8.627	63		96764	58.787	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery =	117.580%		
56) 1,1,2,2-Tetrachloroeth...	10.750	84		58302	5.578	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery =	111.600%		
66) 1,2-Dichlorobenzene-d4	12.190	152		60224	5.096	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery =	102.000%		
Target Compounds							
13) Acetone	2.624	43		24482m	18.443	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062524\
Data File : VU059472.D
Acq On : 25 Jun 2024 15:30
Operator : MD/SY
Sample : P2961-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GE0

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 06/26/2024
Supervised By :Semsettin Yesilyurt 06/26/2024

Quant Time: Jun 26 04:30:17 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 26 04:26:20 2024
Response via : Initial Calibration

