




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062524\
Data File : VU059478.D
Acq On : 25 Jun 2024 17:54
Operator : MD/SY
Sample : P2961-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G87

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 06/26/2024
Supervised By :Semsettin Yesilyurt 06/26/2024

Quant Time: Jun 26 04:31:43 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 26 04:26:20 2024
Response via : Initial Calibration

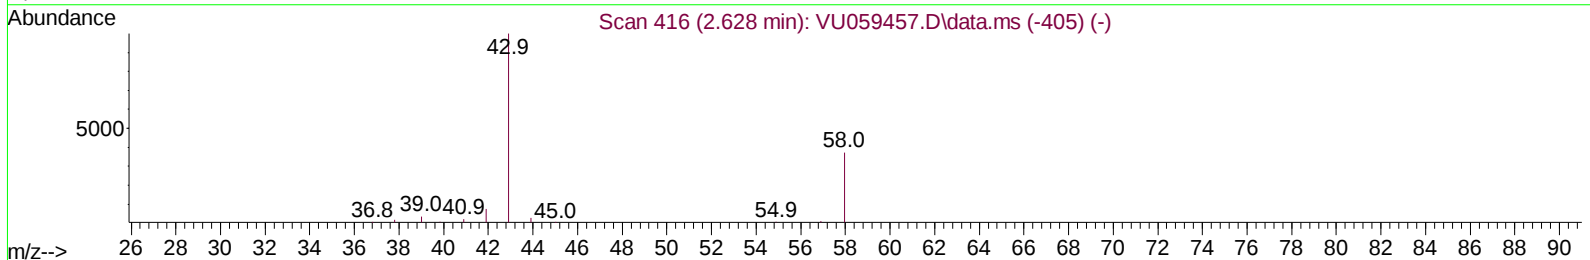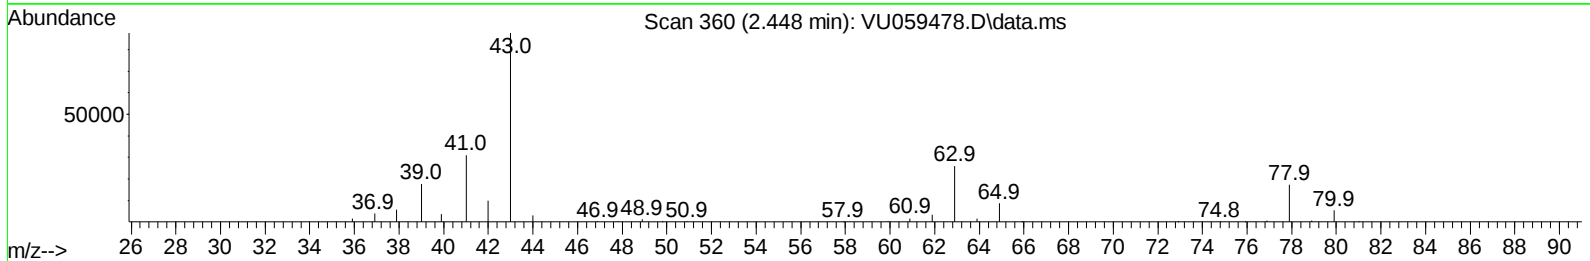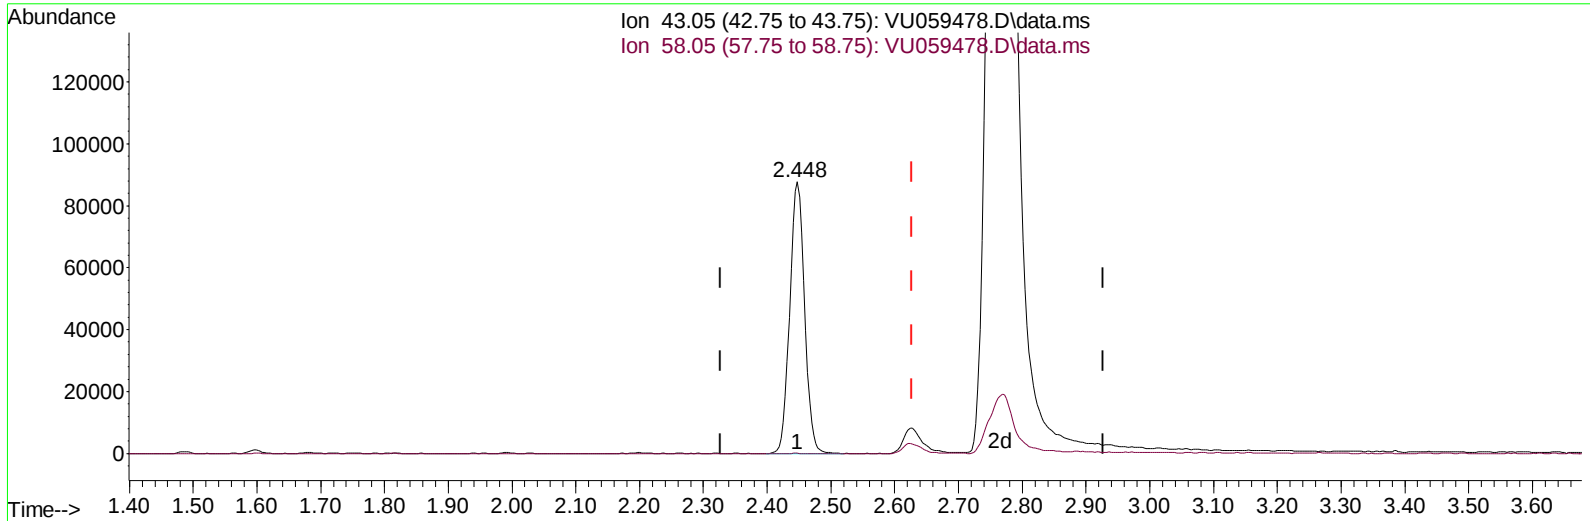

TIC: VU059478.D\data.ms

(13) Acetone (T)

2.448min (-0.180) 109.78 ug/L

response 141671

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	4.57
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062524\
Data File : VU059478.D
Acq On : 25 Jun 2024 17:54
Operator : MD/SY
Sample : P2961-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G87

Manual IntegrationsAPPROVED

Quant Time: Jun 26 04:31:43 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 26 04:26:20 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/26/2024
Supervised By :Semsettin Yesilyurt 06/26/2024

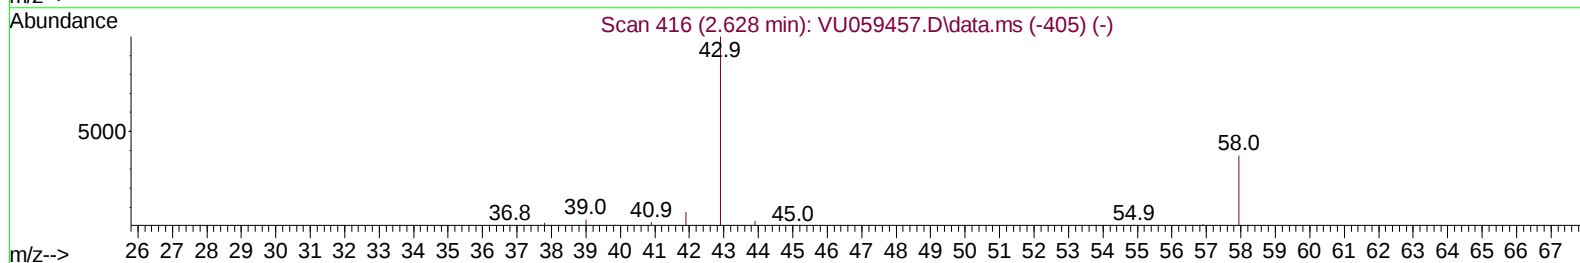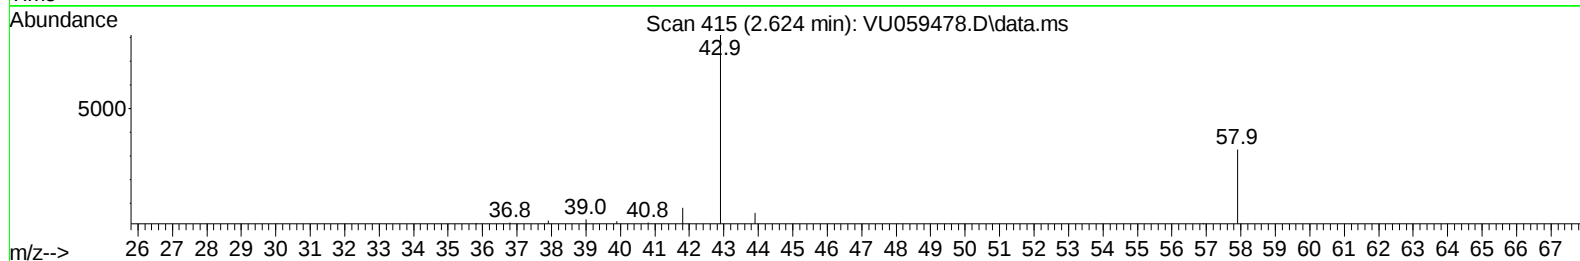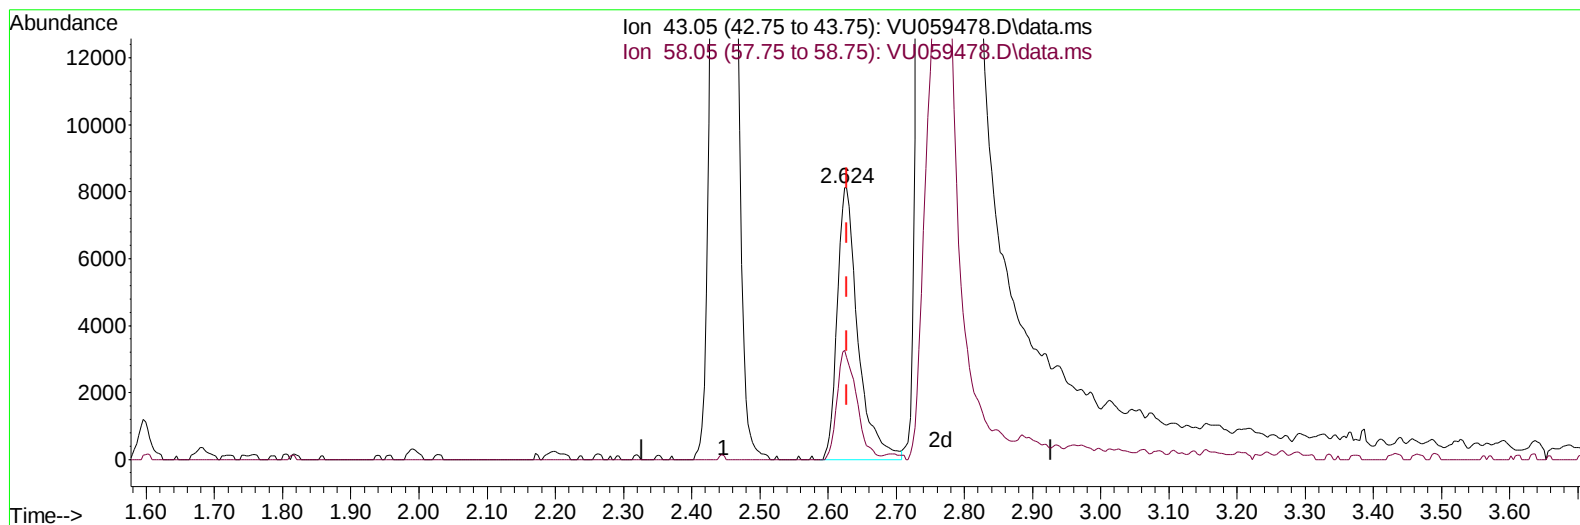

TIC: VU059478.D\data.ms

(13) Acetone (T)

2.624min (-0.003) 13.31 ug/L m

response 17183

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	37.72
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062524\
 Data File : VU059478.D
 Acq On : 25 Jun 2024 17:54
 Operator : MD/SY
 Sample : P2961-10
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1G87

Manual IntegrationsAPPROVED

Quant Time: Jun 26 04:31:43 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 26 04:26:20 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/26/2024
 Supervised By :Semsettin Yesilyurt 06/26/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.245	114		138898	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		147649	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.811	152		63924	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.592	65		28007	2.900	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	58.000%	
7) Chloroethane-d5	1.907	69		34165	3.676	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	73.600%	
11) 1,1-Dichloroethene-d2	2.560	65		10992	2.743	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	54.800%#	
20) 2-Butanone-d5	4.615	46		133582	67.145	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	134.280%#	
24) Chloroform-d	5.055	84		83939	4.234	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.600%	
26) 1,2-Dichloroethane-d4	5.695	65		45486	4.763	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.200%	
32) Benzene-d6	5.721	84		143556	3.533	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	70.600%	
36) 1,2-Dichloropropane-d6	6.685	67		53111	4.265	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	85.400%	
41) Toluene-d8	7.894	98		107306	2.841	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	56.800%#	
43) trans-1,3-Dichloroprop...	8.177	79		15341	3.935	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	78.600%	
46) 2-Hexanone-d5	8.627	63		94575	58.378	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	116.760%	
56) 1,1,2,2-Tetrachloroeth...	10.749	84		54956	5.342	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	106.800%	
66) 1,2-Dichlorobenzene-d4	12.190	152		54125	4.757	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.200%	
Target Compounds							
13) Acetone	2.624	43		17183m	13.315	ug/L	
22) cis-1,2-Dichloroethene	4.663	96		5614	0.497	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062524\
Data File : VU059478.D
Acq On : 25 Jun 2024 17:54
Operator : MD/SY
Sample : P2961-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G87

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 06/26/2024
Supervised By :Semsettin Yesilyurt 06/26/2024

Quant Time: Jun 26 04:31:43 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 26 04:26:20 2024
Response via : Initial Calibration

