




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062524\
Data File : VU059479.D
Acq On : 25 Jun 2024 18:18
Operator : MD/SY
Sample : P2961-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G88

Manual IntegrationsAPPROVED

Quant Time: Jun 26 04:31:58 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 26 04:26:20 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/26/2024
Supervised By :Semsettin Yesilyurt 06/26/2024

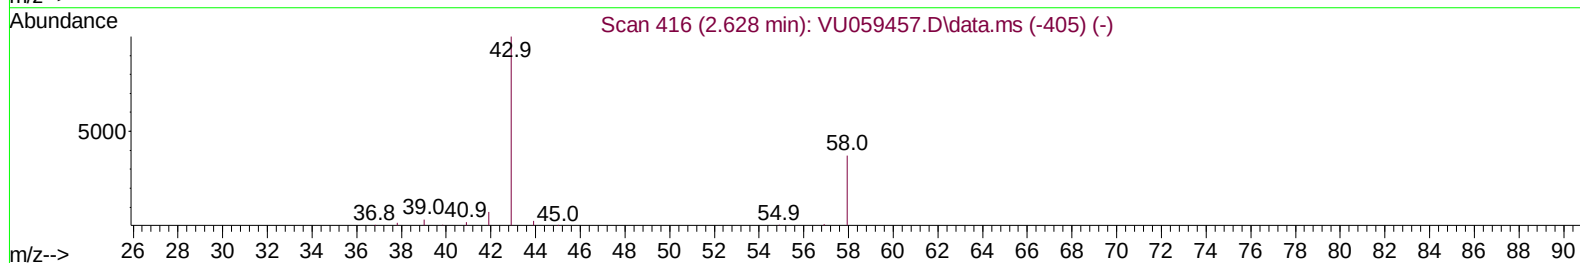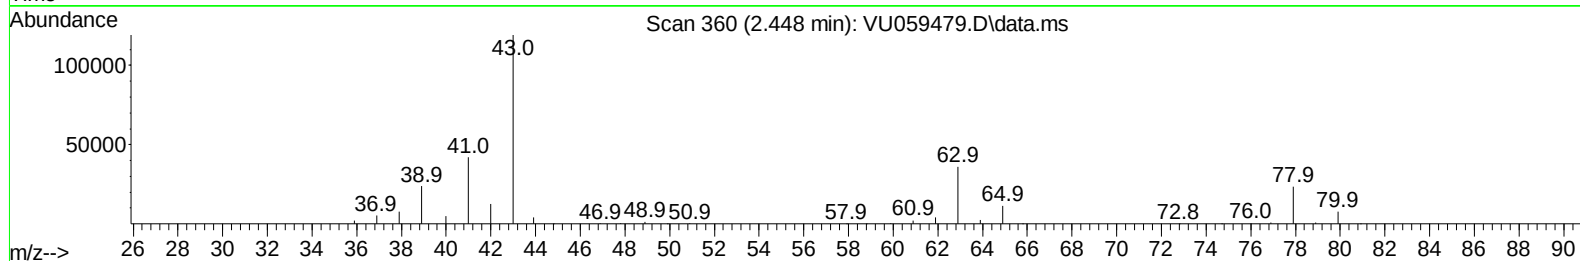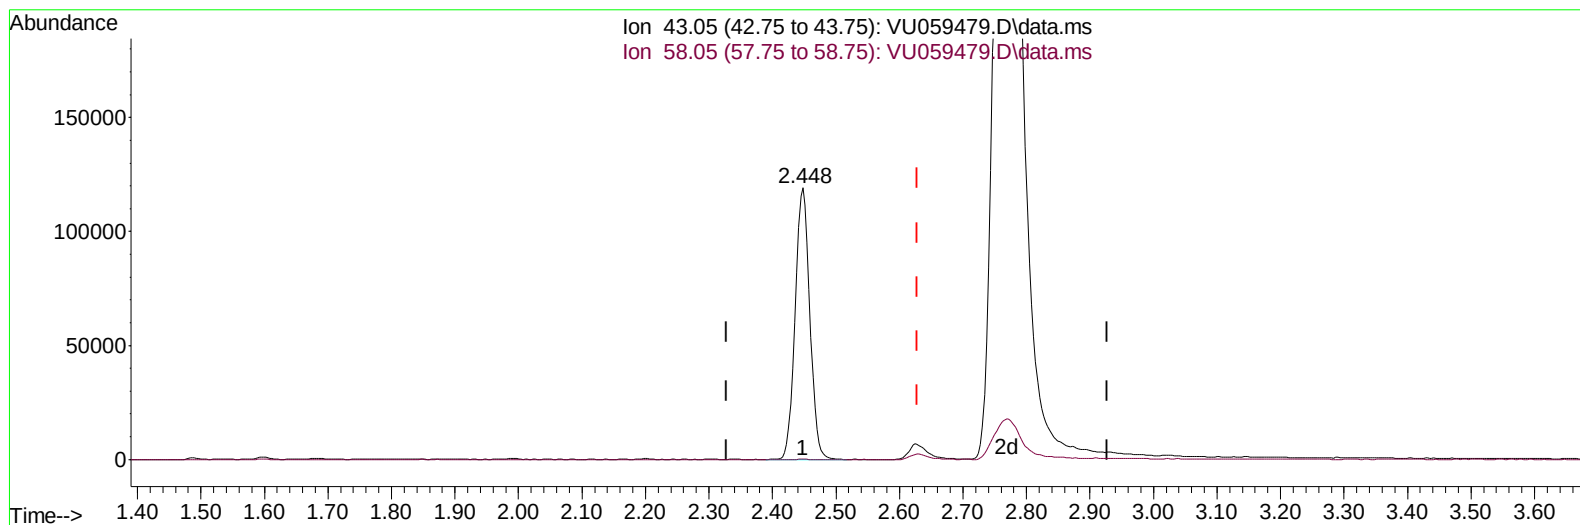

TIC: VU059479.D\data.ms

(13) Acetone (T)

2.448min (-0.180) 146.90 ug/L

response 191503

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	2.40
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062524\
Data File : VU059479.D
Acq On : 25 Jun 2024 18:18
Operator : MD/SY
Sample : P2961-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G88

Manual IntegrationsAPPROVED

Quant Time: Jun 26 04:31:58 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 26 04:26:20 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/26/2024
Supervised By :Semsettin Yesilyurt 06/26/2024

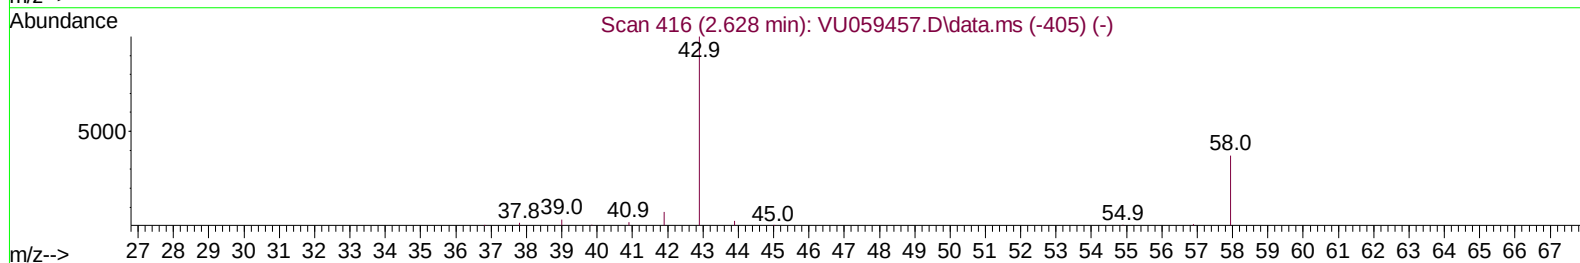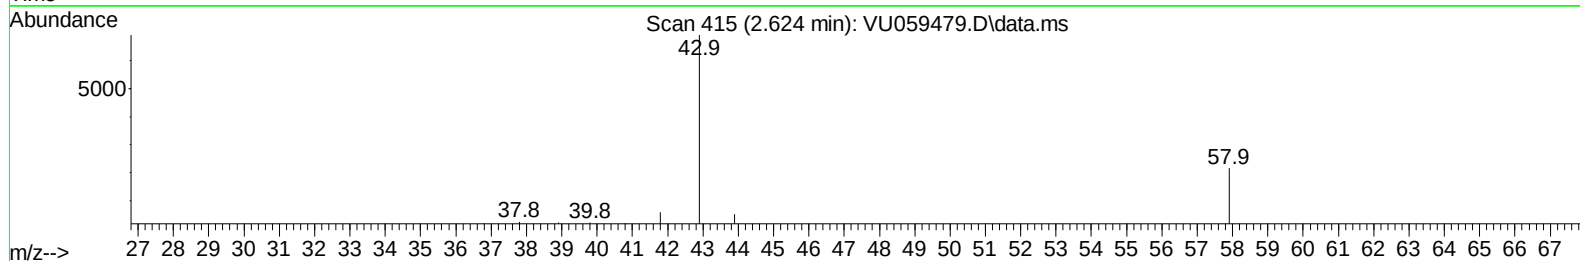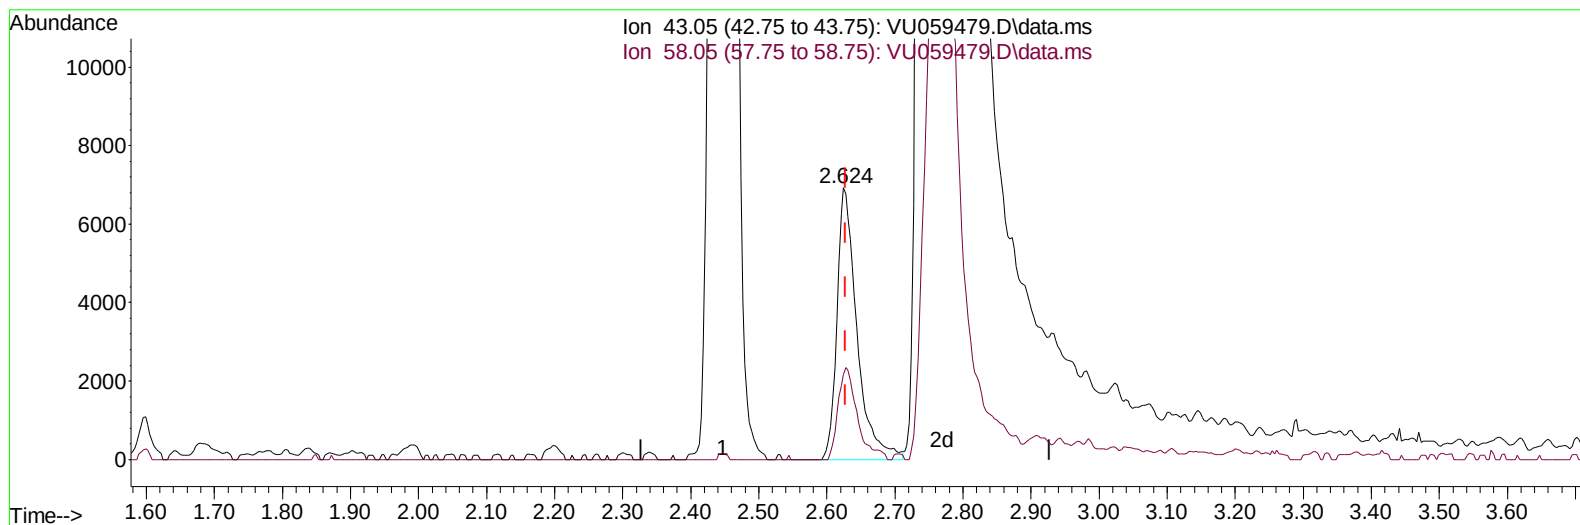

TIC: VU059479.D\data.ms

(13) Acetone (T)

2.624min (-0.003) 10.80 ug/L m

response 14079

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	32.65
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062524\
 Data File : VU059479.D
 Acq On : 25 Jun 2024 18:18
 Operator : MD/SY
 Sample : P2961-11
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1G88

Manual IntegrationsAPPROVED

Quant Time: Jun 26 04:31:58 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 26 04:26:20 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/26/2024
 Supervised By :Semsettin Yesilyurt 06/26/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.245	114		140307	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		147558	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.811	152		63836	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.592	65		28106	2.881	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	57.600%	
7) Chloroethane-d5	1.907	69		34213	3.645	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	72.800%	
11) 1,1-Dichloroethene-d2	2.560	65		11535	2.850	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	57.000%#	
20) 2-Butanone-d5	4.615	46		134019	66.688	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery	=	133.380%#	
24) Chloroform-d	5.055	84		86671	4.328	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	86.600%	
26) 1,2-Dichloroethane-d4	5.695	65		44935	4.658	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	93.200%	
32) Benzene-d6	5.721	84		145216	3.576	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	71.600%	
36) 1,2-Dichloropropane-d6	6.685	67		54295	4.363	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	87.200%	
41) Toluene-d8	7.894	98		106883	2.831	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	56.600%#	
43) trans-1,3-Dichloroprop...	8.177	79		16026	4.113	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	82.200%	
46) 2-Hexanone-d5	8.627	63		94398	58.304	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	116.600%	
56) 1,1,2,2-Tetrachloroeth...	10.750	84		55635	5.411	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	108.200%	
66) 1,2-Dichlorobenzene-d4	12.190	152		53370	4.697	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	94.000%	
Target Compounds							
							Qvalue
13) Acetone	2.624	43		14079m	10.800	ug/L	
42) Toluene	7.965	91		28100	0.592	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062524\
Data File : VU059479.D
Acq On : 25 Jun 2024 18:18
Operator : MD/SY
Sample : P2961-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G88

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 06/26/2024
Supervised By :Semsettin Yesilyurt 06/26/2024

Quant Time: Jun 26 04:31:58 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 26 04:26:20 2024
Response via : Initial Calibration

