




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062524\
Data File : VU059480.D
Acq On : 25 Jun 2024 18:43
Operator : MD/SY
Sample : P2961-17
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G72

Manual IntegrationsAPPROVED

Quant Time: Jun 26 04:32:11 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 26 04:26:20 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/26/2024
Supervised By :Semsettin Yesilyurt 06/26/2024

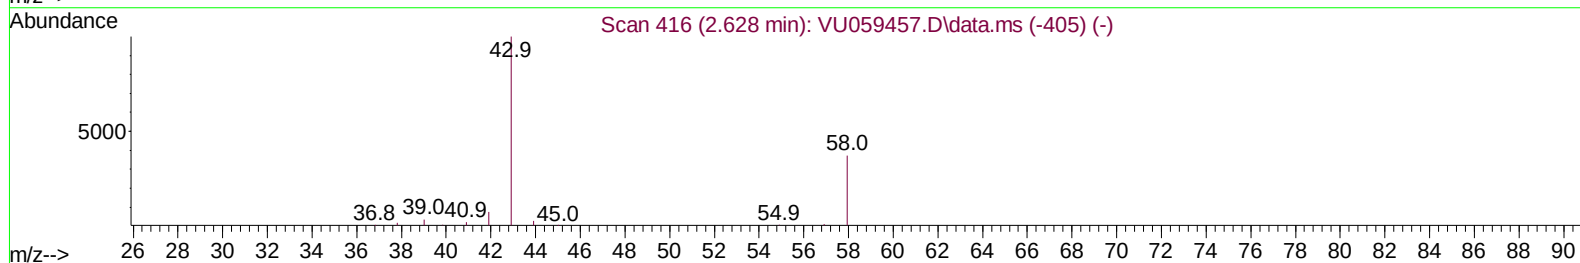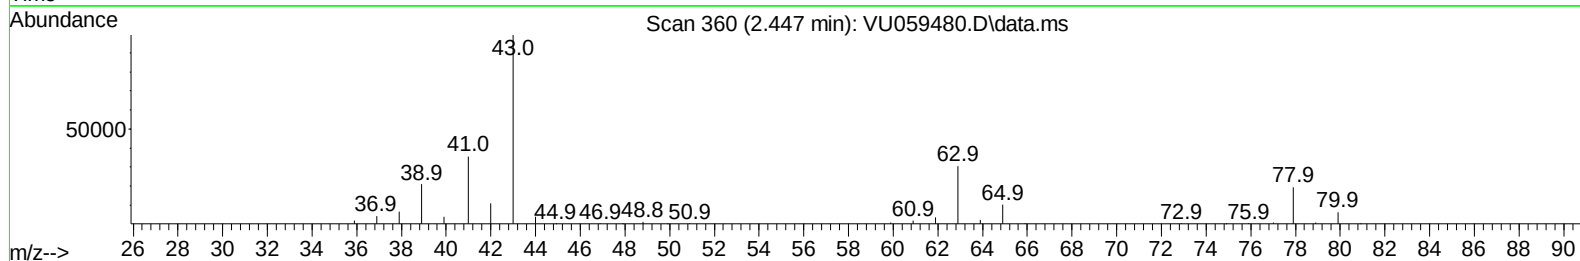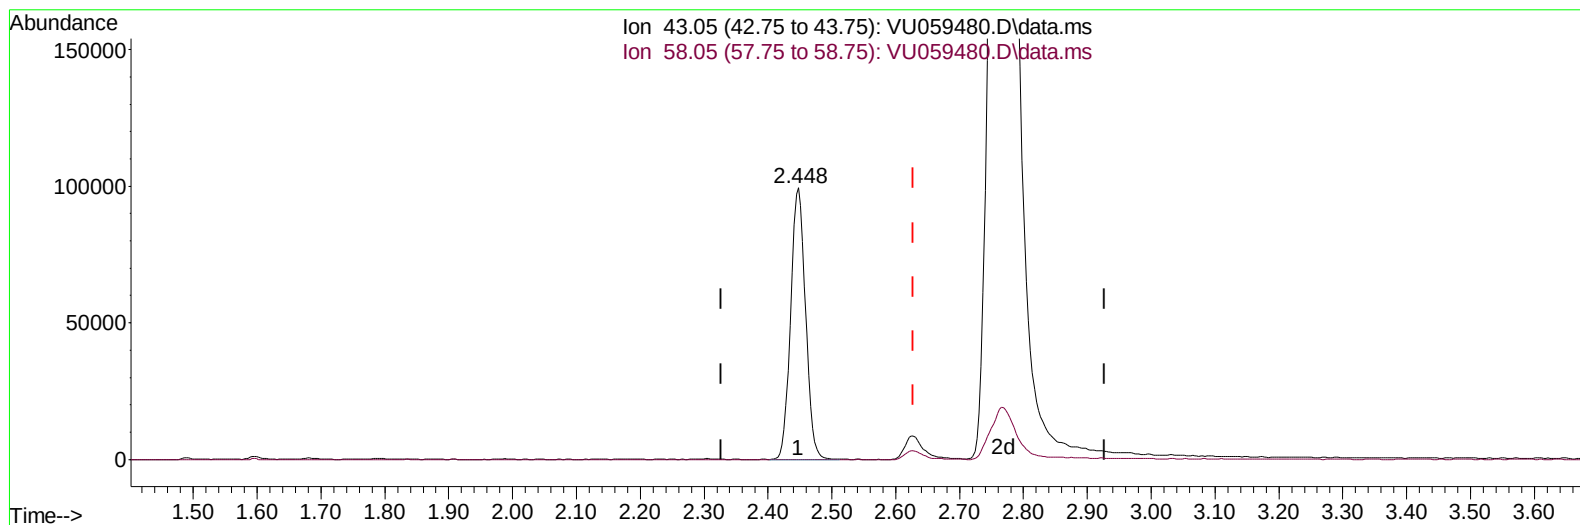

TIC: VU059480.D\data.ms

(13) Acetone (T)

2.447min (-0.180) 125.40 ug/L

response 160673

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	4.08
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062524\
Data File : VU059480.D
Acq On : 25 Jun 2024 18:43
Operator : MD/SY
Sample : P2961-17
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G72

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 06/26/2024
Supervised By :Semsettin Yesilyurt 06/26/2024

Quant Time: Jun 26 04:32:11 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 26 04:26:20 2024
Response via : Initial Calibration

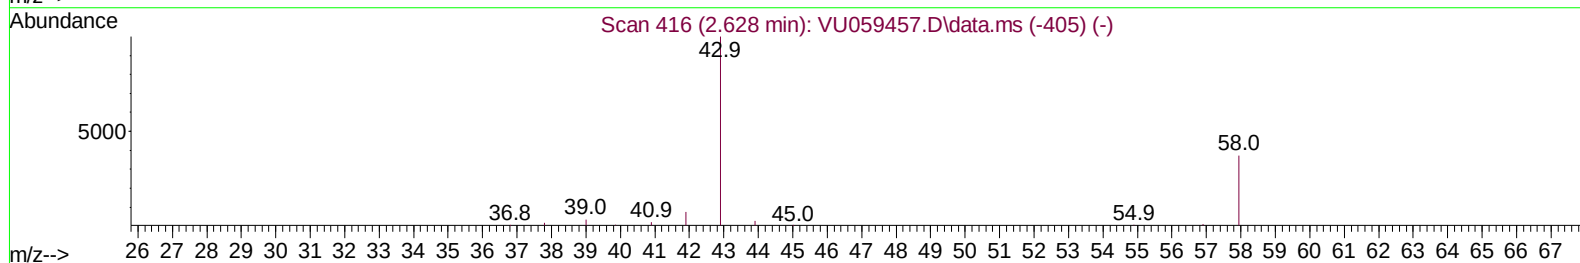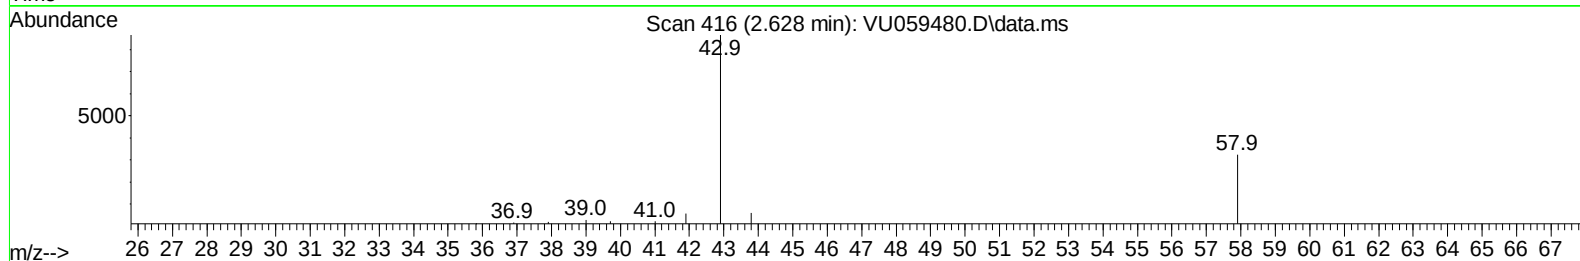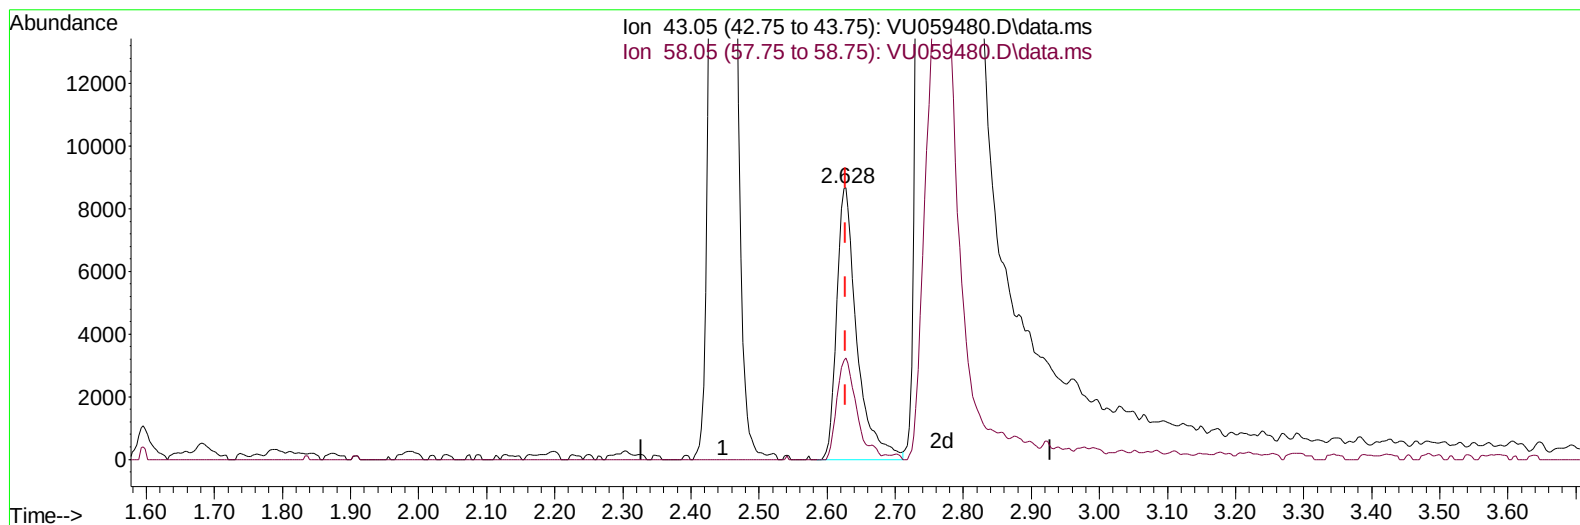

TIC: VU059480.D\data.ms

(13) Acetone (T)

2.628min (+ 0.000) 13.96 ug/L m

response 17885

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	36.63
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062524\
 Data File : VU059480.D
 Acq On : 25 Jun 2024 18:43
 Operator : MD/SY
 Sample : P2961-17
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1G72

Manual IntegrationsAPPROVED

Quant Time: Jun 26 04:32:11 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 26 04:26:20 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/26/2024
 Supervised By :Semsettin Yesilyurt 06/26/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.245	114		137904	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		143133	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.810	152		62075	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.592	65		28399	2.962	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	59.200%	
7) Chloroethane-d5	1.907	69		34433	3.732	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	74.600%	
11) 1,1-Dichloroethene-d2	2.560	65		11047	2.777	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	55.600%#	
20) 2-Butanone-d5	4.615	46		134492	68.089	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery	=	136.180%#	
24) Chloroform-d	5.055	84		86714	4.406	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	88.200%	
26) 1,2-Dichloroethane-d4	5.695	65		45433	4.792	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	95.800%	
32) Benzene-d6	5.721	84		142914	3.628	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	72.600%	
36) 1,2-Dichloropropane-d6	6.682	67		54190	4.489	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	89.800%	
41) Toluene-d8	7.894	98		108140	2.953	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	59.000%#	
43) trans-1,3-Dichloroprop...	8.177	79		15248	4.034	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	80.600%	
46) 2-Hexanone-d5	8.627	63		94105	59.920	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	119.840%	
56) 1,1,2,2-Tetrachloroeth...	10.749	84		55283	5.543	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	110.800%	
66) 1,2-Dichlorobenzene-d4	12.190	152		53885	4.877	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	97.600%	
Target Compounds							
13) Acetone	2.628	43		17885m	13.958	ug/L	
42) Toluene	7.968	91		23703	0.515	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062524\
Data File : VU059480.D
Acq On : 25 Jun 2024 18:43
Operator : MD/SY
Sample : P2961-17
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G72

Manual IntegrationsAPPROVED

Quant Time: Jun 26 04:32:11 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 26 04:26:20 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/26/2024
Supervised By :Semsettin Yesilyurt 06/26/2024

