




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062524\
Data File : VU059498.D
Acq On : 26 Jun 2024 02:31
Operator : MD/SY
Sample : P3006-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JMRH2

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 06/26/2024
Supervised By :Semsettin Yesilyurt 06/26/2024

Quant Time: Jun 26 06:19:55 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 26 05:55:36 2024
Response via : Initial Calibration

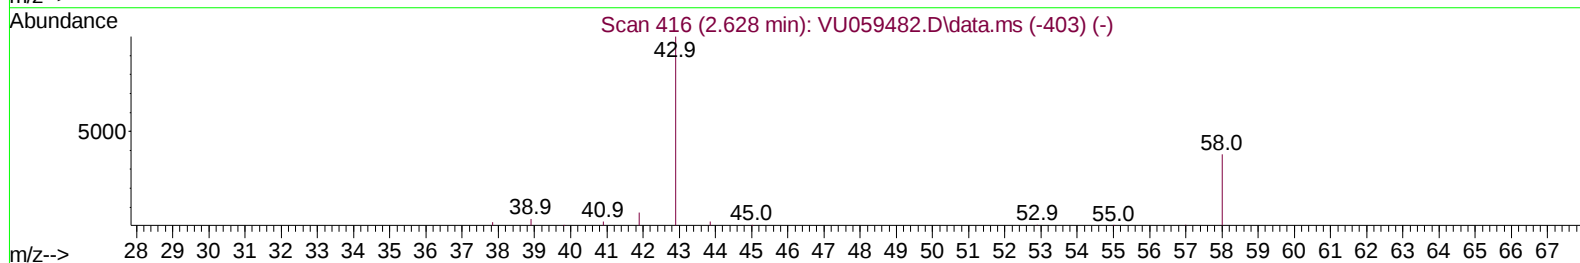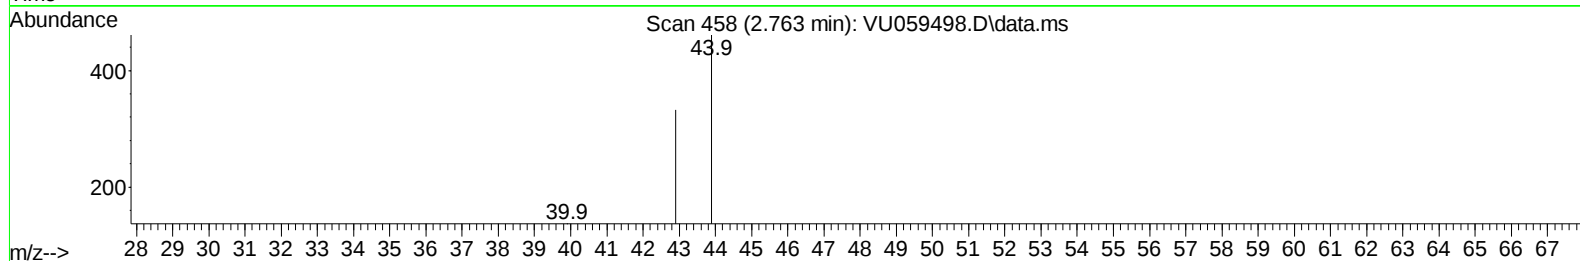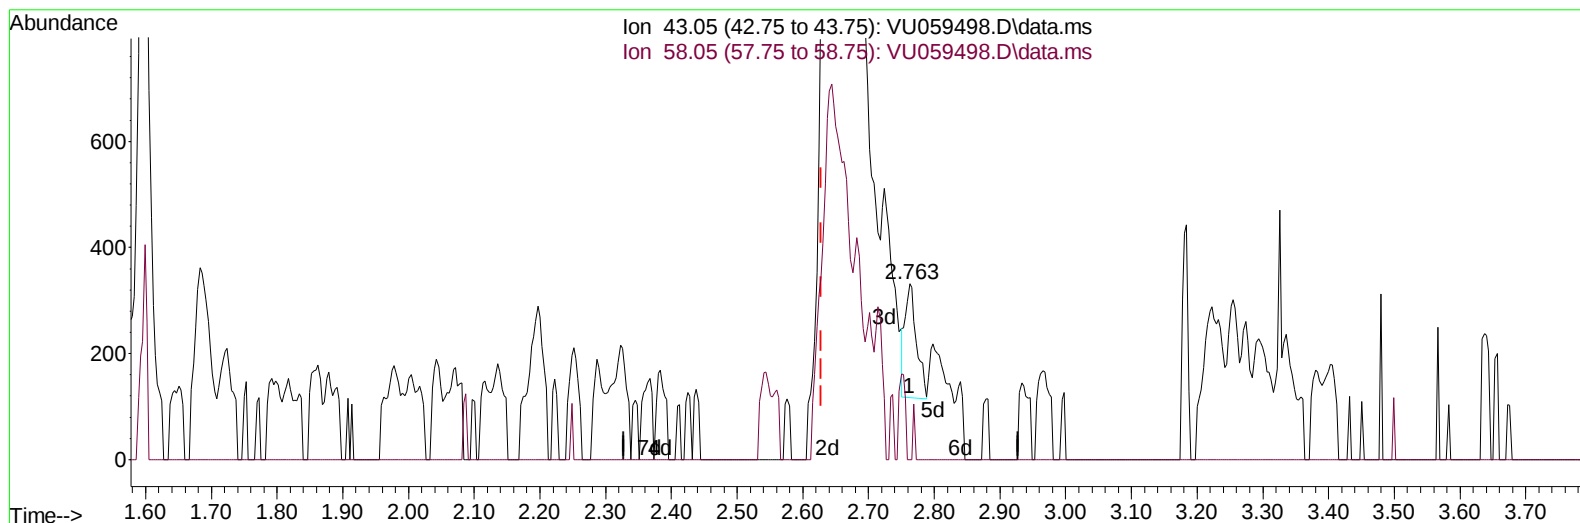

TIC: VU059498.D\data.ms

(13) Acetone (T)

2.763min (+ 0.135) 0.21 ug/L

response 267

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	40.82
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062524\
Data File : VU059498.D
Acq On : 26 Jun 2024 02:31
Operator : MD/SY
Sample : P3006-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JMRH2

Manual IntegrationsAPPROVED

Quant Time: Jun 26 06:19:55 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 26 05:55:36 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/26/2024
Supervised By :Semsettin Yesilyurt 06/26/2024

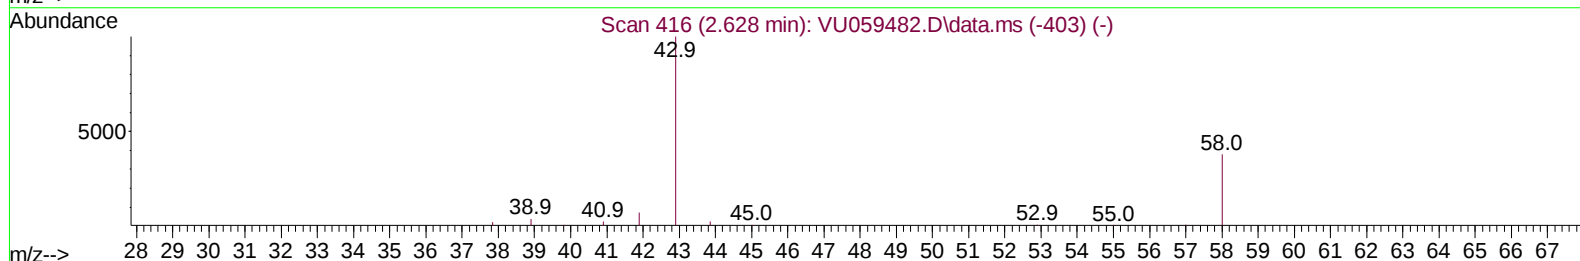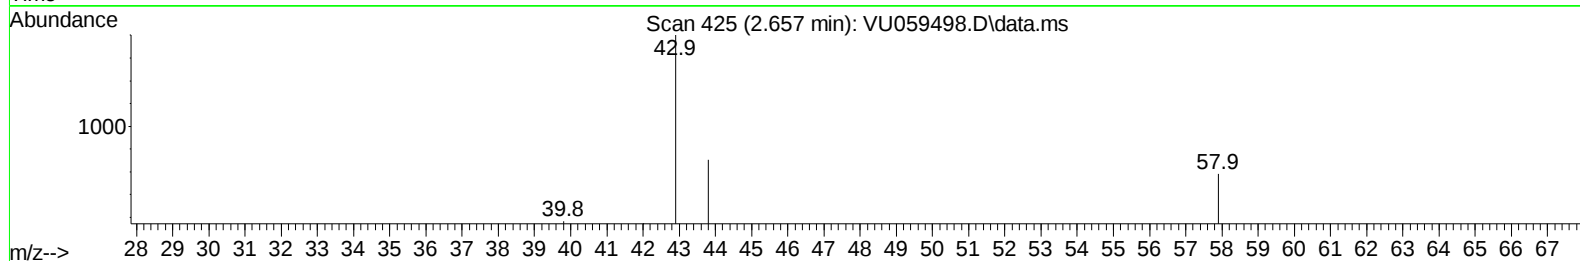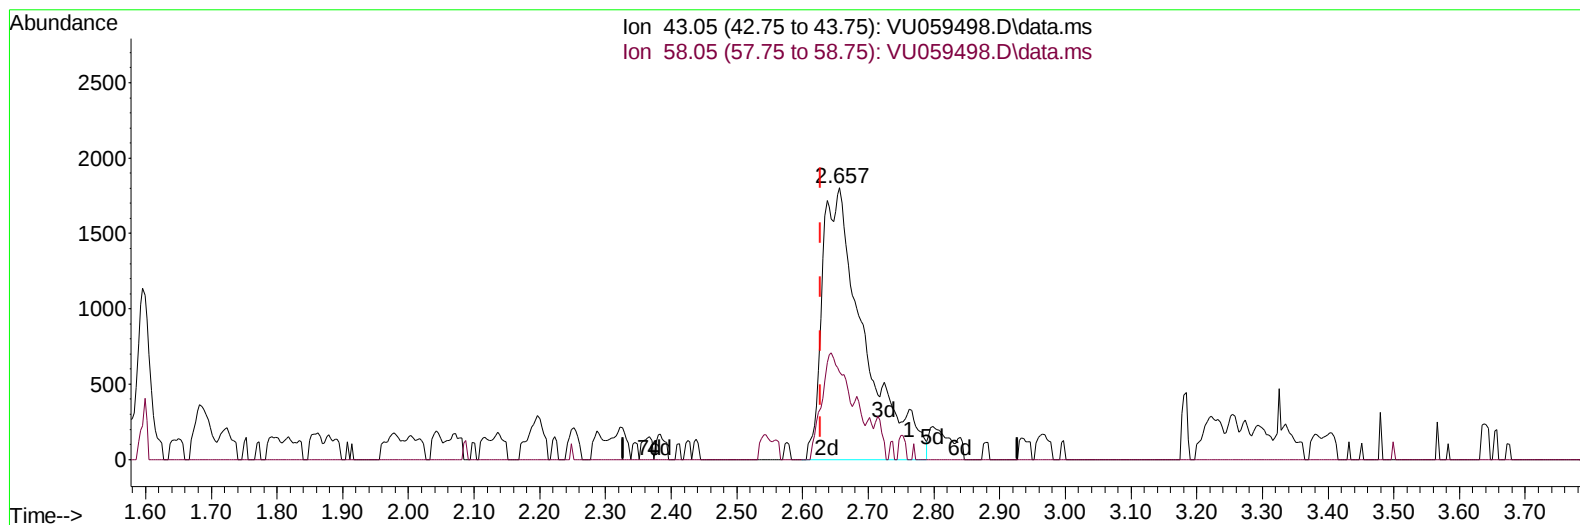

TIC: VU059498.D\data.ms

(13) Acetone (T)

2.657min (+ 0.029) 6.34 ug/L m

response 7951

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	1.37
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062524\
 Data File : VU059498.D
 Acq On : 26 Jun 2024 02:31
 Operator : MD/SY
 Sample : P3006-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 JMRH2

Manual IntegrationsAPPROVED

Quant Time: Jun 26 06:19:55 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 26 05:55:36 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/26/2024
 Supervised By :Semsettin Yesilyurt 06/26/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.242	114		134900	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		145737	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		62863	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.592	65		42724	4.555	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	91.000%	
7) Chloroethane-d5	1.907	69		40671	4.506	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.200%	
11) 1,1-Dichloroethene-d2	2.557	65		18694	4.804	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	96.000%	
20) 2-Butanone-d5	4.631	46		101342	52.449	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.900%	
24) Chloroform-d	5.055	84		90261	4.688	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.800%	
26) 1,2-Dichloroethane-d4	5.692	65		45190	4.872	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.400%	
32) Benzene-d6	5.718	84		177560	4.427	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.600%	
36) 1,2-Dichloropropane-d6	6.682	67		54717	4.452	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.000%	
41) Toluene-d8	7.891	98		147288	3.950	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.000%	
43) trans-1,3-Dichloroprop...	8.177	79		15723	4.085	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.800%	
46) 2-Hexanone-d5	8.627	63		73259	45.813	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.620%	
56) 1,1,2,2-Tetrachloroeth...	10.749	84		49736	4.898	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.000%	
66) 1,2-Dichlorobenzene-d4	12.190	152		55433	4.954	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.000%	
Target Compounds							
13) Acetone	2.657	43		7951m	6.344	ug/L	
18) trans-1,2-Dichloroethene	3.345	96		1212	0.122	ug/L	97
34) Trichloroethene	6.537	95		22906	1.911	ug/L	90
38) Bromodichloromethane	7.103	83		2050	0.143	ug/L #	87
42) Toluene	7.965	91		22068	0.471	ug/L	100
49) Dibromochloromethane	8.801	129		1954	0.209	ug/L	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062524\
Data File : VU059498.D
Acq On : 26 Jun 2024 02:31
Operator : MD/SY
Sample : P3006-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JMRH2

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 06/26/2024
Supervised By :Semsettin Yesilyurt 06/26/2024

Quant Time: Jun 26 06:19:55 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 26 05:55:36 2024
Response via : Initial Calibration

