

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062524\
 Data File : VU059469.D
 Acq On : 25 Jun 2024 14:18
 Operator : MD/SY
 Sample : P2961-12
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GB3

Quant Time: Jun 26 04:29:37 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 26 04:26:20 2024
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 06/26/2024
 Supervised By :Semsettin Yesilyurt 06/26/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	144723	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	151207	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	67602	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	29236	2.905	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	58.200%		
7) Chloroethane-d5	1.907	69	35173	3.632	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	72.600%		
11) 1,1-Dichloroethene-d2	2.560	65	11817	2.830	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	56.600%#		
20) 2-Butanone-d5	4.615	46	137701	66.429	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	132.860%#		
24) Chloroform-d	5.055	84	86938	4.209	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	84.200%		
26) 1,2-Dichloroethane-d4	5.695	65	47189	4.743	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	94.800%		
32) Benzene-d6	5.721	84	148916	3.578	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	71.600%		
36) 1,2-Dichloropropane-d6	6.685	67	55491	4.352	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	87.000%		
41) Toluene-d8	7.894	98	113282	2.928	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	58.600%#		
43) trans-1,3-Dichloroprop...	8.177	79	16539	4.142	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	82.800%		
46) 2-Hexanone-d5	8.627	63	96653	58.256	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	116.520%		
56) 1,1,2,2-Tetrachloroeth...	10.749	84	57464	5.454	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	109.000%		
66) 1,2-Dichlorobenzene-d4	12.190	152	60129	4.997	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	100.000%		
Target Compounds					Qvalue	
13) Acetone	2.624	43	29273m	21.770	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062524\
Data File : VU059469.D
Acq On : 25 Jun 2024 14:18
Operator : MD/SY
Sample : P2961-12
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1


Instrument :
MSVOA_U
ClientSampleId :
E1GB3

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 06/26/2024
Supervised By :Semsettin Yesilyurt 06/26/2024


Quant Time: Jun 26 04:29:37 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 26 04:26:20 2024
Response via : Initial Calibration

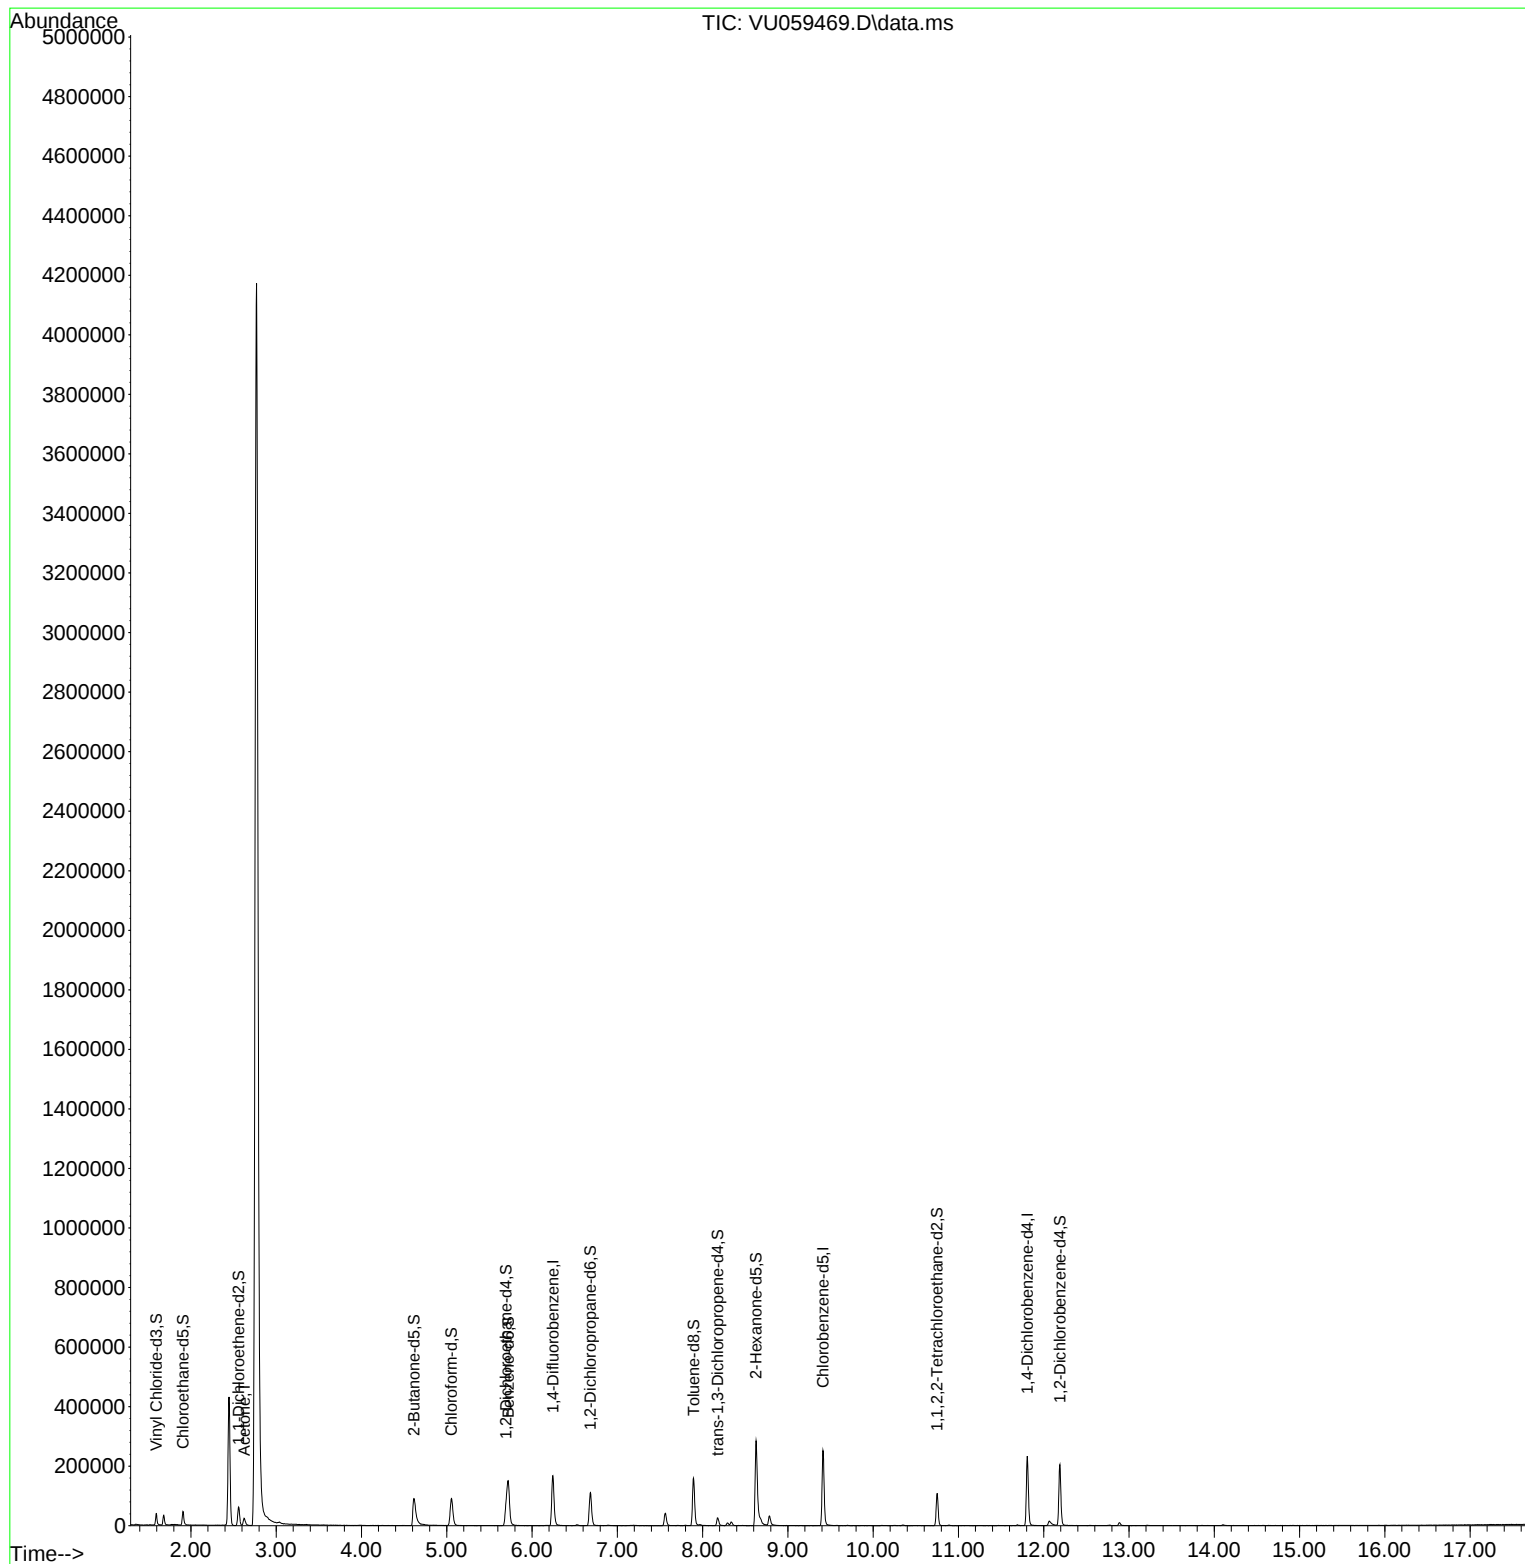

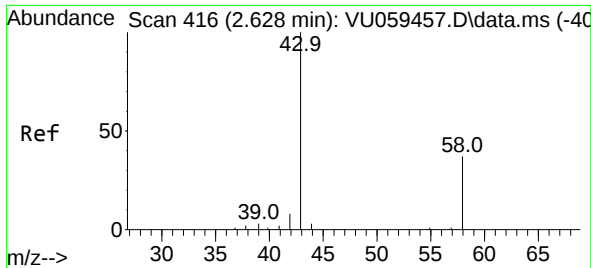

#13
Acetone
Concen: 21.770 ug/L m
RT: 2.624 min Scan# 41
Delta R.T. -0.003 min
Lab File: VU059469.D
Acq: 25 Jun 2024 14:18

Instrument :
MSVOA_U
ClientSampleId :
E1GB3

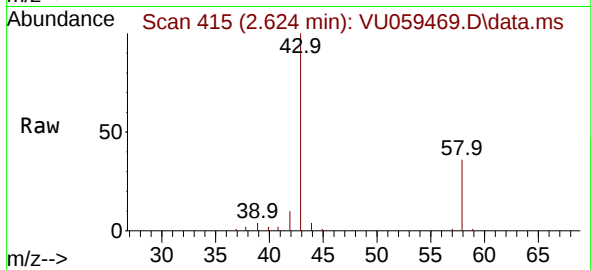

Tgt Ion: 43 Resp: 2927
Ion Ratio Lower Upper
43 100
58 35.9 0.0 68.0

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 06/26/2024
Supervised By :Semsettin Yesilyurt 06/26/2024

