

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062524\
 Data File : VU059472.D
 Acq On : 25 Jun 2024 15:30
 Operator : MD/SY
 Sample : P2961-15
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GE0

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 06/26/2024
 Supervised By :Semsettin Yesilyurt 06/26/2024

Quant Time: Jun 26 04:30:17 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 26 04:26:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	142870	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	150015	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	66401	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	28701	2.889	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	57.800%		
7) Chloroethane-d5	1.907	69	34704	3.631	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	72.600%		
11) 1,1-Dichloroethene-d2	2.560	65	11658	2.829	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	56.600%#		
20) 2-Butanone-d5	4.615	46	138819	67.837	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	135.680%#		
24) Chloroform-d	5.055	84	88263	4.328	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	86.600%		
26) 1,2-Dichloroethane-d4	5.695	65	47065	4.792	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	95.800%		
32) Benzene-d6	5.721	84	150729	3.651	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	73.000%		
36) 1,2-Dichloropropane-d6	6.685	67	55985	4.425	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	88.600%		
41) Toluene-d8	7.894	98	112209	2.924	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	58.400%#		
43) trans-1,3-Dichloroprop...	8.177	79	16136	4.073	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	81.400%		
46) 2-Hexanone-d5	8.627	63	96764	58.787	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	117.580%		
56) 1,1,2,2-Tetrachloroeth...	10.750	84	58302	5.578	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	111.600%		
66) 1,2-Dichlorobenzene-d4	12.190	152	60224	5.096	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	102.000%		
Target Compounds					Qvalue	
13) Acetone	2.624	43	24482m	18.443	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062524\
Data File : VU059472.D
Acq On : 25 Jun 2024 15:30
Operator : MD/SY
Sample : P2961-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1


Instrument :
MSVOA_U
ClientSampleId :
E1GE0

Quant Time: Jun 26 04:30:17 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 26 04:26:20 2024
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 06/26/2024
Supervised By :Semsettin Yesilyurt 06/26/2024

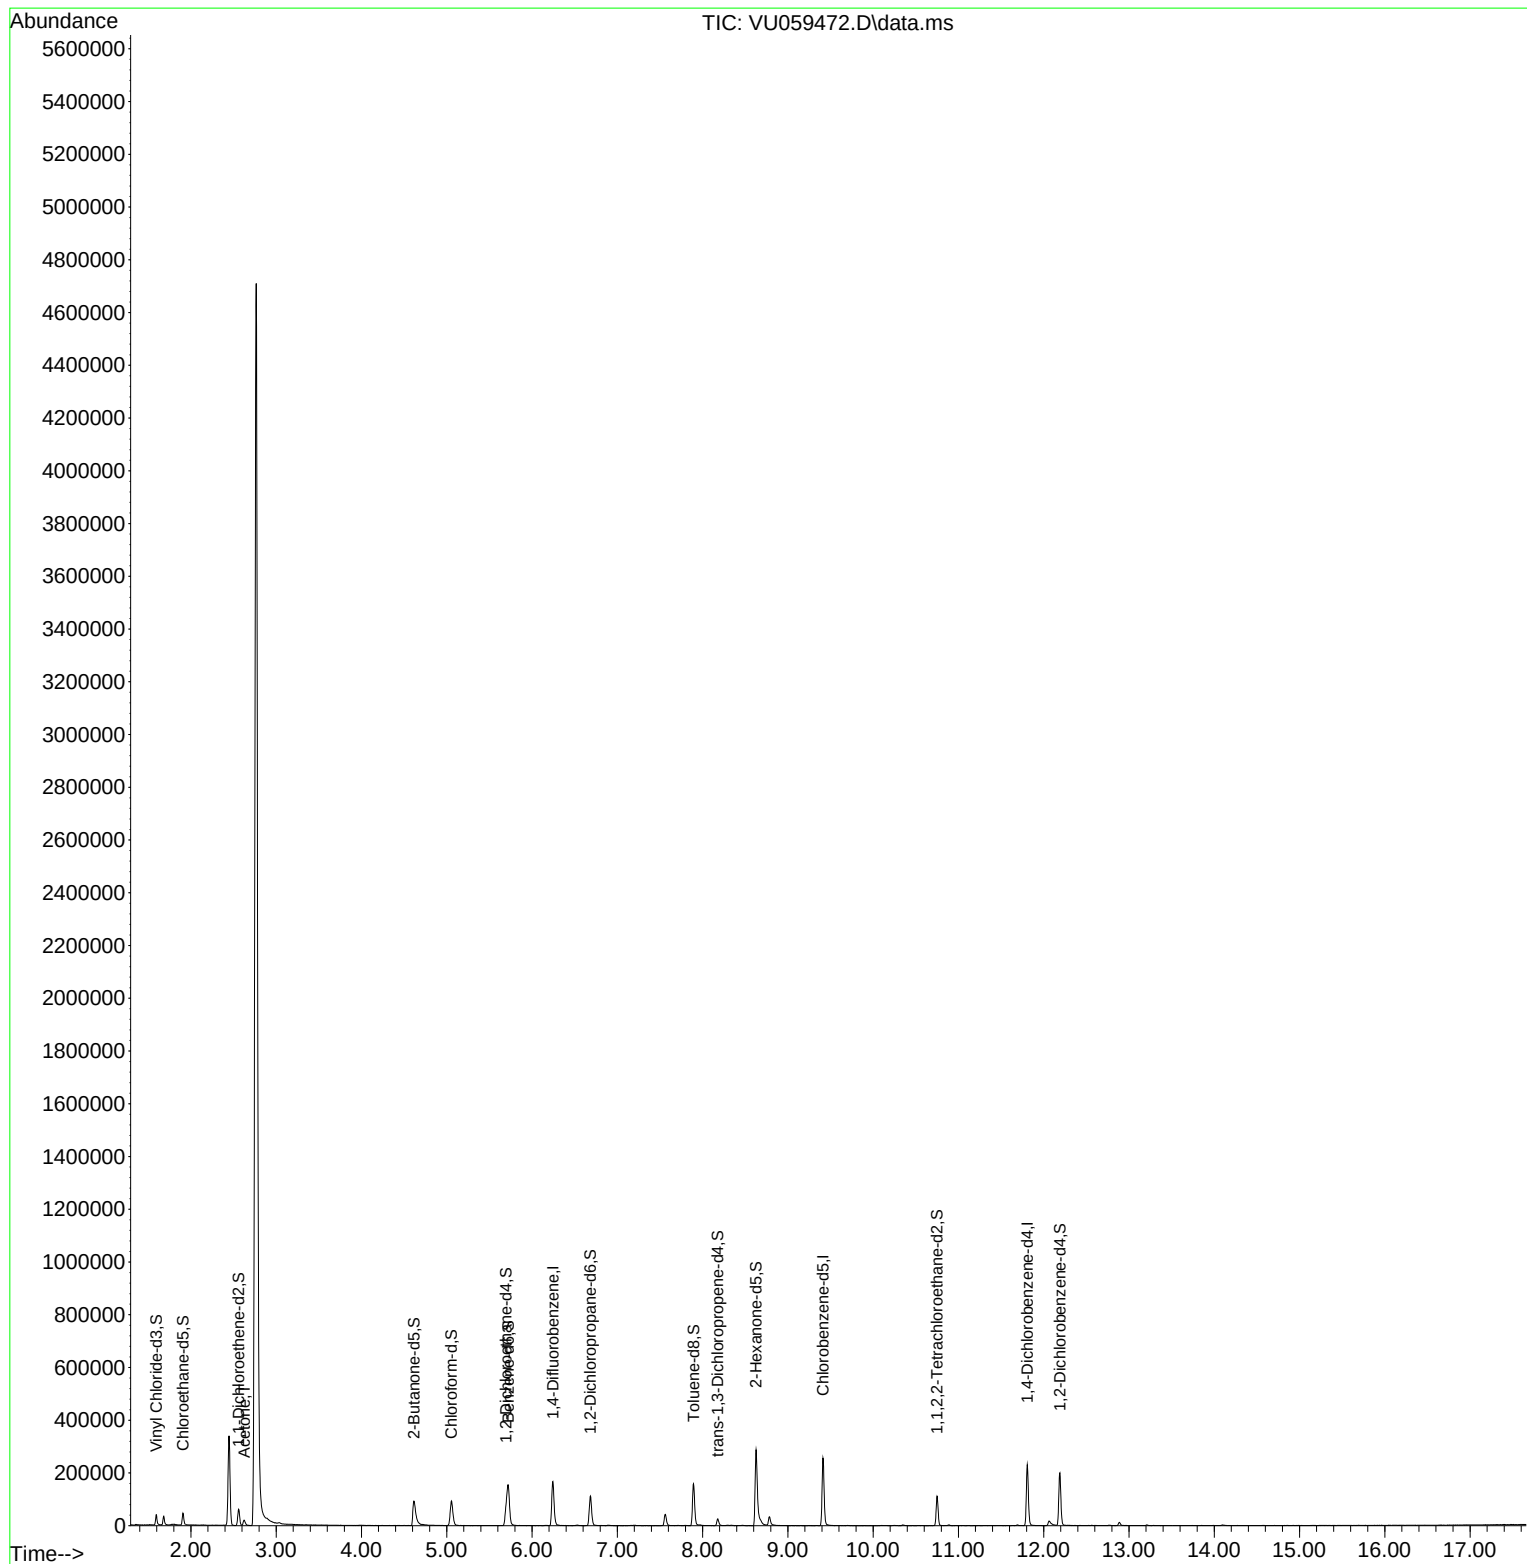

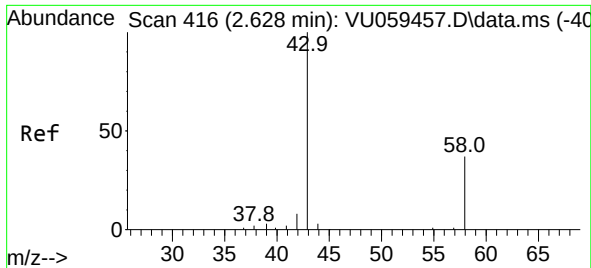

#13

Acetone

Concen: 18.443 ug/L m

RT: 2.624 min Scan# 41

Delta R.T. -0.003 min

Lab File: VU059472.D

Acq: 25 Jun 2024 15:30

Instrument :

MSVOA_U

ClientSampleId :

E1GE0

Tgt Ion: 43 Resp: 2448

Ion Ratio Lower Upper

43 100

58 35.0 0.0 68.0

Manual Integrations

APPROVED

Reviewed By :Mahesh Dadoda 06/26/2024

Supervised By :Semsettin Yesilyurt 06/26/2024

