

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062524\
 Data File : VU059473.D
 Acq On : 25 Jun 2024 15:54
 Operator : MD/SY
 Sample : P2961-16
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GE1

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 06/26/2024
 Supervised By :Semsettin Yesilyurt 06/26/2024

Quant Time: Jun 26 04:30:30 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 26 04:26:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	136111	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	143413	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	63502	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	30702	3.244	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	64.800%	
7) Chloroethane-d5	1.904	69	36096	3.964	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	79.200%	
11) 1,1-Dichloroethene-d2	2.560	65	11825	3.012	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	60.200%	
20) 2-Butanone-d5	4.615	46	142934	73.316	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	146.640%#	
24) Chloroform-d	5.055	84	91045	4.687	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	93.800%	
26) 1,2-Dichloroethane-d4	5.695	65	47662	5.093	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	101.800%	
32) Benzene-d6	5.721	84	153765	3.896	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	78.000%	
36) 1,2-Dichloropropane-d6	6.682	67	57001	4.713	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	94.200%	
41) Toluene-d8	7.894	98	116265	3.169	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	63.400%#	
43) trans-1,3-Dichloroprop...	8.177	79	17141	4.526	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	90.600%	
46) 2-Hexanone-d5	8.627	63	102301	65.012	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	130.020%#	
56) 1,1,2,2-Tetrachloroeth...	10.750	84	59372	5.941	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	118.800%	
66) 1,2-Dichlorobenzene-d4	12.190	152	60421	5.346	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	107.000%	
Target Compounds					Qvalue	
13) Acetone	2.624	43	20804m	16.450	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062524\
Data File : VU059473.D
Acq On : 25 Jun 2024 15:54
Operator : MD/SY
Sample : P2961-16
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1


Instrument :
MSVOA_U
ClientSampleId :
E1GE1

Quant Time: Jun 26 04:30:30 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 26 04:26:20 2024
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 06/26/2024
Supervised By :Semsettin Yesilyurt 06/26/2024

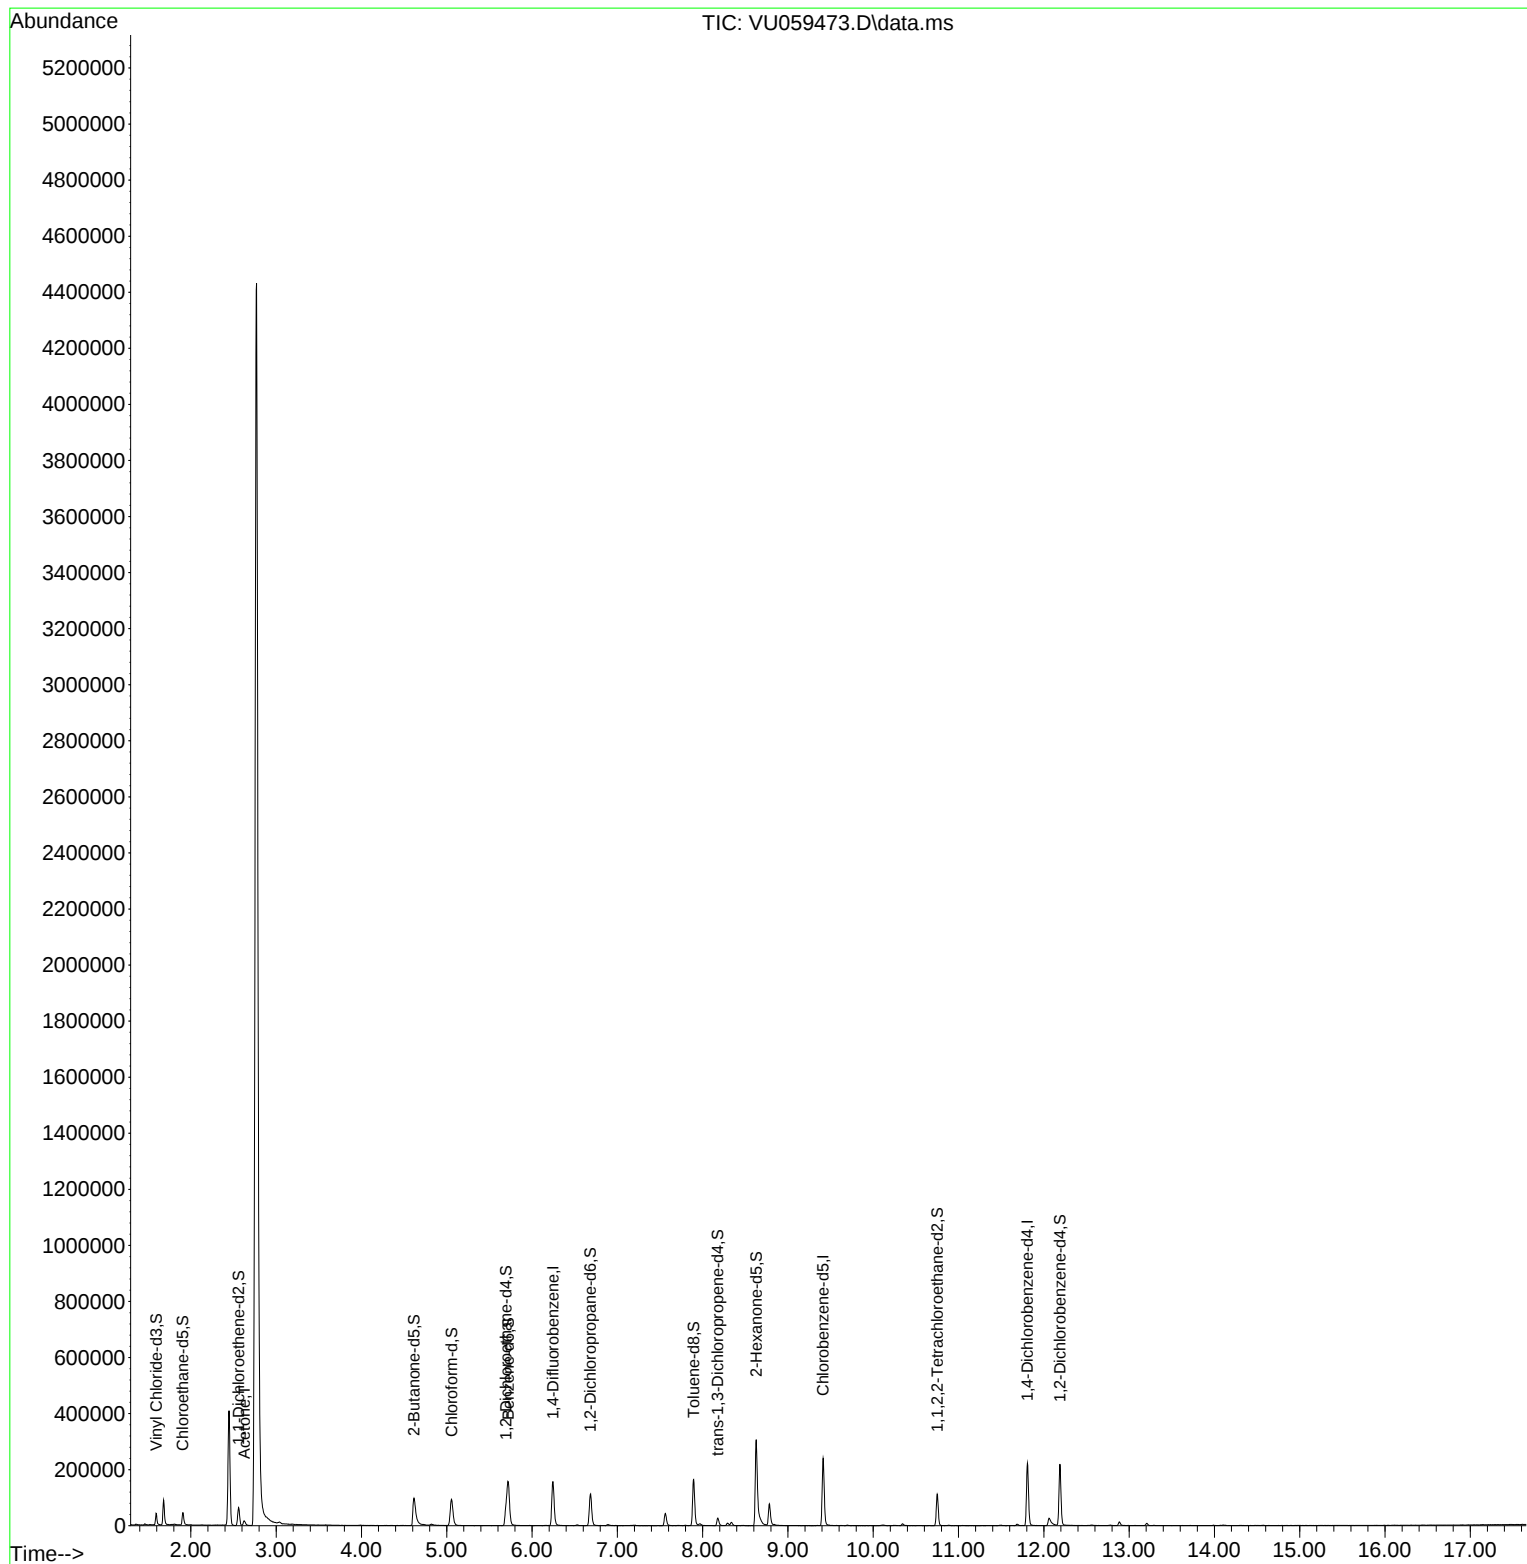

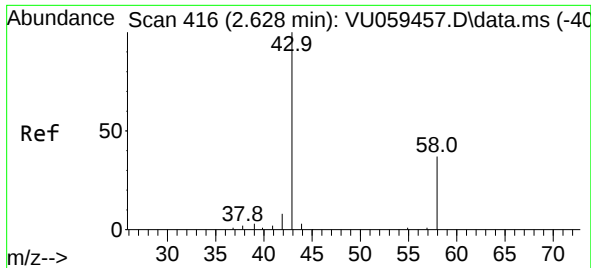

#13
 Acetone
 Concen: 16.450 ug/L m
 RT: 2.624 min Scan# 41
 Delta R.T. -0.003 min
 Lab File: VU059473.D
 Acq: 25 Jun 2024 15:54

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GE1

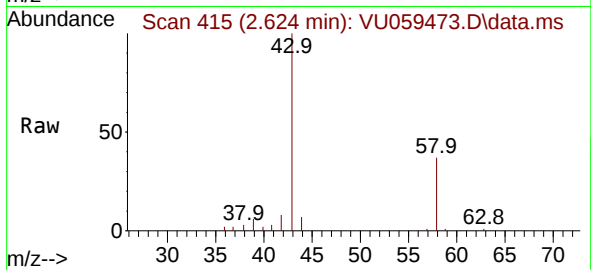

Tgt Ion: 43 Resp: 20804
 Ion Ratio Lower Upper
 43 100
 58 36.8 0.0 68.0

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 06/26/2024
 Supervised By :Semsettin Yesilyurt 06/26/2024

