

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062524\
 Data File : VU059474.D
 Acq On : 25 Jun 2024 16:18
 Operator : MD/SY
 Sample : P2961-19
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GB4

Quant Time: Jun 26 04:30:44 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 26 04:26:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	136572	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	145139	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	65127	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	31449	3.312	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	66.200%
7) Chloroethane-d5	1.907	69	35261	3.859	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	77.200%
11) 1,1-Dichloroethene-d2	2.560	65	11998	3.045	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	61.000%
20) 2-Butanone-d5	4.615	46	137827	70.458	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	140.920%#
24) Chloroform-d	5.055	84	90221	4.629	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.600%
26) 1,2-Dichloroethane-d4	5.695	65	47698	5.080	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.600%
32) Benzene-d6	5.721	84	150757	3.774	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	75.400%
36) 1,2-Dichloropropane-d6	6.685	67	57680	4.712	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.200%
41) Toluene-d8	7.894	98	113930	3.068	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	61.400%#
43) trans-1,3-Dichloroprop...	8.177	79	15538	4.054	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.000%
46) 2-Hexanone-d5	8.627	63	100273	62.965	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	125.940%
56) 1,1,2,2-Tetrachloroeth...	10.749	84	57952	5.730	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	114.600%
66) 1,2-Dichlorobenzene-d4	12.190	152	60324	5.204	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.000%
Target Compounds						
					Qvalue	
13) Acetone	2.621	43	44237	34.862	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062524\
Data File : VU059474.D
Acq On : 25 Jun 2024 16:18
Operator : MD/SY
Sample : P2961-19
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GB4

Quant Time: Jun 26 04:30:44 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 26 04:26:20 2024
Response via : Initial Calibration

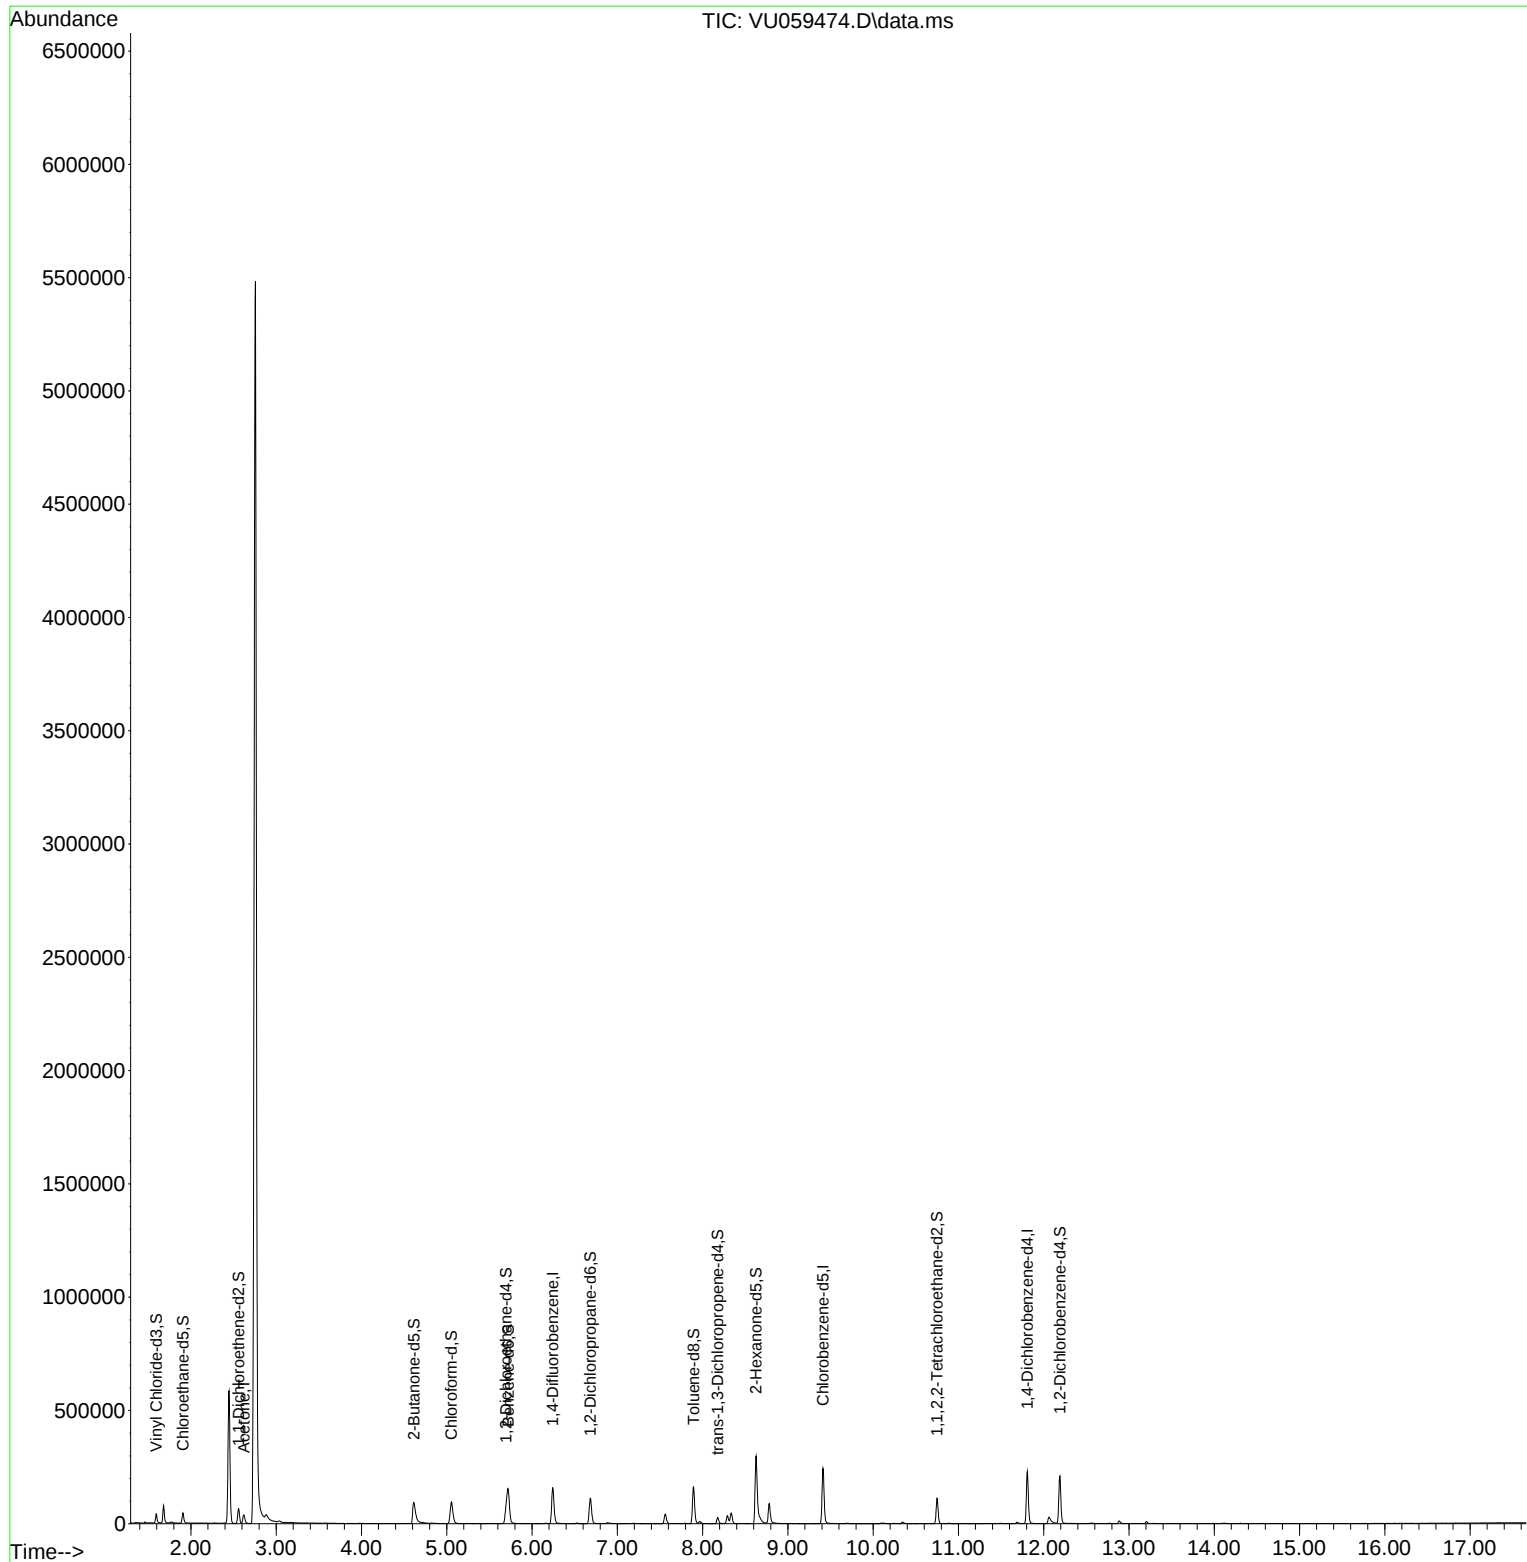

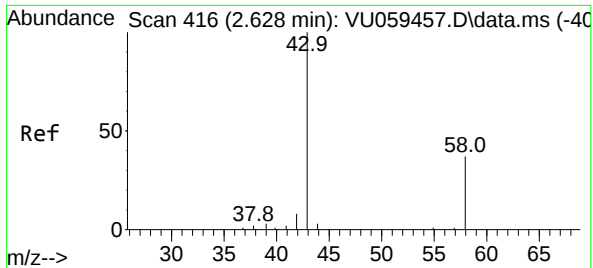

#13
 Acetone
 Concen: 34.862 ug/L
 RT: 2.621 min Scan# 41
 Delta R.T. -0.006 min
 Lab File: VU059474.D
 Acq: 25 Jun 2024 16:18

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GB4

Tgt Ion: 43 Resp: 44237
 Ion Ratio Lower Upper
 43 100
 58 36.6 0.0 68.0

