

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062524\
 Data File : VU059492.D
 Acq On : 26 Jun 2024 00:07
 Operator : MD/SY
 Sample : P3006-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 JMRG6

Quant Time: Jun 26 06:18:21 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 26 05:55:36 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	145604	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	149905	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	63370	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	28014	2.767	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	55.400%
7) Chloroethane-d5	1.907	69	33517	3.441	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	68.800%
11) 1,1-Dichloroethene-d2	2.560	65	11282	2.686	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	53.800%#
20) 2-Butanone-d5	4.621	46	137796	66.073	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	132.140%#
24) Chloroform-d	5.055	84	85020	4.091	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.800%
26) 1,2-Dichloroethane-d4	5.695	65	45295	4.525	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.400%
32) Benzene-d6	5.721	84	139117	3.372	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	67.400%#
36) 1,2-Dichloropropane-d6	6.685	67	52671	4.166	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	83.400%
41) Toluene-d8	7.894	98	103839	2.707	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	54.200%#
43) trans-1,3-Dichloroprop...	8.177	79	14776	3.733	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	74.600%
46) 2-Hexanone-d5	8.627	63	97355	59.189	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	118.380%
56) 1,1,2,2-Tetrachloroeth...	10.749	84	57375	5.493	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	109.800%
66) 1,2-Dichlorobenzene-d4	12.190	152	52588	4.663	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	93.200%
Target Compounds						
					Qvalue	
25) Chloroform	5.081	83	11334	0.543	ug/L	94
34) Trichloroethene	6.537	95	19598	1.590	ug/L	92
47) Tetrachloroethene	8.547	164	55325	5.783	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062524\
Data File : VU059492.D
Acq On : 26 Jun 2024 00:07
Operator : MD/SY
Sample : P3006-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JMRG6

Quant Time: Jun 26 06:18:21 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 26 05:55:36 2024
Response via : Initial Calibration




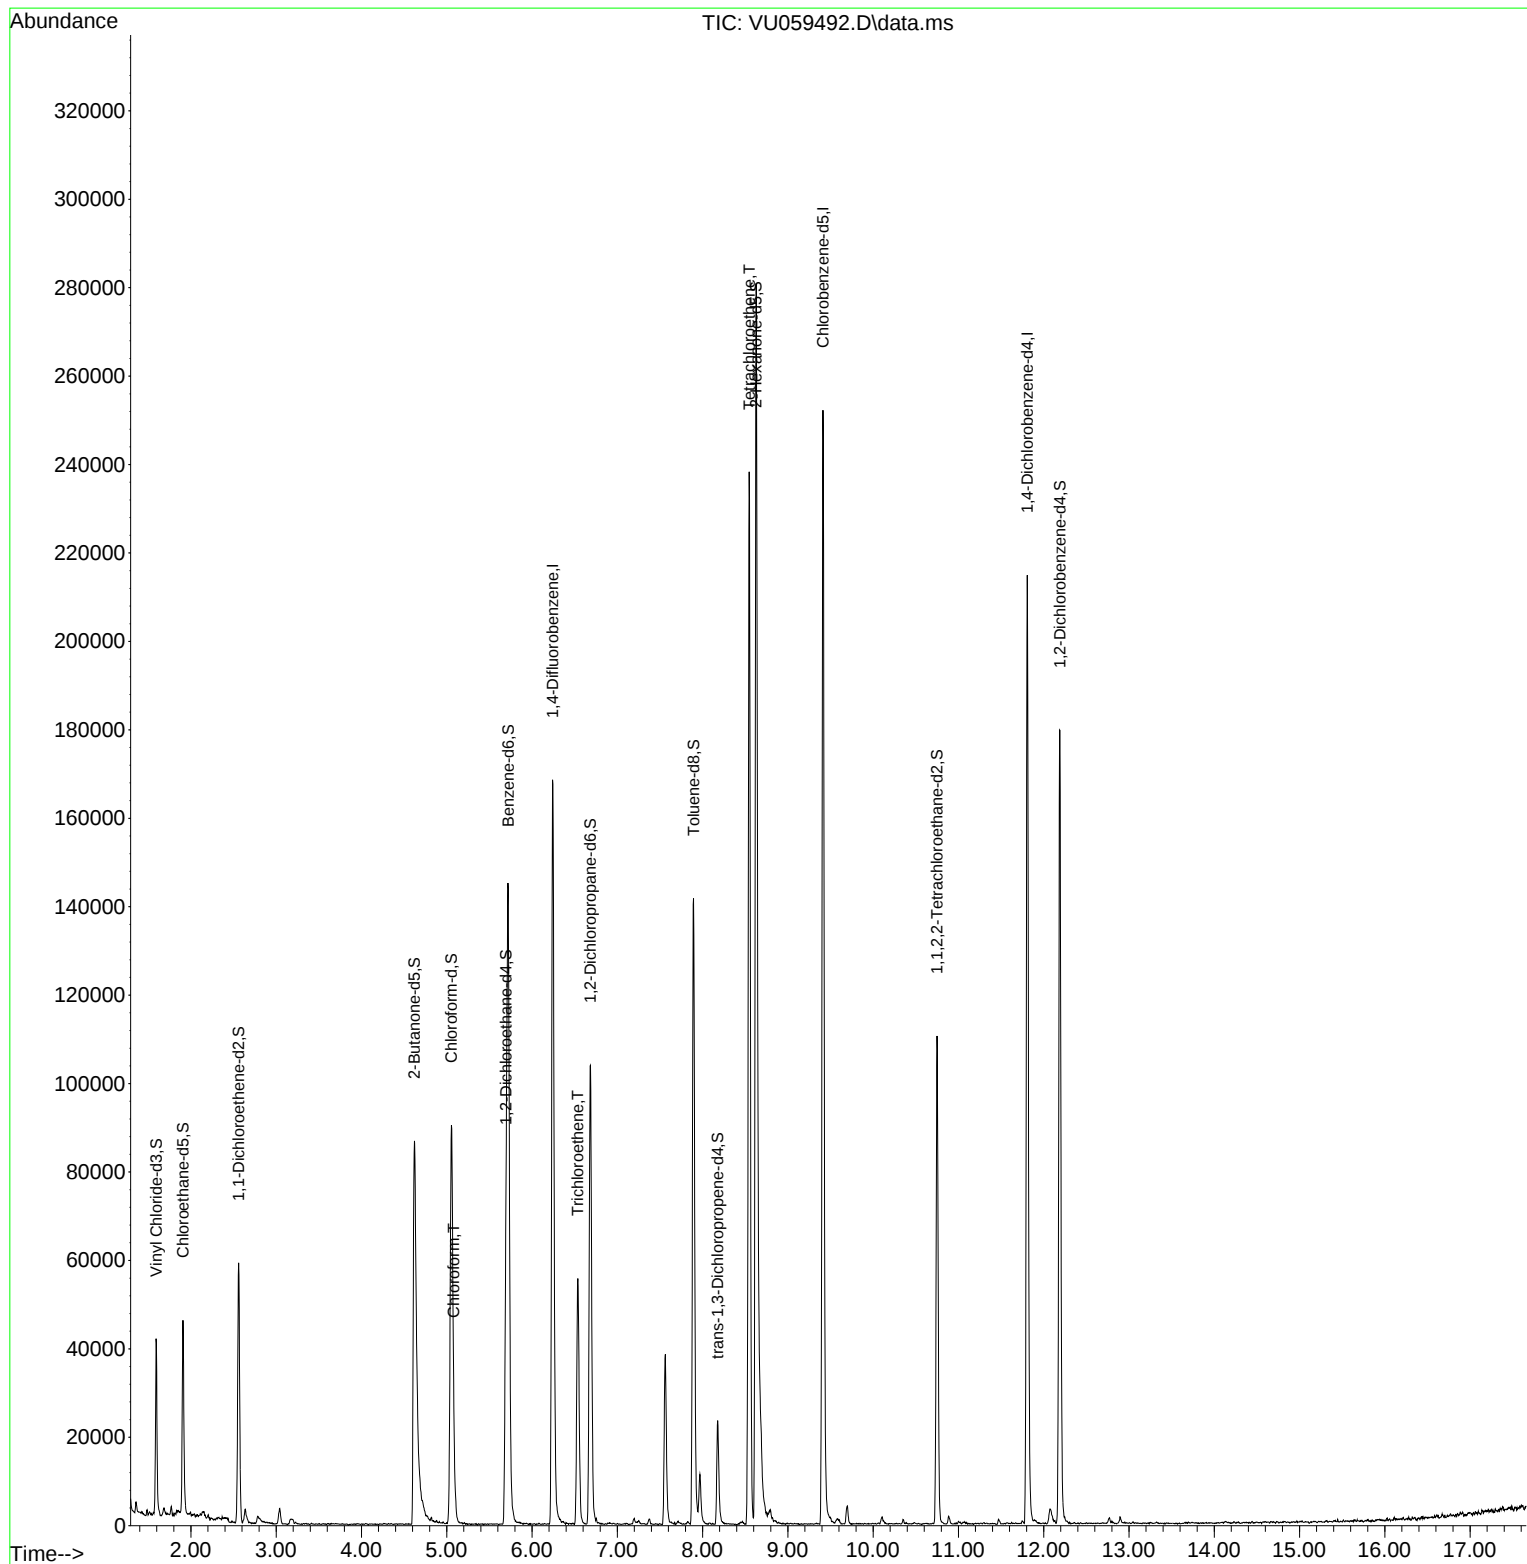


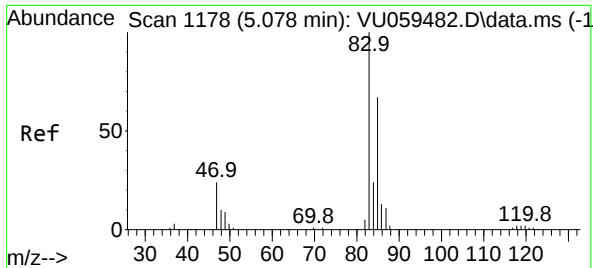

#25
Chloroform
Concen: 0.543 ug/L
RT: 5.081 min Scan# 1178
Delta R.T. 0.003 min
Lab File: VU059492.D
Acq: 26 Jun 2024 00:07




Instrument :
MSVOA_U
ClientSampleId :
JMRG6


Tgt Ion: 83 Resp: 11334
Ion Ratio Lower Upper
83 100
85 68.4 44.7 83.1

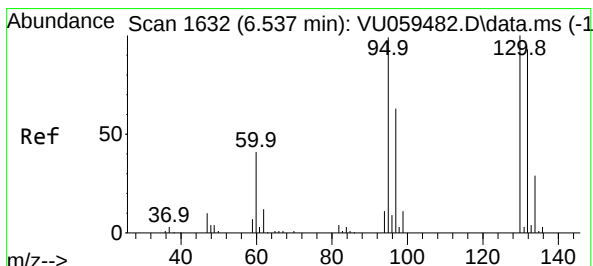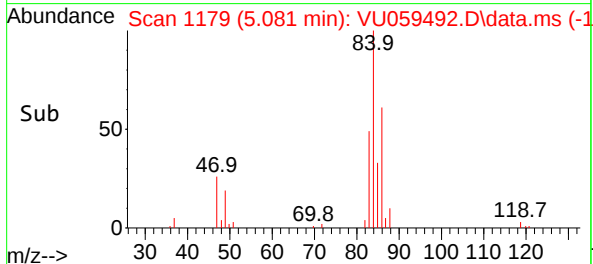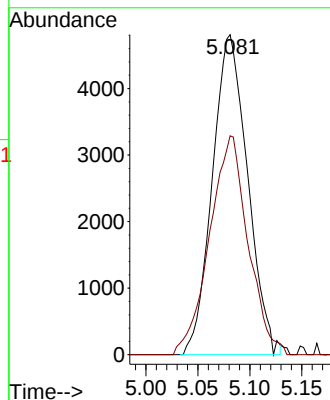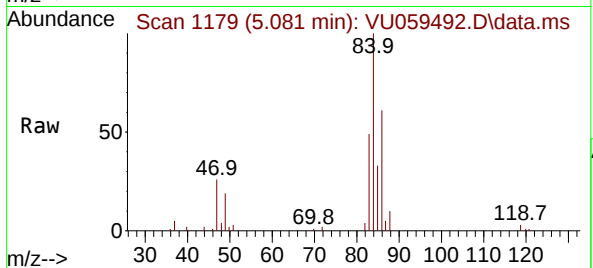

#34
Trichloroethene
Concen: 1.590 ug/L
RT: 6.537 min Scan# 1632
Delta R.T. 0.000 min
Lab File: VU059492.D
Acq: 26 Jun 2024 00:07


Tgt Ion: 95 Resp: 19598
Ion Ratio Lower Upper
95 100
97 67.5 45.3 84.1
132 102.3 64.0 119.0
130 105.8 69.1 128.3

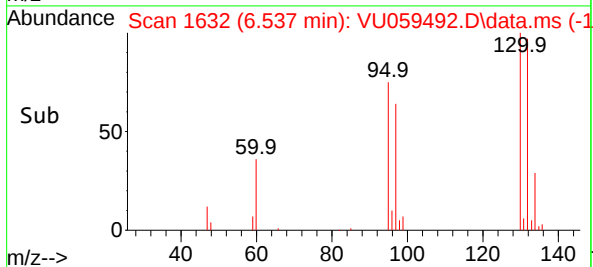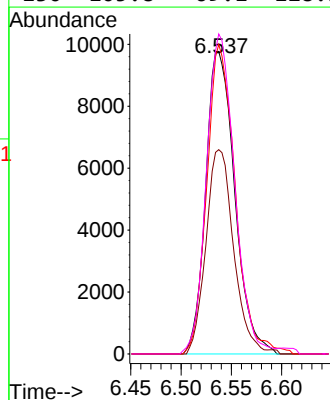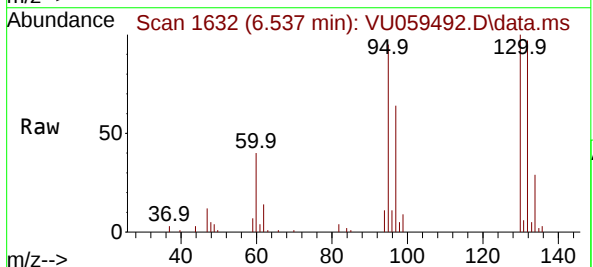

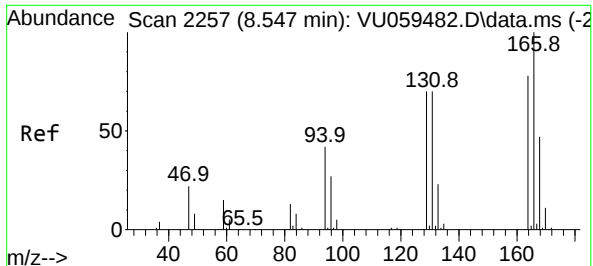

#47
Tetrachloroethene
Concen: 5.783 ug/L
RT: 8.547 min Scan# 21
Delta R.T. -0.000 min
Lab File: VU059492.D
Acq: 26 Jun 2024 00:07

Instrument :
MSVOA_U
ClientSampleId :
JMRG6

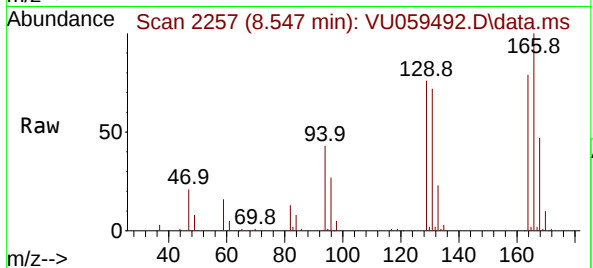

Tgt Ion:	164	Resp:	55325
Ion	Ratio	Lower	Upper
164	100		
129	95.3	70.8	131.4
131	90.6	64.8	120.3
166	126.0	91.1	169.1

