


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062524\
Data File : VU059456.D
Acq On : 25 Jun 2024 08:00
Operator : MD/SY
Sample : BFB165
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB165

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Jun 27 02:36:31 2024

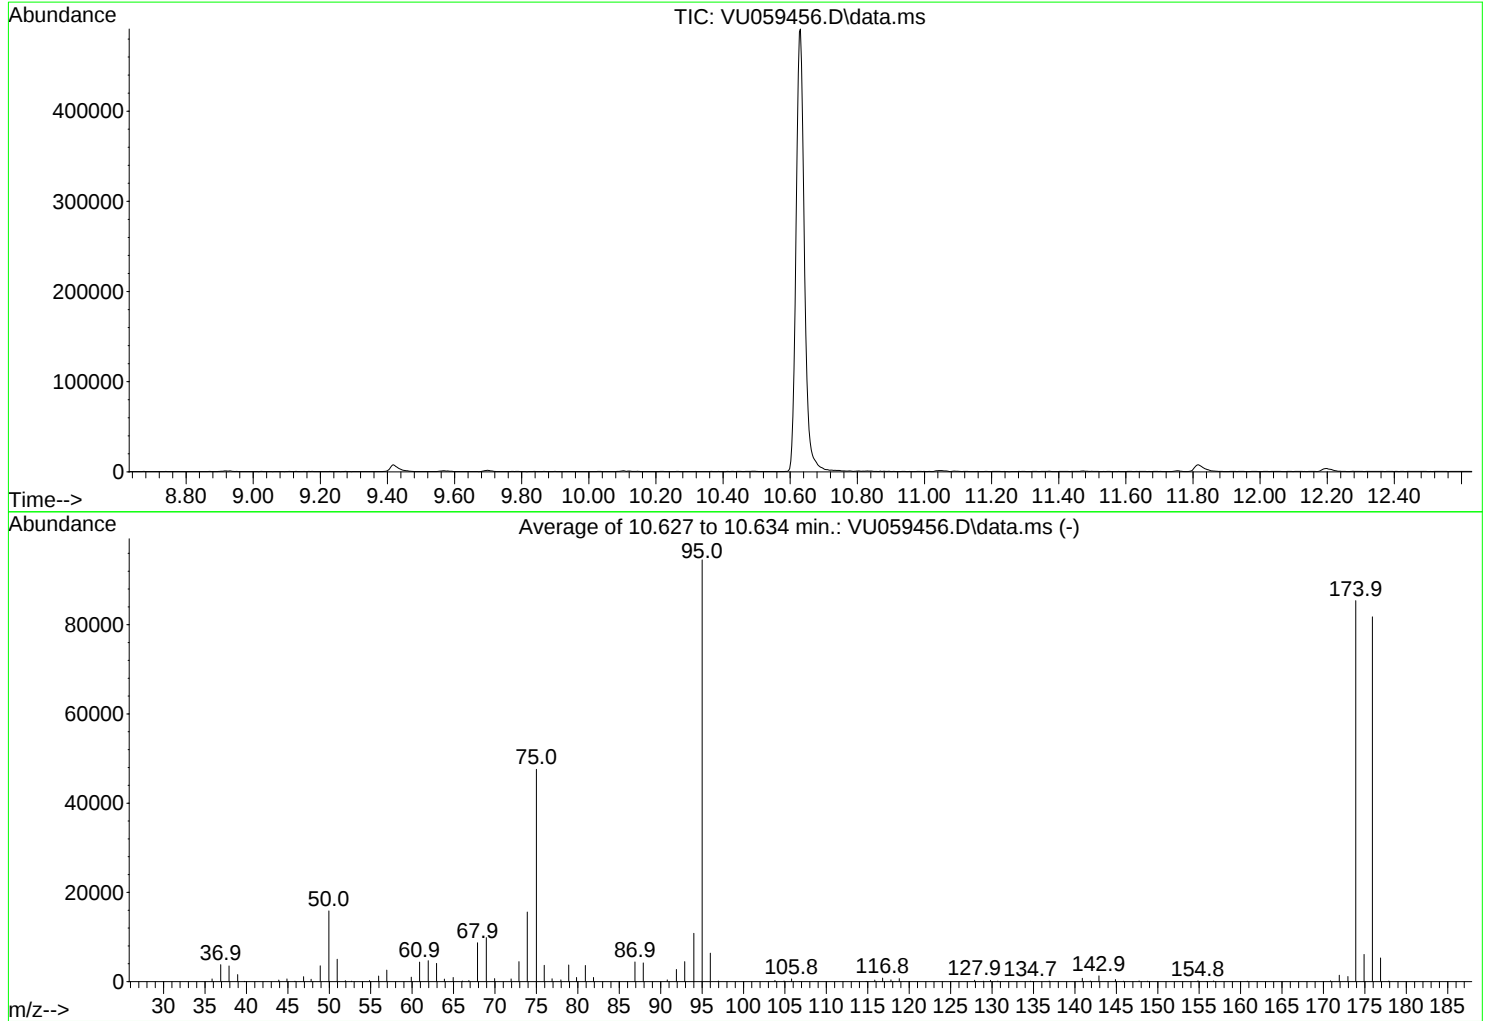

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.8	15869	PASS
75	95	30	80	50.3	47589	PASS
95	95	100	100	100.0	94539	PASS
96	95	5	9	6.8	6392	PASS
173	174	0.00	2	1.4	1155	PASS
174	95	50	120	90.3	85373	PASS
175	174	5	9	7.2	6112	PASS
176	174	95	101	95.8	81755	PASS
177	176	5	9	6.5	5312	PASS

Scan 2890 (10.582 min): VU059456.D\data.ms
BFB165

m/z	Abundance
39.80	158.0
43.90	256.0

Instrument :
MSVOA_U
ClientSampleId :
BFB165

m/z	Abundance
35.90	676.0
36.90	4111.0
37.90	3818.0
39.00	1746.0
39.90	247.0
43.90	660.0
44.80	602.0
45.90	117.0
46.90	1106.0
47.80	591.0
48.90	3804.0
50.00	16768.0
51.00	5002.0
51.90	234.0
52.70	108.0
55.00	261.0
56.00	1387.0
57.00	2723.0
59.90	1055.0
60.90	4766.0
61.90	5117.0
63.00	4150.0
63.90	629.0
65.00	940.0
66.10	131.0
66.90	275.0
67.90	9043.0
69.00	10281.0
69.90	736.0
72.00	650.0
72.90	4649.0
73.90	16270.0
75.00	49320.0
76.00	3851.0
76.90	601.0
77.90	424.0
78.90	4010.0
79.90	936.0
80.90	3845.0
81.90	966.0
86.90	4505.0
87.90	4371.0
90.80	422.0
91.90	2958.0
92.90	4699.0
94.00	11185.0
95.00	96560.0
96.00	6528.0
96.90	154.0
103.80	249.0
104.90	149.0
105.80	642.0
106.80	112.0
115.90	354.0
116.80	801.0
117.80	379.0
118.80	689.0
127.90	326.0
129.00	139.0
129.80	334.0
130.70	134.0
134.60	160.0
136.90	145.0
140.90	728.0
141.90	141.0
142.90	1403.0
144.90	464.0
145.90	117.0
147.80	219.0
148.80	100.0
154.80	238.0
156.80	162.0
160.80	119.0
170.90	210.0
171.90	1474.0
173.00	1105.0
173.90	86504.0
174.90	6195.0
175.90	80536.0
176.90	5414.0
177.90	151.0

Instrument :
MSVOA_U
ClientSampleId :
BFB165

m/z	Abundance
35.90	609.0
36.90	3939.0
37.90	3607.0
39.00	1611.0
39.80	244.0
43.90	617.0
44.90	614.0
45.80	126.0
46.90	1166.0
47.80	542.0
48.90	3609.0
50.00	16247.0
51.00	5139.0
51.90	233.0
52.70	114.0
54.80	242.0
55.90	1283.0
57.00	2722.0
59.90	1034.0
60.90	4452.0
62.00	4793.0
63.00	4249.0
63.90	565.0
64.90	978.0
66.00	161.0
66.90	236.0
67.90	9040.0
68.90	10156.0
69.90	695.0
71.90	655.0
72.90	4607.0
73.90	16132.0
75.00	48776.0
76.00	3795.0
76.90	636.0
77.90	394.0
78.90	3803.0
79.90	934.0
80.90	3699.0
81.90	957.0
86.90	4573.0
87.90	4284.0
90.80	393.0
91.90	2842.0
92.90	4674.0
94.00	11130.0
95.00	97456.0
96.00	6562.0
97.00	167.0
103.80	300.0
104.90	158.0
105.80	627.0
114.80	119.0
115.80	365.0
116.80	775.0
117.80	429.0
118.80	703.0
127.90	322.0
128.90	111.0
129.80	327.0
130.70	145.0
134.70	138.0
136.90	152.0
140.90	776.0
141.80	166.0
142.90	1356.0
144.90	465.0
145.80	110.0
147.70	181.0
148.80	124.0
154.90	228.0
155.90	106.0
156.70	167.0
160.80	120.0
170.90	193.0
171.90	1483.0
172.90	1183.0
173.90	87968.0
174.90	6242.0
175.90	84432.0
176.90	5462.0
177.90	133.0

Instrument :
MSVOA_U
ClientSampleId :
BFB165

m/z	Abundance
35.80	606.0
36.90	3386.0
37.90	3150.0
38.90	1339.0
39.70	242.0
43.90	619.0
45.00	591.0
45.80	123.0
46.90	1037.0
47.80	517.0
48.90	3243.0
49.90	14592.0
50.90	4908.0
52.00	237.0
52.70	122.0
54.80	215.0
55.90	1132.0
56.90	2361.0
59.90	944.0
60.90	3887.0
62.00	4162.0
62.90	3907.0
63.90	489.0
64.90	895.0
66.00	118.0
66.80	212.0
67.90	8083.0
68.90	9202.0
70.00	630.0
72.00	586.0
72.90	4185.0
73.90	14393.0
75.00	44672.0
75.90	3343.0
76.90	679.0
78.00	330.0
78.90	3359.0
79.80	902.0
80.90	3351.0
81.90	850.0
86.00	122.0
86.90	4159.0
87.90	3970.0
90.80	346.0
91.90	2409.0
92.90	4137.0
94.00	10182.0
95.00	89600.0
96.00	6085.0
97.00	162.0
103.80	367.0
104.90	158.0
105.80	520.0
114.80	154.0
115.80	328.0
116.80	770.0
117.80	372.0
118.80	650.0
127.90	319.0
128.90	106.0
129.80	258.0
130.70	139.0
134.90	125.0
136.90	122.0
140.90	812.0
141.80	181.0
142.90	1167.0
144.90	439.0
145.80	111.0
147.80	138.0
148.80	106.0
154.90	204.0
156.70	190.0
160.80	130.0
170.80	181.0
171.90	1332.0
172.90	1178.0
173.90	81648.0
174.90	5898.0
175.90	80296.0
176.90	5059.0
177.90	103.0

Instrument :
MSVOA_U
ClientSampleId :
BFB165