
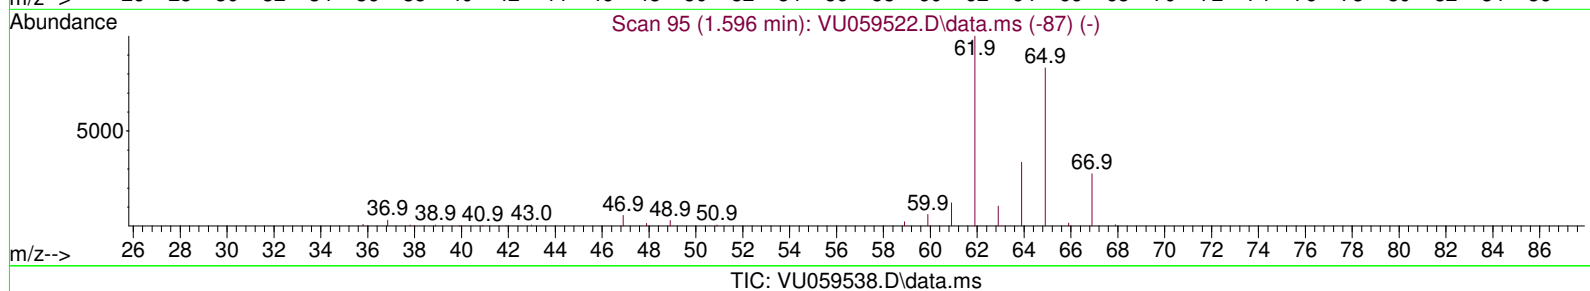
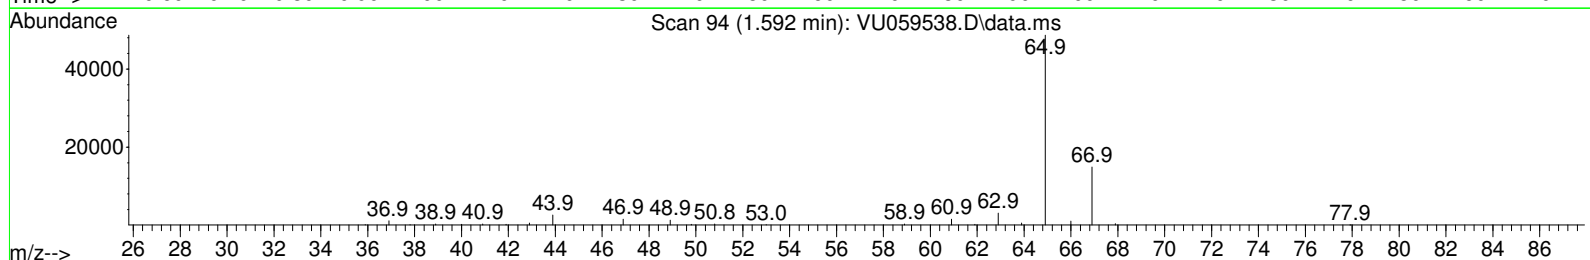


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
Data File : VU059538.D
Acq On : 26 Jun 2024 20:57
Operator : MD/SY
Sample : P3055-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Jun 27 04:55:42 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jun 27 04:10:00 2024
Response via : Initial Calibration

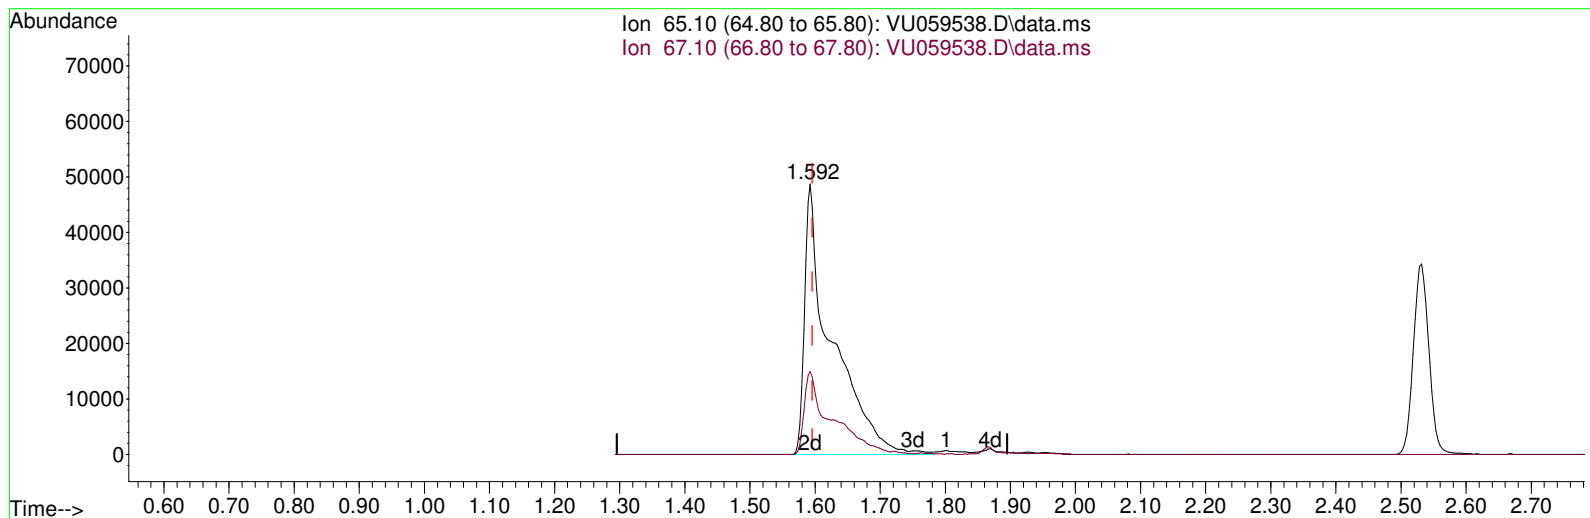

(4) Vinyl Chloride-d3 (S)

1.592min (-0.003) 49.35 ug/L m

response 139475

Ion	Exp%	Act%
65.10	100.00	100.00
67.10	31.60	0.06#
0.00	0.00	0.00
0.00	0.00	0.00