

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
 Data File : VU059530.D
 Acq On : 26 Jun 2024 17:39
 Operator : MD/SY
 Sample : P2909-12ME
 Misc : 4.30g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4CP1ME

Quant Time: Jun 27 04:37:05 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jun 27 04:10:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.239	114	216132	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	220854	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.811	152	109273	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	66867	51.672	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 103.340%			
7) Chloroethane-d5	1.869	69	32731	29.527	ug/L	-0.04
Spiked Amount 50.000	Range 70 - 130		Recovery = 59.060%#			
11) 1,1-Dichloroethene-d2	2.538	63	87856	34.395	ug/L	-0.03
Spiked Amount 50.000	Range 60 - 125		Recovery = 68.780%			
21) 2-Butanone-d5	4.621	46	117169	96.060	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 96.060%			
24) Chloroform-d	5.052	84	129317	50.198	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 100.400%			
26) 1,2-Dichloroethane-d4	5.692	65	83182	52.682	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 105.360%			
32) Benzene-d6	5.714	84	269600	53.187	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 106.380%			
36) 1,2-Dichloropropane-d6	6.682	67	86768	49.645	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 99.300%			
41) Toluene-d8	7.891	98	231417	53.780	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 107.560%			
43) trans-1,3-Dichloroprop...	8.174	79	37619	53.249	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 106.500%			
47) 2-Hexanone-d5	8.637	63	82833	102.489	ug/L	0.01
Spiked Amount 100.000	Range 45 - 130		Recovery = 102.490%			
56) 1,1,2,2-Tetrachloroeth...	10.753	84	151720	51.292	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 102.580%			
66) 1,2-Dichlorobenzene-d4	12.190	152	99781	61.188	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 122.380%#			
Target Compounds						Qvalue
15) Methyl Acetate	2.946	43	25225	11.107	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
Data File : VU059530.D
Acq On : 26 Jun 2024 17:39
Operator : MD/SY
Sample : P2909-12ME
Misc : 4.30g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4CP1ME

Quant Time: Jun 27 04:37:05 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jun 27 04:10:00 2024
Response via : Initial Calibration

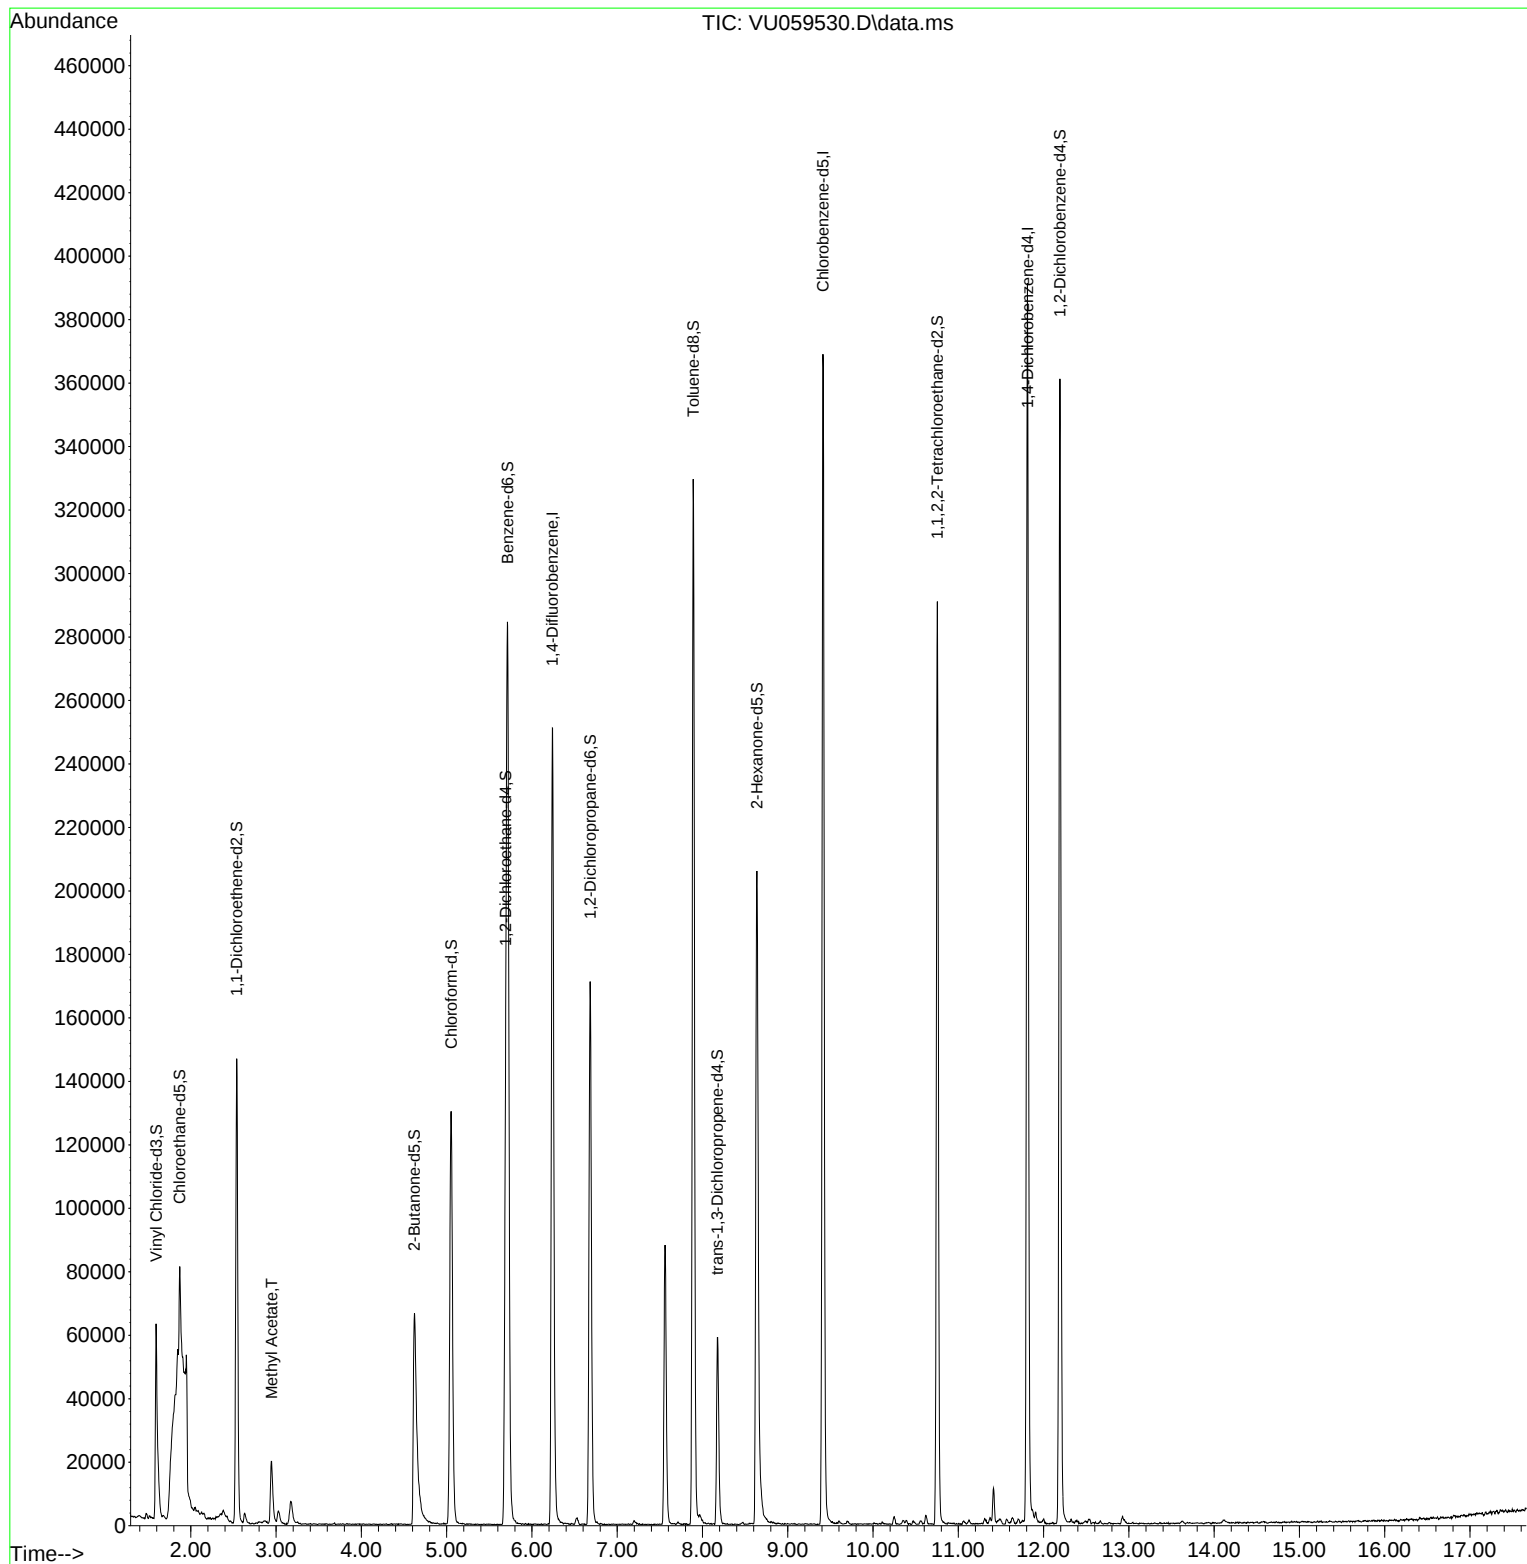

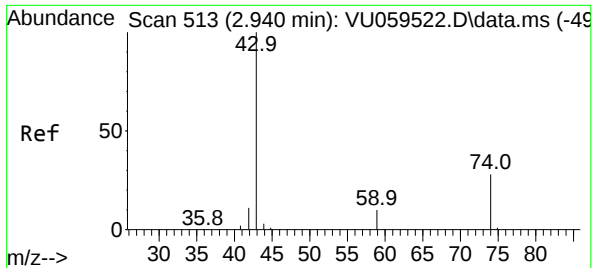

#15
Methyl Acetate
Concen: 11.107 ug/L
RT: 2.946 min Scan# 51
Delta R.T. 0.006 min
Lab File: VU059530.D
Acq: 26 Jun 2024 17:39

Instrument :
MSVOA_U
ClientSampleId :
A4CP1ME

Tgt Ion: 43 Resp: 25225
Ion Ratio Lower Upper
43 100
74 29.5 20.8 31.2

