

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
 Data File : VU059540.D
 Acq On : 26 Jun 2024 22:27
 Operator : MD/SY
 Sample : P3055-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08D9

Quant Time: Jun 27 05:04:27 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jun 27 04:10:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	197837	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	203846	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	89355	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	64578	54.518	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	109.040%
7) Chloroethane-d5	1.907	69	53404	52.631	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	105.260%
11) 1,1-Dichloroethene-d2	2.557	63	79123	33.841	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	67.680%
21) 2-Butanone-d5	4.615	46	102505	91.809	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	91.810%
24) Chloroform-d	5.055	84	116670	49.477	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.960%
26) 1,2-Dichloroethane-d4	5.695	65	73035	50.533	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.060%
32) Benzene-d6	5.721	84	235540	50.344	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.680%
36) 1,2-Dichloropropane-d6	6.682	67	78543	48.689	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	97.380%
41) Toluene-d8	7.894	98	201321	50.689	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.380%
43) trans-1,3-Dichloroprop...	8.177	79	29249	44.856	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	89.720%
47) 2-Hexanone-d5	8.627	63	61229	82.079	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	82.080%
56) 1,1,2,2-Tetrachloroeth...	10.749	84	122034	44.699	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	89.400%
66) 1,2-Dichlorobenzene-d4	12.190	152	73534	55.145	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	110.280%
Target Compounds						
13) Acetone	2.624	43	6145	4.682	ug/L	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
Data File : VU059540.D
Acq On : 26 Jun 2024 22:27
Operator : MD/SY
Sample : P3055-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08D9

Quant Time: Jun 27 05:04:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jun 27 04:10:00 2024
Response via : Initial Calibration

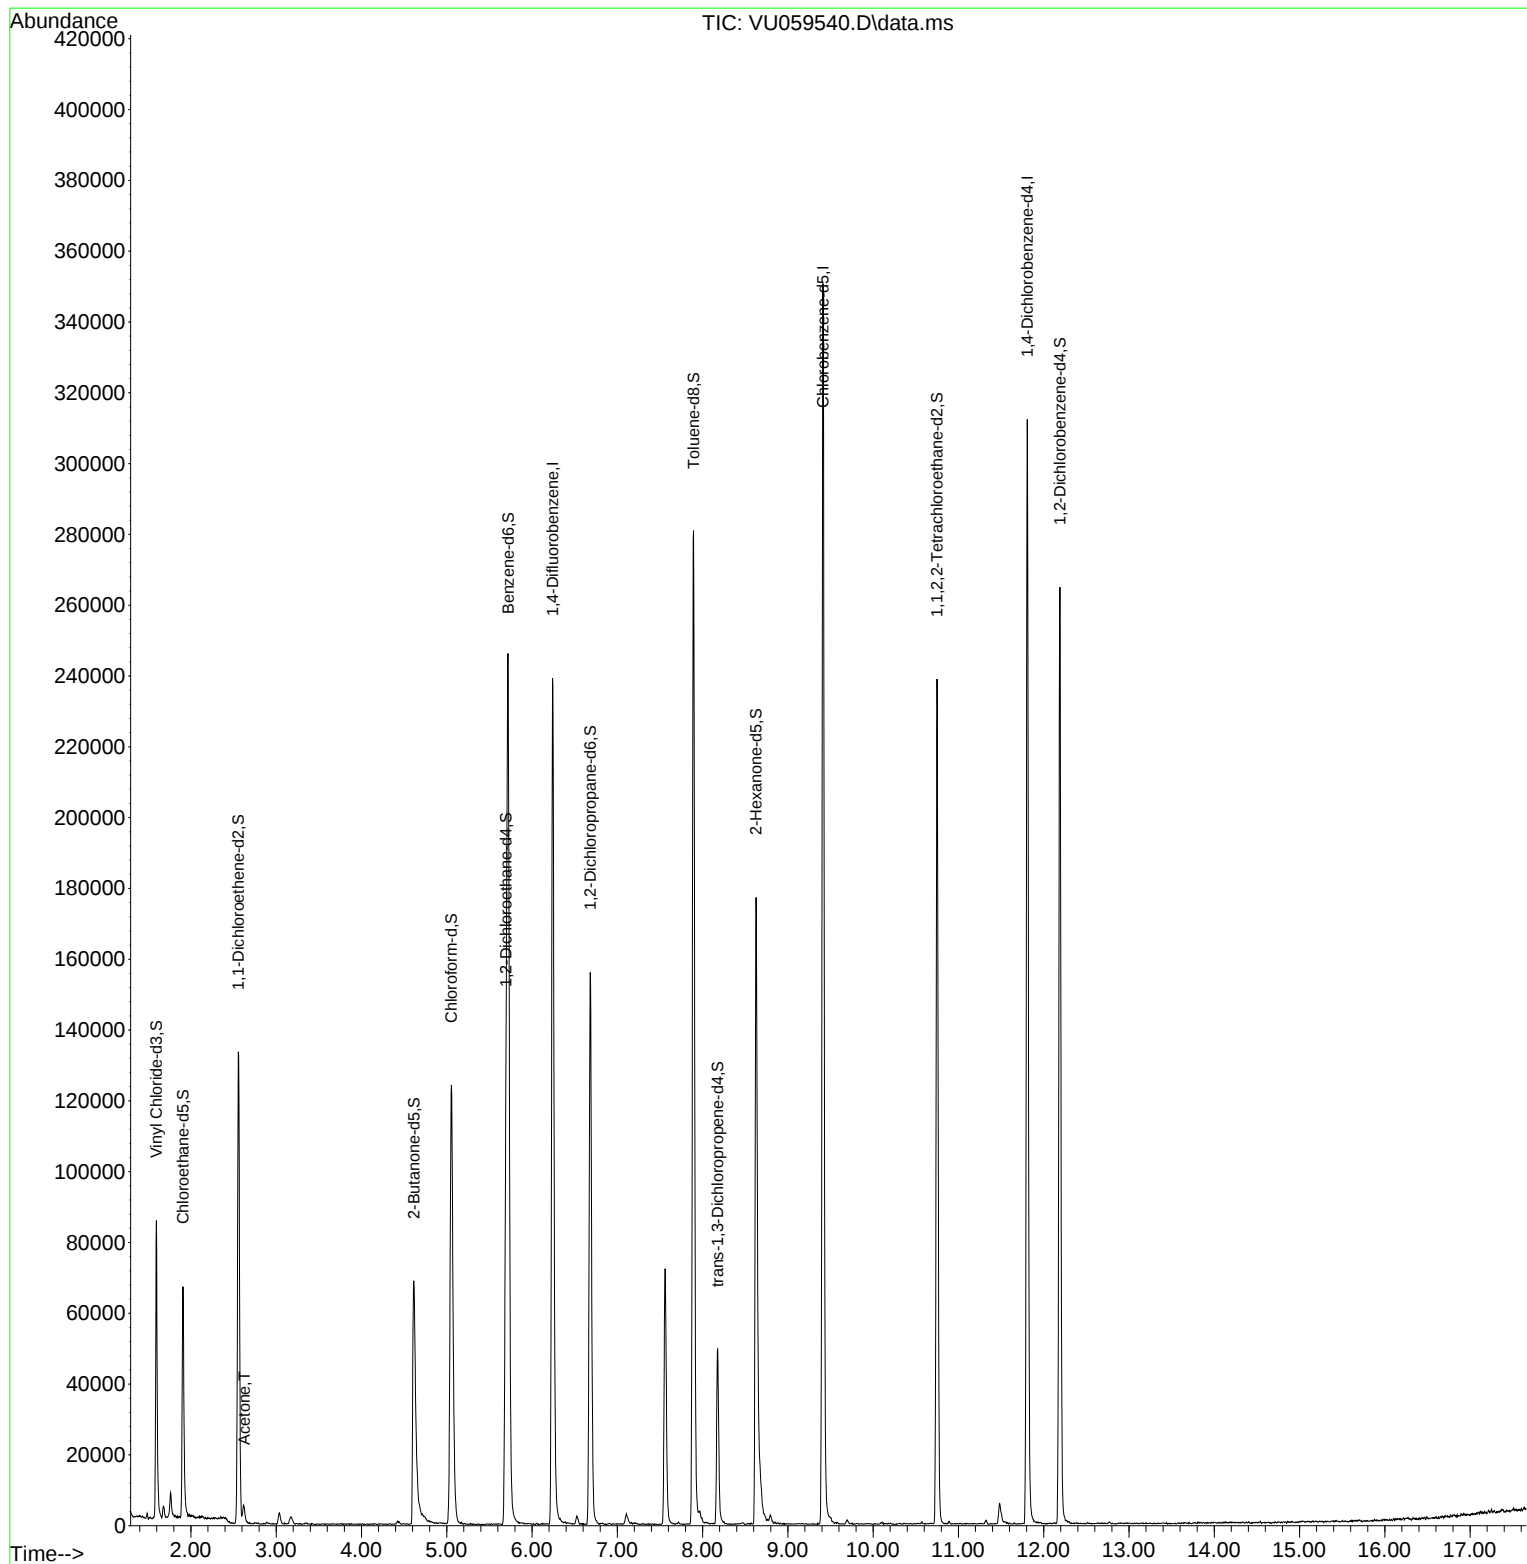

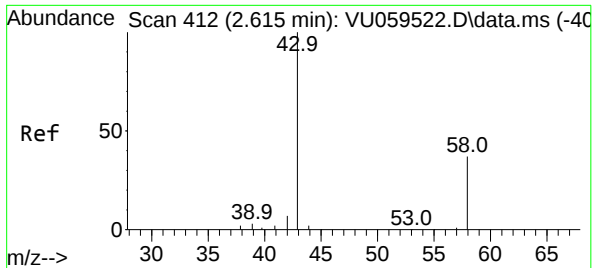

#13
 Acetone
 Concen: 4.682 ug/L
 RT: 2.624 min Scan# 41
 Delta R.T. 0.010 min
 Lab File: VU059540.D
 Acq: 26 Jun 2024 22:27

Instrument :
 MSVOA_U
 ClientSampleId :
 E08D9

Tgt Ion: 43 Resp: 6145
 Ion Ratio Lower Upper
 43 100
 58 36.6 0.0 68.8

