

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
 Data File : VU059523.D
 Acq On : 26 Jun 2024 15:00
 Operator : MD/SY
 Sample : VU0626MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK085

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M

Title : VOC Analysis

Signal : TIC: VU059523.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	114	rBV	79673	95590	14.74%	1.853%
2	1.760	141	146	152	rVB2	4763	5649	0.87%	0.109%
3	1.908	184	192	207	rBV	63043	89657	13.83%	1.738%
4	2.560	384	395	409	rBV	131074	211481	32.61%	4.099%
5	2.689	433	435	440	rBV2	232	211	0.03%	0.004%
6	2.750	451	454	458	rVV2	335	194	0.03%	0.004%
7	2.779	459	463	465	rVV2	462	365	0.06%	0.007%
8	2.792	465	467	477	rVB3	632	705	0.11%	0.014%
9	2.875	489	493	499	rBV2	314	367	0.06%	0.007%
10	3.039	534	544	555	rVB2	4622	9081	1.40%	0.176%
11	3.364	641	645	651	rBV2	149	197	0.03%	0.004%
12	3.573	705	710	717	rVB2	333	366	0.06%	0.007%
13	3.609	717	721	723	rBV2	186	171	0.03%	0.003%
14	3.715	750	754	756	rBV	288	190	0.03%	0.004%
15	3.946	822	826	831	rVB2	241	207	0.03%	0.004%
16	4.200	899	905	910	rBV2	405	589	0.09%	0.011%
17	4.422	971	974	979	rVB	269	234	0.04%	0.005%
18	4.483	989	993	997	rVB2	241	204	0.03%	0.004%
19	4.567	1014	1019	1023	rVB2	309	282	0.04%	0.005%
20	4.615	1024	1034	1064	rBV	61061	152450	23.51%	2.955%
21	5.055	1155	1171	1200	rBV	118171	261821	40.38%	5.075%
22	5.232	1223	1226	1229	rVB2	395	211	0.03%	0.004%
23	5.338	1257	1259	1265	rVB	218	182	0.03%	0.004%
24	5.371	1265	1269	1274	rBV2	174	179	0.03%	0.003%
25	5.718	1357	1377	1400	rBV3	236432	648473	100.00%	12.569%
26	5.901	1431	1434	1437	rBV2	268	200	0.03%	0.004%
27	5.988	1459	1461	1464	rBV3	296	186	0.03%	0.004%
28	6.039	1474	1477	1483	rBV3	527	495	0.08%	0.010%
29	6.145	1503	1510	1514	rBV2	264	400	0.06%	0.008%
30	6.245	1528	1541	1560	rBV	231950	450231	69.43%	8.727%
31	6.432	1596	1599	1605	rVB2	365	280	0.04%	0.005%
32	6.525	1622	1628	1640	rVB5	1966	3735	0.58%	0.072%
33	6.596	1646	1650	1652	rBV2	258	187	0.03%	0.004%
34	6.686	1661	1678	1703	rBV	149394	293019	45.19%	5.680%
35	6.817	1717	1719	1722	rVB	431	232	0.04%	0.004%
36	6.840	1722	1726	1733	rVB3	282	294	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
 Data File : VU059523.D
 Acq On : 26 Jun 2024 15:00
 Operator : MD/SY
 Sample : VU0626MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK085

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

37	7.001	1772	1776	1781	rBV2	157	159	0.02%	0.003%
38	7.107	1803	1809	1811	rBV	183	181	0.03%	0.004%
39	7.194	1832	1836	1839	rBV3	346	307	0.05%	0.006%
40	7.261	1852	1857	1859	rBV	197	165	0.03%	0.003%
41	7.419	1902	1906	1911	rVV2	155	173	0.03%	0.003%
42	7.448	1912	1915	1921	rVB2	255	289	0.04%	0.006%
43	7.563	1939	1951	1967	rBV2	74660	133086	20.52%	2.580%
44	7.740	2004	2006	2009	rVB2	398	182	0.03%	0.004%
45	7.769	2012	2015	2021	rVB	308	222	0.03%	0.004%
46	7.895	2041	2054	2084	rBV	279185	491648	75.82%	9.530%
47	8.177	2131	2142	2161	rBV	51581	89795	13.85%	1.740%
48	8.512	2241	2246	2250	rBV2	204	249	0.04%	0.005%
49	8.560	2257	2261	2264	rVB2	321	250	0.04%	0.005%
50	8.628	2272	2282	2320	rBV	156028	312893	48.25%	6.065%
51	8.907	2365	2369	2370	rBV2	273	157	0.02%	0.003%
52	8.975	2387	2390	2395	rBV	180	180	0.03%	0.003%
53	9.280	2482	2485	2491	rBV2	163	185	0.03%	0.004%
54	9.412	2514	2526	2546	rBV	347767	583362	89.96%	11.307%
55	9.653	2598	2601	2604	rVB2	248	164	0.03%	0.003%
56	9.679	2604	2609	2612	rBV2	246	165	0.03%	0.003%
57	9.705	2612	2617	2622	rBV2	377	420	0.06%	0.008%
58	9.837	2654	2658	2661	rBV2	236	202	0.03%	0.004%
59	9.927	2683	2686	2690	rVB2	305	222	0.03%	0.004%
60	9.975	2697	2701	2706	rBV2	149	156	0.02%	0.003%
61	10.004	2707	2710	2715	rVB2	196	176	0.03%	0.003%
62	10.136	2748	2751	2755	rBV2	352	256	0.04%	0.005%
63	10.335	2808	2813	2818	rBV	229	266	0.04%	0.005%
64	10.377	2823	2826	2830	rVB2	223	155	0.02%	0.003%
65	10.399	2830	2833	2837	rBV2	152	166	0.03%	0.003%
66	10.425	2838	2841	2846	rVB2	223	177	0.03%	0.003%
67	10.493	2857	2862	2865	rBV2	247	240	0.04%	0.005%
68	10.644	2903	2909	2911	rBV	202	214	0.03%	0.004%
69	10.682	2917	2921	2925	rBV	201	199	0.03%	0.004%
70	10.750	2930	2942	2963	rBV	222455	367599	56.69%	7.125%
71	10.869	2975	2979	2981	rBV3	244	189	0.03%	0.004%
72	10.888	2981	2985	2988	rBV2	275	245	0.04%	0.005%
73	11.110	3050	3054	3059	rVB2	196	169	0.03%	0.003%
74	11.155	3065	3068	3073	rVB	222	196	0.03%	0.004%
75	11.203	3079	3083	3088	rBV	164	198	0.03%	0.004%
76	11.666	3223	3227	3233	rVB	369	388	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
 Data File : VU059523.D
 Acq On : 26 Jun 2024 15:00
 Operator : MD/SY
 Sample : VU0626MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK085

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

77	11.750	3248	3253	3256	rBV2	682	603	0.09%	0.012%
78	11.808	3260	3271	3298	rBV	304262	505111	77.89%	9.791%
79	11.991	3326	3328	3331	rBV2	318	209	0.03%	0.004%
80	12.071	3350	3353	3356	rVV2	252	168	0.03%	0.003%
81	12.091	3356	3359	3367	rVB2	191	163	0.03%	0.003%
82	12.190	3376	3390	3420	rBV	258538	434240	66.96%	8.417%
83	12.354	3438	3441	3448	rBV	161	211	0.03%	0.004%
84	12.386	3448	3451	3453	rBV	275	191	0.03%	0.004%
85	12.759	3564	3567	3572	rBV	235	226	0.03%	0.004%
86	12.808	3579	3582	3585	rBV	236	240	0.04%	0.005%
87	13.274	3720	3727	3729	rBV	267	290	0.04%	0.006%
88	13.473	3784	3789	3790	rBV	362	296	0.05%	0.006%
89	13.499	3794	3797	3799	rBV	208	154	0.02%	0.003%
90	13.666	3846	3849	3851	rBV2	222	167	0.03%	0.003%
91	13.759	3876	3878	3882	rVB	328	208	0.03%	0.004%
92	13.782	3882	3885	3886	rBV	350	181	0.03%	0.004%
93	13.981	3944	3947	3950	rBV	344	281	0.04%	0.005%
94	14.724	4174	4178	4181	rBV3	339	281	0.04%	0.005%
95	14.852	4214	4218	4220	rBV2	400	341	0.05%	0.007%
96	15.068	4282	4285	4287	rBV	363	242	0.04%	0.005%
97	15.344	4366	4371	4374	rBV3	482	545	0.08%	0.011%
98	15.553	4434	4436	4441	rVB3	478	365	0.06%	0.007%
99	15.650	4464	4466	4470	rBV4	358	172	0.03%	0.003%
100	16.274	4658	4660	4663	rVB	709	313	0.05%	0.006%




Sum of corrected areas: 5159158

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
Data File : VU059523.D
Acq On : 26 Jun 2024 15:00
Operator : MD/SY
Sample : VU0626MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK085

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

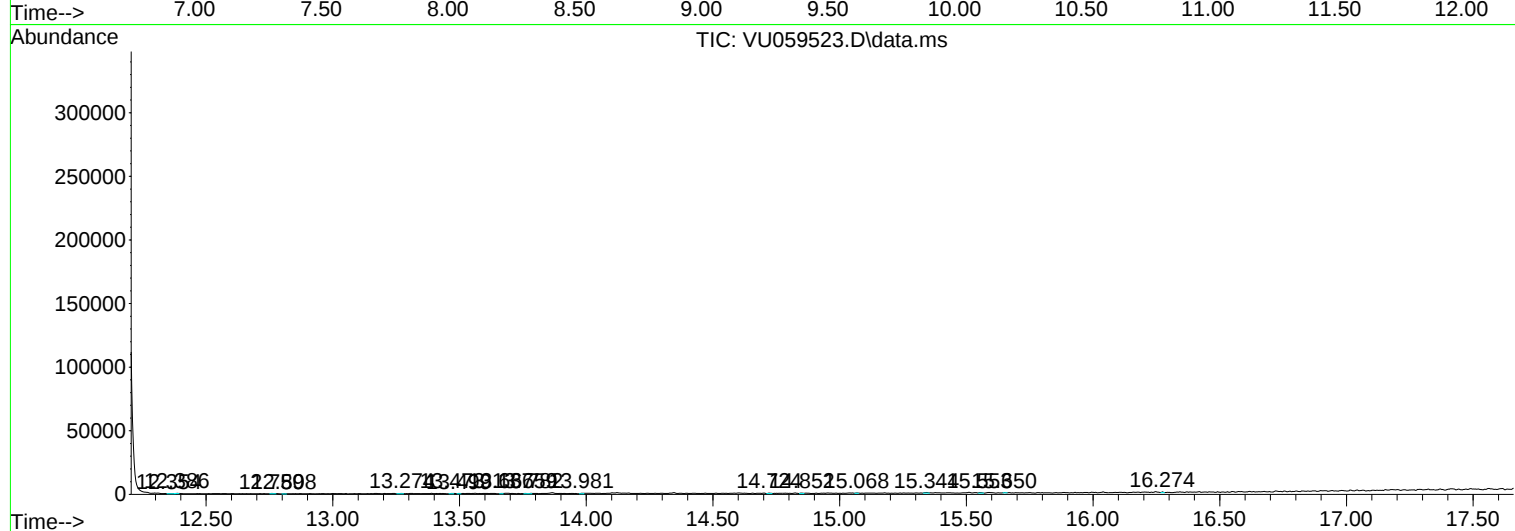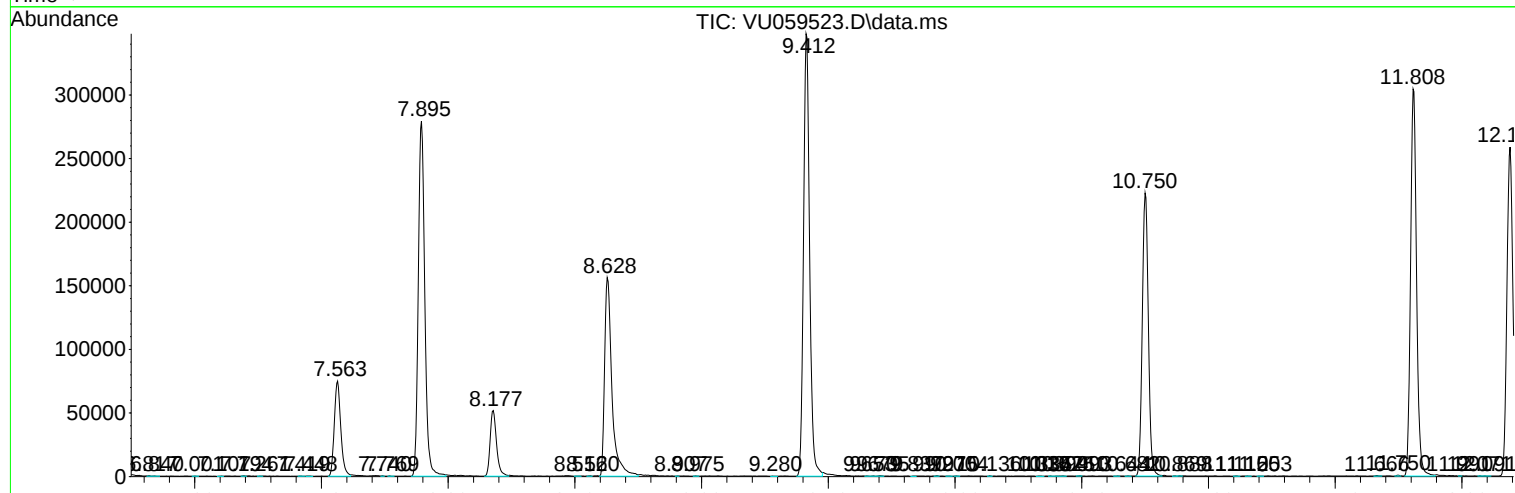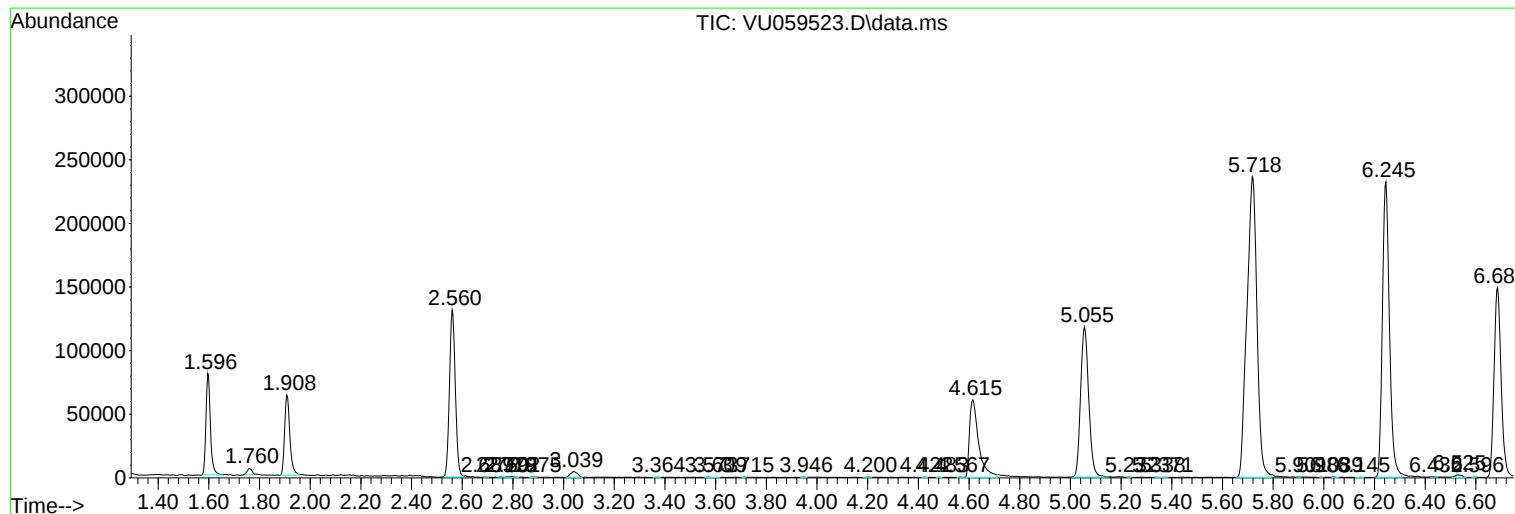

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
Data File : VU059523.D
Acq On : 26 Jun 2024 15:00
Operator : MD/SY
Sample : VU0626MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK085

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
Data File : VU059523.D
Acq On : 26 Jun 2024 15:00
Operator : MD/SY
Sample : VU0626MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK085

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc