

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
 Data File : VU059524.D
 Acq On : 26 Jun 2024 15:21
 Operator : MD/SY
 Sample : VU0626WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK086

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

Signal : TIC: VU059524.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	88	95	114	rVB	74068	90036	14.60%	1.837%
2	1.898	182	189	208	rVB	55570	82377	13.36%	1.681%
3	2.557	383	394	412	rBV	120092	198328	32.16%	4.047%
4	2.695	435	437	441	rBB3	300	181	0.03%	0.004%
5	2.830	477	479	480	rBV	263	96	0.02%	0.002%
6	3.036	534	543	556	rBV4	5596	10767	1.75%	0.220%
7	3.277	615	618	621	rVB2	318	195	0.03%	0.004%
8	3.309	626	628	633	rVB2	233	130	0.02%	0.003%
9	3.341	633	638	641	rBV2	207	202	0.03%	0.004%
10	3.512	688	691	696	rBV2	192	188	0.03%	0.004%
11	4.039	851	855	862	rBV2	212	298	0.05%	0.006%
12	4.091	868	871	877	rVB	290	274	0.04%	0.006%
13	4.119	877	880	882	rBV	160	97	0.02%	0.002%
14	4.136	882	885	886	rBV	91	51	0.01%	0.001%
15	4.216	907	910	912	rBV2	98	72	0.01%	0.001%
16	4.280	927	930	933	rBV	211	138	0.02%	0.003%
17	4.312	937	940	942	rBV	178	121	0.02%	0.002%
18	4.422	972	974	978	rBV2	134	85	0.01%	0.002%
19	4.463	984	987	991	rBV2	127	132	0.02%	0.003%
20	4.550	1012	1014	1017	rVB	160	85	0.01%	0.002%
21	4.611	1023	1033	1063	rBV	61526	155327	25.19%	3.169%
22	4.991	1148	1151	1152	rBV	204	95	0.02%	0.002%
23	5.052	1155	1170	1193	rVV	110668	246654	40.00%	5.033%
24	5.209	1216	1219	1228	rVB3	542	473	0.08%	0.010%
25	5.431	1286	1288	1289	rBV	101	48	0.01%	0.001%
26	5.560	1325	1328	1330	rBV	210	141	0.02%	0.003%
27	5.589	1335	1337	1340	rBV	102	57	0.01%	0.001%
28	5.717	1356	1377	1404	rBV2	223499	616653	100.00%	12.583%
29	5.926	1437	1442	1446	rBV3	312	368	0.06%	0.008%
30	5.991	1454	1462	1464	rBV	367	399	0.06%	0.008%
31	6.010	1464	1468	1471	rBV2	356	280	0.05%	0.006%
32	6.177	1515	1520	1522	rBV2	141	139	0.02%	0.003%
33	6.197	1523	1526	1527	rBV2	232	134	0.02%	0.003%
34	6.242	1528	1540	1565	rBV	221159	426458	69.16%	8.702%
35	6.528	1622	1629	1637	rVB7	2067	3876	0.63%	0.079%
36	6.560	1637	1639	1641	rBV2	227	138	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
 Data File : VU059524.D
 Acq On : 26 Jun 2024 15:21
 Operator : MD/SY
 Sample : VU0626WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK086

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

37	6.682	1664	1677	1707	rVB	142292	278606	45.18%	5.685%
38	6.878	1736	1738	1744	rVB2	220	167	0.03%	0.003%
39	6.975	1766	1768	1770	rBV	124	80	0.01%	0.002%
40	7.431	1908	1910	1911	rBV2	64	34	0.01%	0.001%
41	7.560	1939	1950	1976	rBV	71949	128295	20.81%	2.618%
42	7.804	2020	2026	2029	rBV3	382	466	0.08%	0.010%
43	7.891	2041	2053	2074	rBV	260503	457540	74.20%	9.336%
44	8.174	2131	2141	2159	rBV2	50400	85137	13.81%	1.737%
45	8.293	2177	2178	2179	rBV2	147	47	0.01%	0.001%
46	8.328	2185	2189	2192	rBV2	312	220	0.04%	0.004%
47	8.463	2227	2231	2237	rBV3	335	387	0.06%	0.008%
48	8.627	2270	2282	2313	rBV	165254	319911	51.88%	6.528%
49	8.827	2341	2344	2345	rBV	385	215	0.03%	0.004%
50	8.936	2376	2378	2379	rBV	169	62	0.01%	0.001%
51	9.299	2488	2491	2493	rBV	119	68	0.01%	0.001%
52	9.412	2514	2526	2547	rBV	330611	545796	88.51%	11.137%
53	9.569	2573	2575	2579	rBV	329	267	0.04%	0.005%
54	9.721	2620	2622	2625	rVB	267	135	0.02%	0.003%
55	9.746	2627	2630	2634	rBV2	301	260	0.04%	0.005%
56	10.267	2789	2792	2793	rBV2	202	119	0.02%	0.002%
57	10.749	2930	2942	2970	rVB	218551	358354	58.11%	7.312%
58	11.402	3142	3145	3147	rBV	205	139	0.02%	0.003%
59	11.601	3204	3207	3210	rBV	257	160	0.03%	0.003%
60	11.682	3230	3232	3234	rBV	141	85	0.01%	0.002%
61	11.749	3249	3253	3258	rBV2	531	561	0.09%	0.011%
62	11.807	3259	3271	3290	rBV	285419	475044	77.04%	9.693%
63	12.187	3377	3389	3408	rBV	242977	412322	66.86%	8.414%
64	12.354	3438	3441	3444	rBV2	351	240	0.04%	0.005%
65	12.669	3536	3539	3542	rBV	446	296	0.05%	0.006%
66	13.855	3905	3908	3909	rBV	595	369	0.06%	0.008%
67	13.929	3928	3931	3933	rBV	316	242	0.04%	0.005%




Sum of corrected areas: 4900717

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
Data File : VU059524.D
Acq On : 26 Jun 2024 15:21
Operator : MD/SY
Sample : VU0626WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK086

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

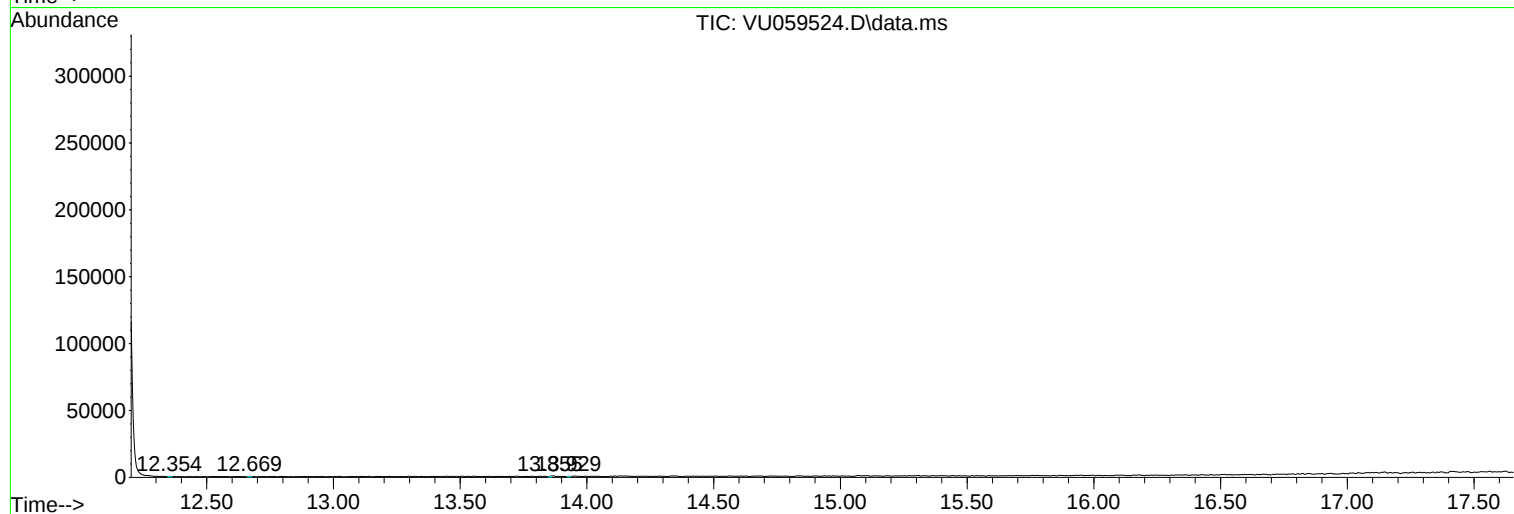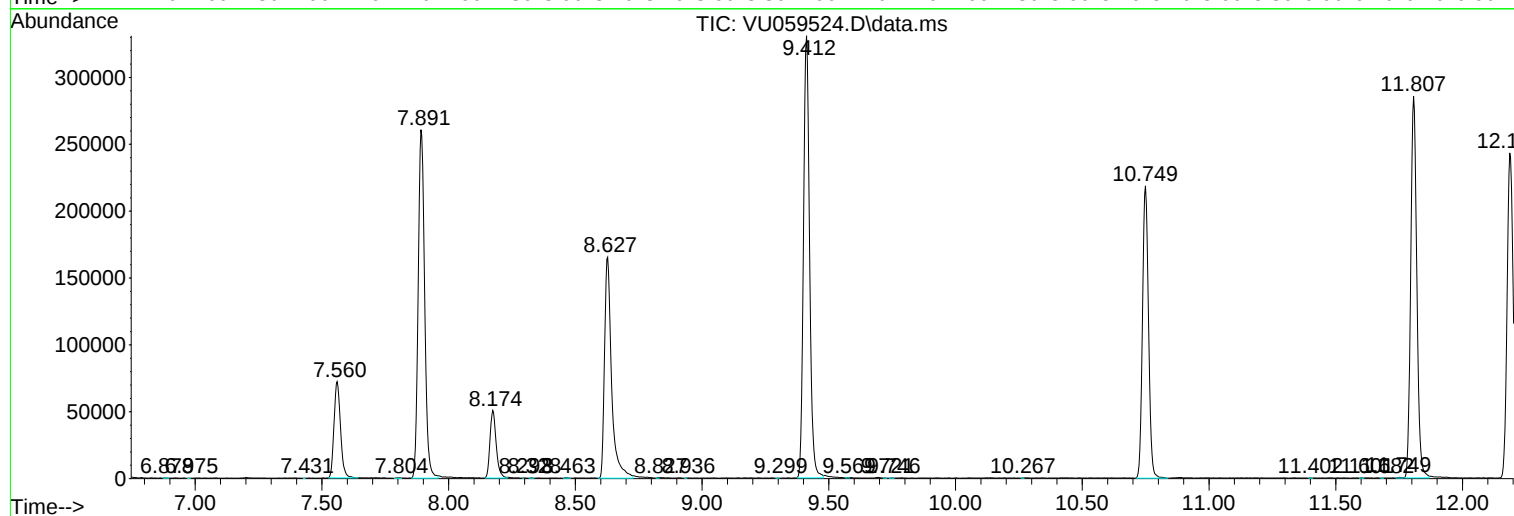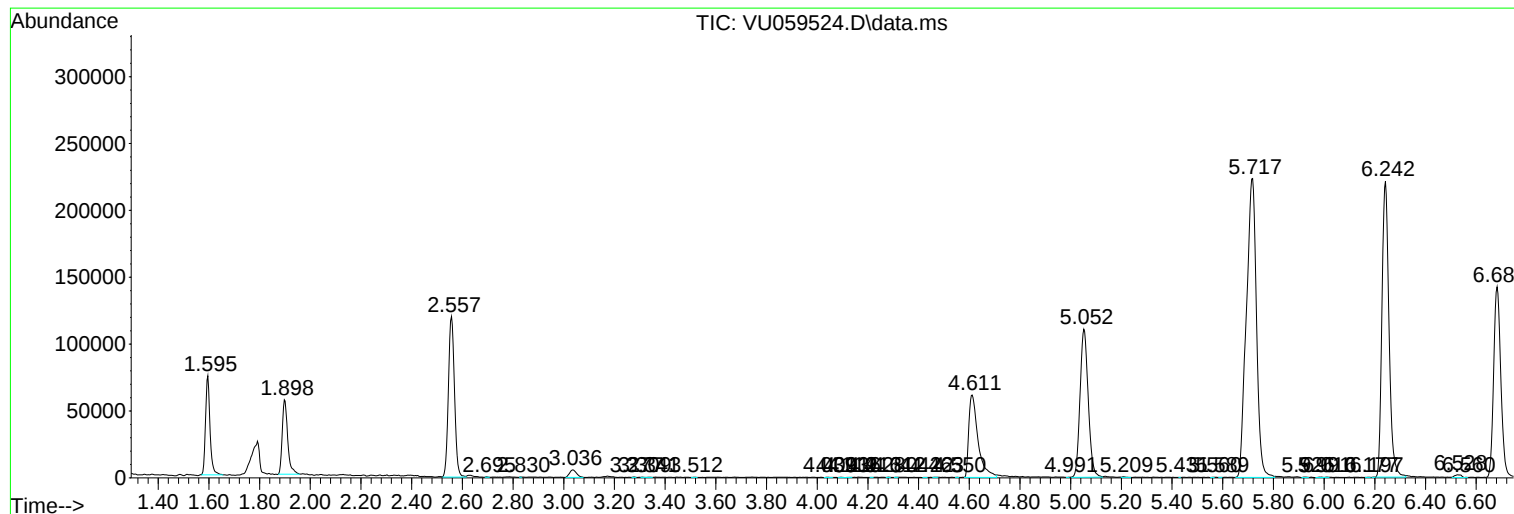

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
Data File : VU059524.D
Acq On : 26 Jun 2024 15:21
Operator : MD/SY
Sample : VU0626WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK086

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
Data File : VU059524.D
Acq On : 26 Jun 2024 15:21
Operator : MD/SY
Sample : VU0626WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK086

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc