

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
 Data File : VU059525.D
 Acq On : 26 Jun 2024 15:43
 Operator : MD/SY
 Sample : P3017-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

Signal : TIC: VU059525.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	114	rVB	68743	86405	14.16%	1.784%
2	1.898	182	189	211	rVB	55491	82085	13.45%	1.694%
3	2.557	382	394	410	rBV	118374	192484	31.55%	3.973%
4	2.788	459	466	471	rBV2	430	693	0.11%	0.014%
5	3.036	534	543	559	rBV2	6222	11520	1.89%	0.238%
6	3.158	577	581	582	rBV2	440	312	0.05%	0.006%
7	3.274	614	617	624	rVB	178	200	0.03%	0.004%
8	3.313	626	629	631	rBV	112	75	0.01%	0.002%
9	3.390	650	653	658	rVB	209	168	0.03%	0.003%
10	3.415	658	661	666	rVB2	178	128	0.02%	0.003%
11	3.454	670	673	675	rBV	192	118	0.02%	0.002%
12	3.550	699	703	708	rBV2	188	223	0.04%	0.005%
13	4.219	909	911	915	rBV2	158	131	0.02%	0.003%
14	4.306	934	938	940	rBV2	168	105	0.02%	0.002%
15	4.322	940	943	946	rVB	167	83	0.01%	0.002%
16	4.554	1008	1015	1019	rVB2	182	240	0.04%	0.005%
17	4.573	1019	1021	1023	rBV2	105	66	0.01%	0.001%
18	4.608	1023	1032	1064	rBV	62077	153734	25.20%	3.173%
19	5.052	1155	1170	1192	rBV	109642	243264	39.87%	5.022%
20	5.210	1218	1219	1220	rBV	130	41	0.01%	0.001%
21	5.232	1224	1226	1230	rVB2	223	147	0.02%	0.003%
22	5.390	1272	1275	1281	rVB2	345	251	0.04%	0.005%
23	5.435	1286	1289	1291	rBV	96	47	0.01%	0.001%
24	5.457	1292	1296	1300	rBV2	178	159	0.03%	0.003%
25	5.476	1300	1302	1305	rBV2	80	40	0.01%	0.001%
26	5.496	1305	1308	1311	rBV	139	95	0.02%	0.002%
27	5.560	1327	1328	1332	rBV2	145	63	0.01%	0.001%
28	5.583	1332	1335	1337	rBV2	114	73	0.01%	0.002%
29	5.618	1343	1346	1348	rBV2	114	67	0.01%	0.001%
30	5.714	1354	1376	1402	rBV2	224463	610146	100.00%	12.595%
31	6.103	1493	1497	1500	rBV2	176	160	0.03%	0.003%
32	6.242	1526	1540	1559	rBV	221647	421505	69.08%	8.701%
33	6.470	1608	1611	1613	rBV2	306	170	0.03%	0.004%
34	6.528	1620	1629	1631	rBV3	1610	2070	0.34%	0.043%
35	6.557	1636	1638	1642	rVB2	315	163	0.03%	0.003%
36	6.589	1646	1648	1651	rBV	109	67	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
 Data File : VU059525.D
 Acq On : 26 Jun 2024 15:43
 Operator : MD/SY
 Sample : P3017-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

37	6.605	1651	1653	1656	rVB2	171	90	0.01%	0.002%
38	6.624	1656	1659	1661	rBV2	129	80	0.01%	0.002%
39	6.682	1661	1677	1697	rBV	138895	273901	44.89%	5.654%
40	6.795	1709	1712	1714	rVB2	665	350	0.06%	0.007%
41	6.878	1734	1738	1739	rBV	125	75	0.01%	0.002%
42	6.939	1752	1757	1760	rBV2	133	129	0.02%	0.003%
43	6.988	1769	1772	1774	rVB	122	51	0.01%	0.001%
44	7.007	1775	1778	1780	rVB2	145	82	0.01%	0.002%
45	7.023	1780	1783	1785	rBV2	137	85	0.01%	0.002%
46	7.042	1787	1789	1792	rVB2	183	75	0.01%	0.002%
47	7.058	1792	1794	1796	rBV	109	64	0.01%	0.001%
48	7.126	1812	1815	1817	rBV	187	146	0.02%	0.003%
49	7.190	1832	1835	1837	rBV	222	158	0.03%	0.003%
50	7.206	1837	1840	1843	rVB3	401	266	0.04%	0.005%
51	7.319	1872	1875	1878	rBV	201	142	0.02%	0.003%
52	7.393	1895	1898	1900	rVB	186	101	0.02%	0.002%
53	7.406	1900	1902	1905	rBV2	77	43	0.01%	0.001%
54	7.425	1905	1908	1911	rBV	122	71	0.01%	0.001%
55	7.444	1911	1914	1915	rBV	91	50	0.01%	0.001%
56	7.512	1932	1935	1939	rVB2	118	92	0.02%	0.002%
57	7.560	1939	1950	1968	rBV	71623	126319	20.70%	2.608%
58	7.660	1978	1981	1983	rBV	217	129	0.02%	0.003%
59	7.695	1987	1992	1996	rBV4	366	368	0.06%	0.008%
60	7.775	2012	2017	2021	rVB2	238	210	0.03%	0.004%
61	7.891	2041	2053	2075	rBV	255302	451276	73.96%	9.316%
62	8.110	2119	2121	2125	rBV2	267	174	0.03%	0.004%
63	8.174	2131	2141	2154	rBV	49844	83221	13.64%	1.718%
64	8.290	2175	2177	2179	rBV	124	68	0.01%	0.001%
65	8.332	2187	2190	2192	rBV	155	99	0.02%	0.002%
66	8.525	2247	2250	2254	rBV2	238	214	0.04%	0.004%
67	8.586	2266	2269	2271	rBV	153	109	0.02%	0.002%
68	8.624	2271	2281	2312	rBV	168808	315180	51.66%	6.506%
69	8.875	2355	2359	2360	rBV	225	160	0.03%	0.003%
70	8.981	2389	2392	2395	rBV2	166	104	0.02%	0.002%
71	9.187	2451	2456	2461	rBV	162	186	0.03%	0.004%
72	9.274	2480	2483	2485	rBV	80	56	0.01%	0.001%
73	9.322	2495	2498	2501	rBV2	288	225	0.04%	0.005%
74	9.367	2509	2512	2513	rBV	97	53	0.01%	0.001%
75	9.412	2513	2526	2562	rVV	322262	544801	89.29%	11.246%
76	9.563	2569	2573	2576	rBV2	455	440	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
 Data File : VU059525.D
 Acq On : 26 Jun 2024 15:43
 Operator : MD/SY
 Sample : P3017-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

77	9.695	2611	2614	2616	rBV2	312	184	0.03%	0.004%
78	9.782	2638	2641	2643	rBV	181	117	0.02%	0.002%
79	9.891	2672	2675	2677	rBV2	253	177	0.03%	0.004%
80	10.016	2711	2714	2721	rBV2	222	246	0.04%	0.005%
81	10.344	2814	2816	2818	rBV2	167	94	0.02%	0.002%
82	10.460	2849	2852	2855	rBV2	308	232	0.04%	0.005%
83	10.570	2882	2886	2889	rBV2	204	194	0.03%	0.004%
84	10.682	2918	2921	2924	rBV	216	147	0.02%	0.003%
85	10.750	2930	2942	2965	rBV	222002	358683	58.79%	7.404%
86	11.312	3114	3117	3119	rBV	163	113	0.02%	0.002%
87	11.412	3145	3148	3151	rBV2	173	137	0.02%	0.003%
88	11.460	3159	3163	3164	rBV	281	180	0.03%	0.004%
89	11.685	3230	3233	3234	rBV	223	124	0.02%	0.003%
90	11.807	3259	3271	3292	rBV	287758	467480	76.62%	9.650%
91	11.978	3319	3324	3328	rBV2	240	209	0.03%	0.004%
92	12.023	3335	3338	3339	rBV	172	84	0.01%	0.002%
93	12.187	3377	3389	3418	rBV	241669	407739	66.83%	8.417%
94	12.595	3513	3516	3519	rBV2	263	206	0.03%	0.004%
95	12.692	3543	3546	3553	rBV	276	276	0.05%	0.006%
96	13.200	3701	3704	3706	rBV	186	137	0.02%	0.003%
97	13.573	3816	3820	3822	rBV	353	243	0.04%	0.005%
98	13.605	3827	3830	3833	rVB3	302	211	0.03%	0.004%
99	13.968	3940	3943	3947	rBV2	289	210	0.03%	0.004%
100	14.065	3971	3973	3977	rBV	237	177	0.03%	0.004%




Sum of corrected areas: 4844341

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
Data File : VU059525.D
Acq On : 26 Jun 2024 15:43
Operator : MD/SY
Sample : P3017-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

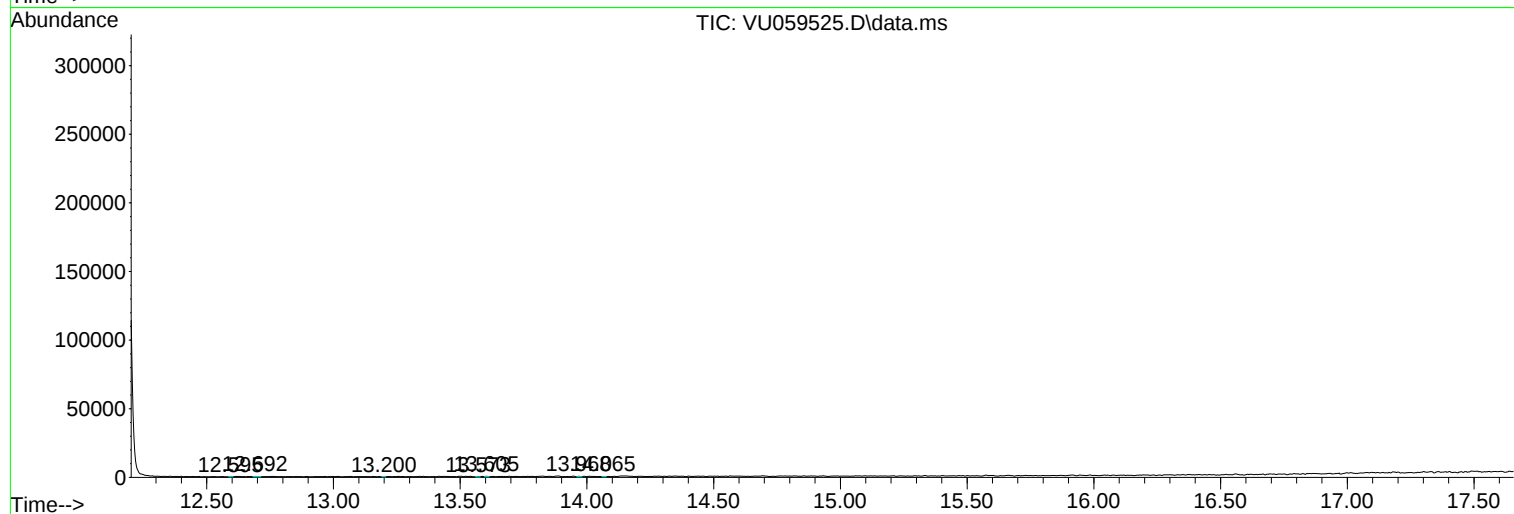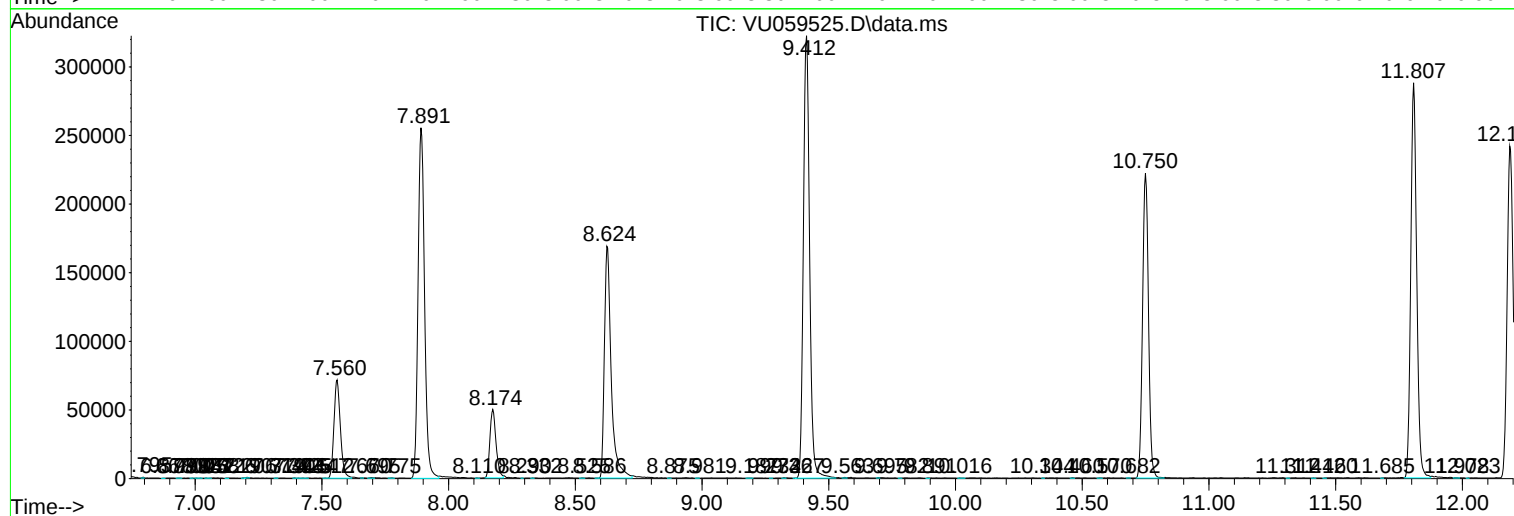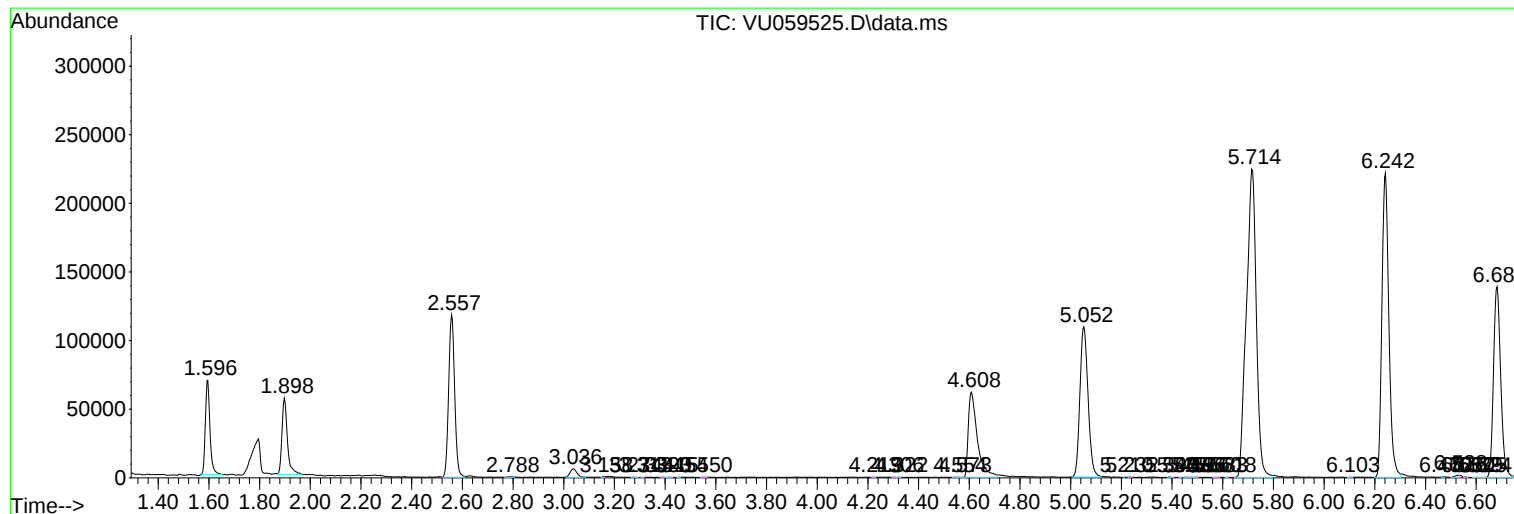

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
Data File : VU059525.D
Acq On : 26 Jun 2024 15:43
Operator : MD/SY
Sample : P3017-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
Data File : VU059525.D
Acq On : 26 Jun 2024 15:43
Operator : MD/SY
Sample : P3017-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc