

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
 Data File : VU059527.D
 Acq On : 26 Jun 2024 16:27
 Operator : MD/SY
 Sample : P3081-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08E2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

Signal : TIC: VU059527.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.592	88	94	114	rVB	76962	98173	15.20%	1.873%
2	1.898	181	189	206	rBV	58948	84452	13.08%	1.611%
3	2.557	382	394	406	rBV	126995	206911	32.04%	3.948%
4	2.679	429	432	434	rBV	283	153	0.02%	0.003%
5	2.695	434	437	439	rBV	124	74	0.01%	0.001%
6	2.721	443	445	449	rBV2	185	128	0.02%	0.002%
7	2.846	481	484	489	rVB	349	209	0.03%	0.004%
8	2.891	495	498	499	rBV	240	144	0.02%	0.003%
9	2.959	515	519	522	rBV2	275	231	0.04%	0.004%
10	3.039	534	544	552	rVB6	1888	3402	0.53%	0.065%
11	3.242	603	607	614	rBV2	186	270	0.04%	0.005%
12	3.342	633	638	641	rBV2	221	220	0.03%	0.004%
13	3.383	648	651	652	rBV2	63	33	0.01%	0.001%
14	3.396	652	655	657	rBV	140	89	0.01%	0.002%
15	3.531	696	697	698	rBV	137	29	0.00%	0.001%
16	3.580	705	712	718	rBV2	303	414	0.06%	0.008%
17	3.641	728	731	733	rBV	115	83	0.01%	0.002%
18	3.679	741	743	748	rVB3	244	161	0.02%	0.003%
19	3.724	755	757	764	rBV2	141	158	0.02%	0.003%
20	3.965	829	832	834	rBV	135	93	0.01%	0.002%
21	3.994	838	841	844	rVB2	179	103	0.02%	0.002%
22	4.017	844	848	851	rBV2	163	152	0.02%	0.003%
23	4.084	866	869	871	rBV2	116	70	0.01%	0.001%
24	4.274	925	928	930	rBV	122	74	0.01%	0.001%
25	4.361	952	955	962	rBV2	207	194	0.03%	0.004%
26	4.547	1009	1013	1017	rBV	182	197	0.03%	0.004%
27	4.612	1023	1033	1069	rBV	65255	165035	25.56%	3.149%
28	5.001	1151	1154	1155	rBV	170	109	0.02%	0.002%
29	5.055	1155	1171	1205	rVV3	124985	335209	51.91%	6.396%
30	5.171	1205	1207	1210	rVB	294	136	0.02%	0.003%
31	5.213	1217	1220	1223	rBV	196	113	0.02%	0.002%
32	5.325	1252	1255	1257	rBV2	94	61	0.01%	0.001%
33	5.377	1265	1271	1280	rVB2	176	298	0.05%	0.006%
34	5.415	1280	1283	1284	rBV	73	36	0.01%	0.001%
35	5.432	1284	1288	1291	rBV	187	158	0.02%	0.003%
36	5.541	1320	1322	1325	rBV2	78	51	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
 Data File : VU059527.D
 Acq On : 26 Jun 2024 16:27
 Operator : MD/SY
 Sample : P3081-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08E2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

37	5.624	1345	1348	1351	rBV2	100	68	0.01%	0.001%
38	5.641	1351	1353	1356	rBV2	147	81	0.01%	0.002%
39	5.715	1357	1376	1409	rVV2	234851	645705	100.00%	12.321%
40	5.930	1440	1443	1446	rVV2	254	168	0.03%	0.003%
41	5.949	1446	1449	1452	rVB	292	177	0.03%	0.003%
42	6.026	1468	1473	1477	rBV2	334	301	0.05%	0.006%
43	6.242	1527	1540	1564	rBV	239561	463876	71.84%	8.851%
44	6.496	1616	1619	1621	rBV2	187	131	0.02%	0.002%
45	6.525	1621	1628	1638	rVB6	1326	2405	0.37%	0.046%
46	6.628	1657	1660	1662	rVB	188	100	0.02%	0.002%
47	6.682	1663	1677	1696	rBV	147120	288549	44.69%	5.506%
48	6.776	1702	1706	1710	rVB3	517	398	0.06%	0.008%
49	6.891	1737	1742	1745	rBV2	121	115	0.02%	0.002%
50	6.975	1764	1768	1769	rBV	152	98	0.02%	0.002%
51	7.026	1779	1784	1786	rBV	139	134	0.02%	0.003%
52	7.100	1799	1807	1819	rVB2	7083	12969	2.01%	0.247%
53	7.194	1832	1836	1837	rBV	453	340	0.05%	0.006%
54	7.358	1882	1887	1890	rBV2	100	102	0.02%	0.002%
55	7.425	1905	1908	1910	rBV2	98	67	0.01%	0.001%
56	7.560	1938	1950	1968	rBV	74697	133692	20.70%	2.551%
57	7.650	1977	1978	1981	rVB	290	78	0.01%	0.001%
58	7.666	1981	1983	1985	rBV2	276	158	0.02%	0.003%
59	7.679	1985	1987	1990	rVB3	234	151	0.02%	0.003%
60	7.891	2041	2053	2069	rBV	276558	480952	74.48%	9.177%
61	8.129	2125	2127	2128	rBV	195	81	0.01%	0.002%
62	8.174	2130	2141	2161	rVV	52445	91215	14.13%	1.740%
63	8.335	2188	2191	2194	rBV2	164	68	0.01%	0.001%
64	8.467	2224	2232	2241	rVB2	3230	5415	0.84%	0.103%
65	8.554	2256	2259	2267	rVB2	339	368	0.06%	0.007%
66	8.628	2272	2282	2317	rBV	173403	328064	50.81%	6.260%
67	9.017	2400	2403	2406	rBV	195	148	0.02%	0.003%
68	9.136	2437	2440	2441	rBV	111	62	0.01%	0.001%
69	9.152	2442	2445	2447	rVB2	265	163	0.03%	0.003%
70	9.412	2514	2526	2543	rBV	349888	586951	90.90%	11.200%
71	9.692	2609	2613	2619	rBV3	728	886	0.14%	0.017%
72	10.049	2721	2724	2728	rBV2	158	155	0.02%	0.003%
73	10.107	2736	2742	2744	rBV2	617	660	0.10%	0.013%
74	10.348	2809	2817	2818	rBV	192	227	0.04%	0.004%
75	10.418	2835	2839	2843	rBV	210	216	0.03%	0.004%
76	10.750	2930	2942	2958	rBV	223770	364407	56.44%	6.953%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
 Data File : VU059527.D
 Acq On : 26 Jun 2024 16:27
 Operator : MD/SY
 Sample : P3081-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08E2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

77	10.888	2975	2985	2999	rBV4	4579	7359	1.14%	0.140%
78	11.100	3048	3051	3052	rBV	175	80	0.01%	0.002%
79	11.370	3131	3135	3140	rVB2	374	385	0.06%	0.007%
80	11.396	3140	3143	3145	rBV	295	245	0.04%	0.005%
81	11.480	3168	3169	3170	rBV	207	63	0.01%	0.001%
82	11.499	3173	3175	3177	rVV2	424	203	0.03%	0.004%
83	11.576	3196	3199	3204	rBV	175	140	0.02%	0.003%
84	11.808	3259	3271	3289	rBV	305858	500773	77.55%	9.555%
85	12.049	3344	3346	3347	rBV	184	65	0.01%	0.001%
86	12.187	3377	3389	3417	rBV	251219	423462	65.58%	8.080%
87	12.981	3634	3636	3641	rBV2	270	158	0.02%	0.003%
88	13.042	3650	3655	3659	rBV2	391	417	0.06%	0.008%
89	13.463	3783	3786	3787	rBV	236	126	0.02%	0.002%




Sum of corrected areas: 5240800

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
Data File : VU059527.D
Acq On : 26 Jun 2024 16:27
Operator : MD/SY
Sample : P3081-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08E2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

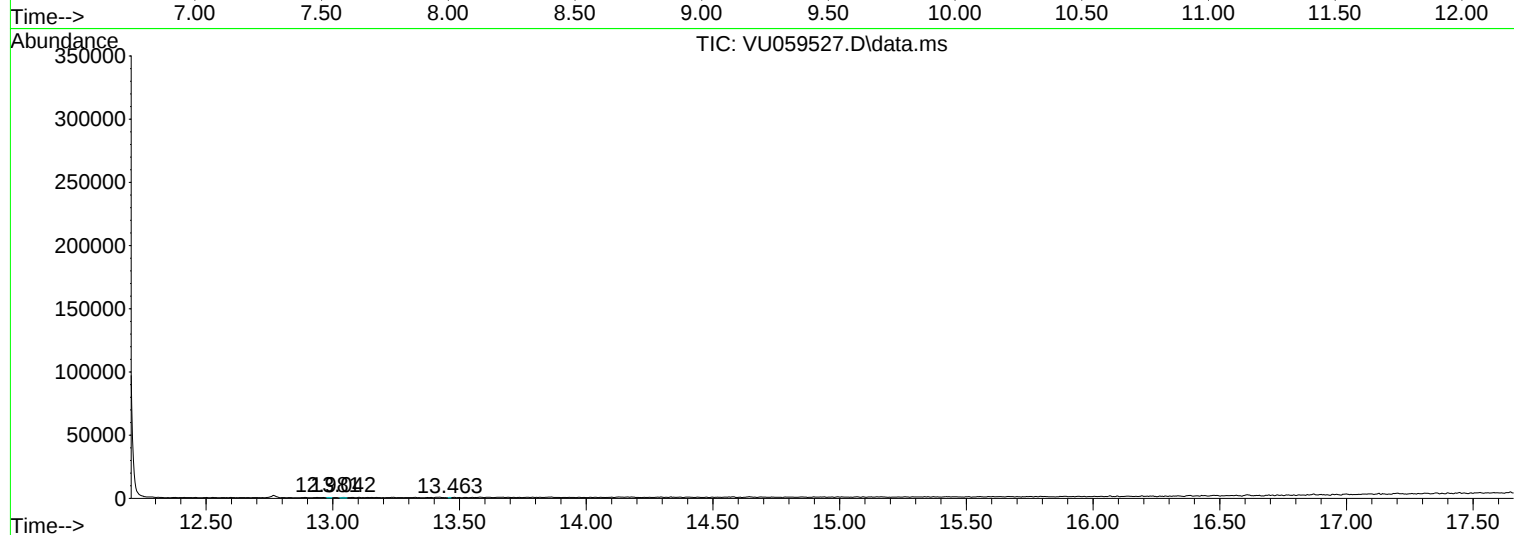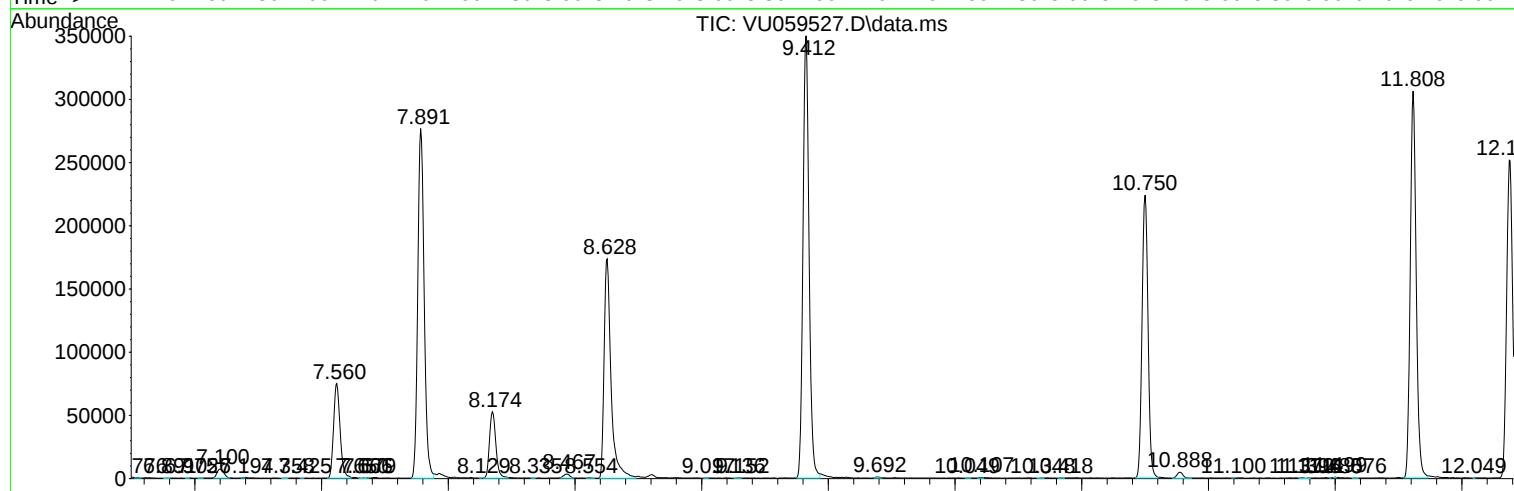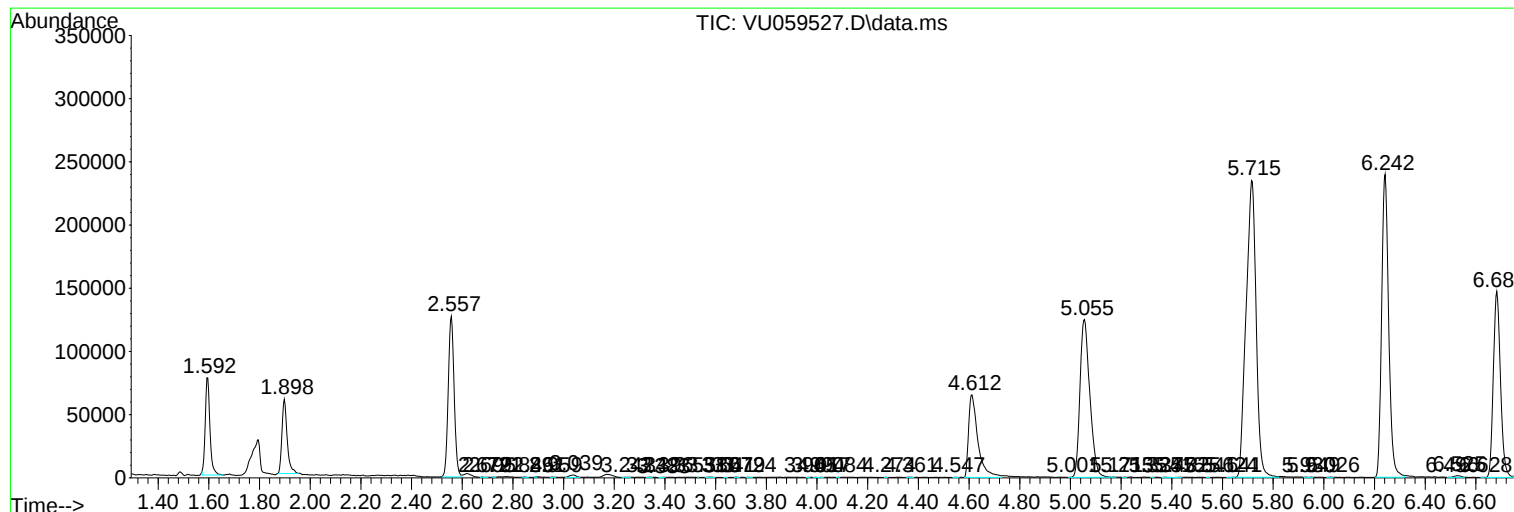

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
Data File : VU059527.D
Acq On : 26 Jun 2024 16:27
Operator : MD/SY
Sample : P3081-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08E2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
Data File : VU059527.D
Acq On : 26 Jun 2024 16:27
Operator : MD/SY
Sample : P3081-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08E2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------