

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
 Data File : VU059536.D
 Acq On : 26 Jun 2024 20:57
 Operator : MD/SY
 Sample : P3055-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08D1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M

Title : VOC Analysis

Signal : TIC: VU059538.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.480	56	59	65	rVB3	3112	2948	0.19%	0.022%
2	1.592	85	94	132	rBV	76298	213501	13.63%	1.611%
3	1.827	138	167	171	rBV4	39832	165774	10.59%	1.251%
4	1.866	175	179	196	rVB	74143	114980	7.34%	0.868%
5	2.364	328	334	342	rVB8	2568	3744	0.24%	0.028%
6	2.531	373	386	405	rBV	304403	495435	31.63%	3.738%
7	2.634	409	418	432	rVV	6768	12465	0.80%	0.094%
8	2.801	464	470	472	rBV3	451	577	0.04%	0.004%
9	2.882	493	495	498	rBV2	310	216	0.01%	0.002%
10	2.933	509	511	518	rBV2	402	345	0.02%	0.003%
11	3.026	527	540	553	rBV3	5816	12157	0.78%	0.092%
12	3.091	558	560	564	rVB2	349	223	0.01%	0.002%
13	3.171	571	585	596	rBV2	6397	15117	0.97%	0.114%
14	3.657	733	736	738	rBV2	757	579	0.04%	0.004%
15	3.721	750	756	758	rBV	257	213	0.01%	0.002%
16	3.763	766	769	775	rVV2	181	176	0.01%	0.001%
17	3.917	812	817	822	rVB2	247	290	0.02%	0.002%
18	4.004	838	844	850	rBV2	224	314	0.02%	0.002%
19	4.206	903	907	910	rVV2	296	209	0.01%	0.002%
20	4.412	968	971	973	rBV2	345	281	0.02%	0.002%
21	4.621	1025	1036	1082	rBV	122824	345595	22.07%	2.608%
22	5.049	1149	1169	1205	rBV	286546	662401	42.30%	4.998%
23	5.203	1214	1217	1220	rVB3	798	529	0.03%	0.004%
24	5.274	1235	1239	1240	rBV	369	218	0.01%	0.002%
25	5.296	1243	1246	1252	rVV2	510	412	0.03%	0.003%
26	5.341	1256	1260	1263	rVB3	238	173	0.01%	0.001%
27	5.711	1351	1375	1409	rBV2	592167	1566116	100.00%	11.816%
28	5.901	1432	1434	1440	rVB3	357	315	0.02%	0.002%
29	5.972	1450	1456	1458	rBV5	1409	1416	0.09%	0.011%
30	6.123	1496	1503	1507	rVB3	417	485	0.03%	0.004%
31	6.239	1524	1539	1575	rBV	567557	1090060	69.60%	8.224%
32	6.521	1619	1627	1641	rVB8	6671	12487	0.80%	0.094%
33	6.599	1641	1651	1658	rBV6	1827	3226	0.21%	0.024%
34	6.682	1663	1677	1699	rVV	366401	715194	45.67%	5.396%
35	6.759	1699	1701	1705	rVB3	1030	625	0.04%	0.005%
36	6.795	1709	1712	1717	rBV5	652	540	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
 Data File : VU059536.D
 Acq On : 26 Jun 2024 20:57
 Operator : MD/SY
 Sample : P3055-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08D1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

37	6.962	1756	1764	1767	rBV2	258	318	0.02%	0.002%
38	7.103	1794	1808	1817	rBV4	2693	5911	0.38%	0.045%
39	7.197	1829	1837	1843	rBV5	1882	3181	0.20%	0.024%
40	7.329	1875	1878	1883	rVB	205	185	0.01%	0.001%
41	7.560	1938	1950	1976	rBV	177732	320835	20.49%	2.421%
42	7.701	1987	1994	2000	rBV2	1227	1676	0.11%	0.013%
43	7.756	2007	2011	2014	rVB2	233	179	0.01%	0.001%
44	7.891	2040	2053	2073	rBV	703331	1213147	77.46%	9.153%
45	8.174	2129	2141	2161	rBV2	122273	213590	13.64%	1.612%
46	8.341	2190	2193	2194	rBV	364	180	0.01%	0.001%
47	8.431	2214	2221	2222	rBV	179	195	0.01%	0.001%
48	8.467	2222	2232	2245	rVB3	5581	9241	0.59%	0.070%
49	8.554	2253	2259	2266	rVB5	770	962	0.06%	0.007%
50	8.637	2272	2285	2315	rBV	419646	877828	56.05%	6.623%
51	9.036	2406	2409	2413	rBV	349	179	0.01%	0.001%
52	9.412	2513	2526	2549	rBV	855104	1416930	90.47%	10.691%
53	9.573	2571	2576	2582	rVB2	1141	1129	0.07%	0.009%
54	9.695	2602	2614	2624	rBV2	5059	8001	0.51%	0.060%
55	9.766	2631	2636	2640	rBV2	206	232	0.01%	0.002%
56	9.836	2653	2658	2662	rBV2	217	212	0.01%	0.002%
57	10.103	2734	2741	2742	rBV	1579	1465	0.09%	0.011%
58	10.271	2788	2793	2797	rVB2	216	292	0.02%	0.002%
59	10.306	2797	2804	2809	rBV2	298	396	0.03%	0.003%
60	10.364	2819	2822	2824	rVV	426	198	0.01%	0.001%
61	10.402	2828	2834	2839	rBV	264	256	0.02%	0.002%
62	10.586	2886	2891	2894	rBV2	405	368	0.02%	0.003%
63	10.631	2900	2905	2910	rBV2	214	222	0.01%	0.002%
64	10.753	2930	2943	2968	rBV	580895	945222	60.35%	7.132%
65	10.891	2975	2986	2996	rBV3	7541	12909	0.82%	0.097%
66	11.049	3030	3035	3038	rVB	199	191	0.01%	0.001%
67	11.097	3046	3050	3053	rBV	235	206	0.01%	0.002%
68	11.116	3053	3056	3060	rBV2	475	398	0.03%	0.003%
69	11.328	3113	3122	3129	rVB4	2129	2936	0.19%	0.022%
70	11.373	3132	3136	3141	rBV	655	574	0.04%	0.004%
71	11.486	3156	3171	3186	rBV4	5525	13723	0.88%	0.104%
72	11.753	3246	3254	3259	rBV3	675	872	0.06%	0.007%
73	11.811	3259	3272	3295	rBV	920634	1473630	94.09%	11.119%
74	11.978	3320	3324	3327	rBV2	336	273	0.02%	0.002%
75	11.997	3327	3330	3335	rVB3	405	348	0.02%	0.003%
76	12.020	3335	3337	3342	rVB2	412	233	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
Data File : VU059536.D
Acq On : 26 Jun 2024 20:57
Operator : MD/SY
Sample : P3055-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08D1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Title : VOC Analysis

77	12.190	3377	3390	3413	rVV	795468	1275273	81.43%	9.622%
78	12.441	3463	3468	3472	rBV2	363	383	0.02%	0.003%
79	12.598	3514	3517	3520	rBV2	352	171	0.01%	0.001%
80	12.682	3540	3543	3549	rVB	352	263	0.02%	0.002%
81	12.711	3549	3552	3554	rBV	361	224	0.01%	0.002%
82	12.766	3560	3569	3582	rBV2	2518	3793	0.24%	0.029%
83	13.068	3660	3663	3668	rBV2	200	174	0.01%	0.001%
84	13.807	3890	3893	3896	rBV	463	324	0.02%	0.002%
85	14.042	3962	3966	3968	rBV2	398	315	0.02%	0.002%
86	14.084	3976	3979	3980	rBV	296	180	0.01%	0.001%
87	14.193	4009	4013	4017	rBV3	322	305	0.02%	0.002%
88	14.338	4056	4058	4064	rVB3	374	274	0.02%	0.002%
89	14.566	4124	4129	4130	rBV2	623	550	0.04%	0.004%
90	14.820	4205	4208	4210	rBV2	438	269	0.02%	0.002%
91	14.862	4219	4221	4226	rBV3	428	426	0.03%	0.003%
92	14.917	4235	4238	4240	rBV2	326	252	0.02%	0.002%
93	15.016	4266	4269	4271	rBV2	320	207	0.01%	0.002%
94	15.032	4271	4274	4277	rVV3	446	291	0.02%	0.002%
95	15.187	4320	4322	4325	rBV	320	230	0.01%	0.002%
96	15.283	4350	4352	4355	rBV2	340	216	0.01%	0.002%
97	15.367	4376	4378	4385	rBV4	377	331	0.02%	0.002%
98	15.946	4556	4558	4561	rVB3	618	264	0.02%	0.002%
99	16.383	4691	4694	4696	rBV2	794	616	0.04%	0.005%
100	16.441	4710	4712	4714	rBV3	656	355	0.02%	0.003%




Sum of corrected areas: 13253845

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
Data File : VU059536.D
Acq On : 26 Jun 2024 20:57
Operator : MD/SY
Sample : P3055-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08D1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

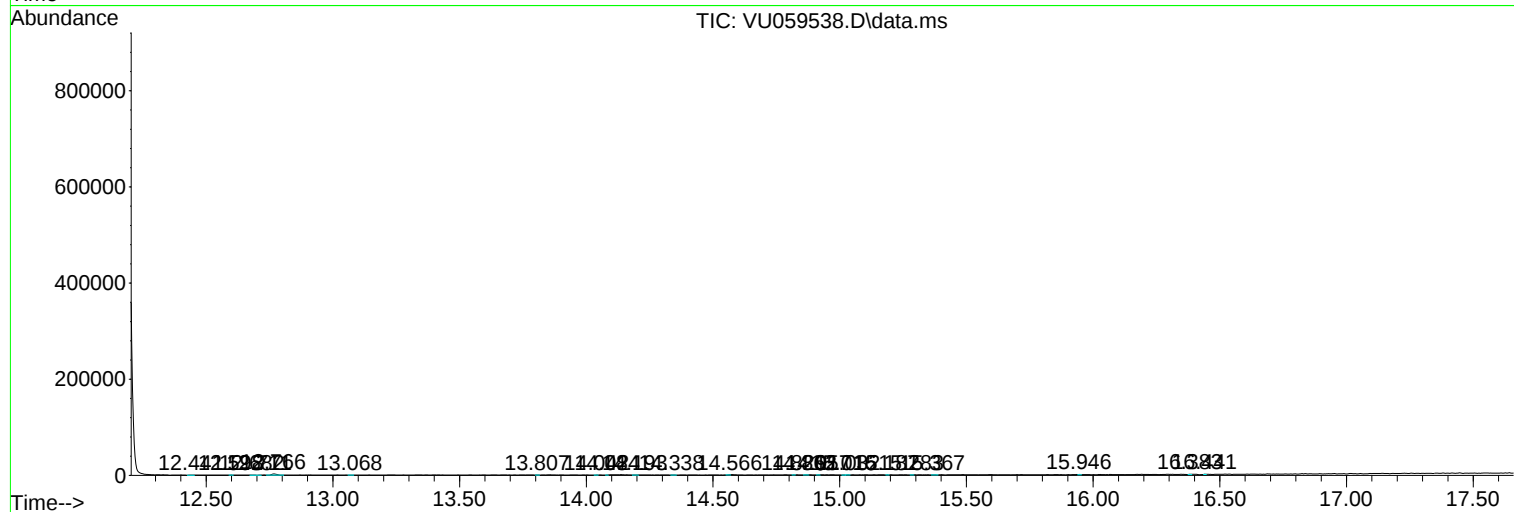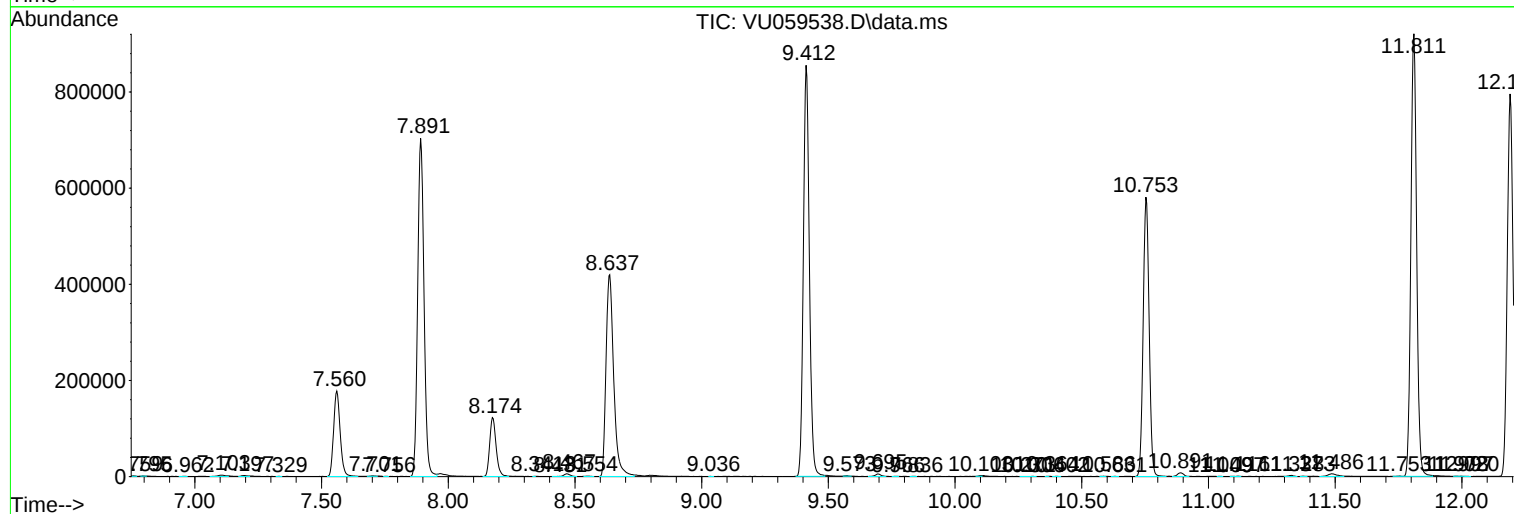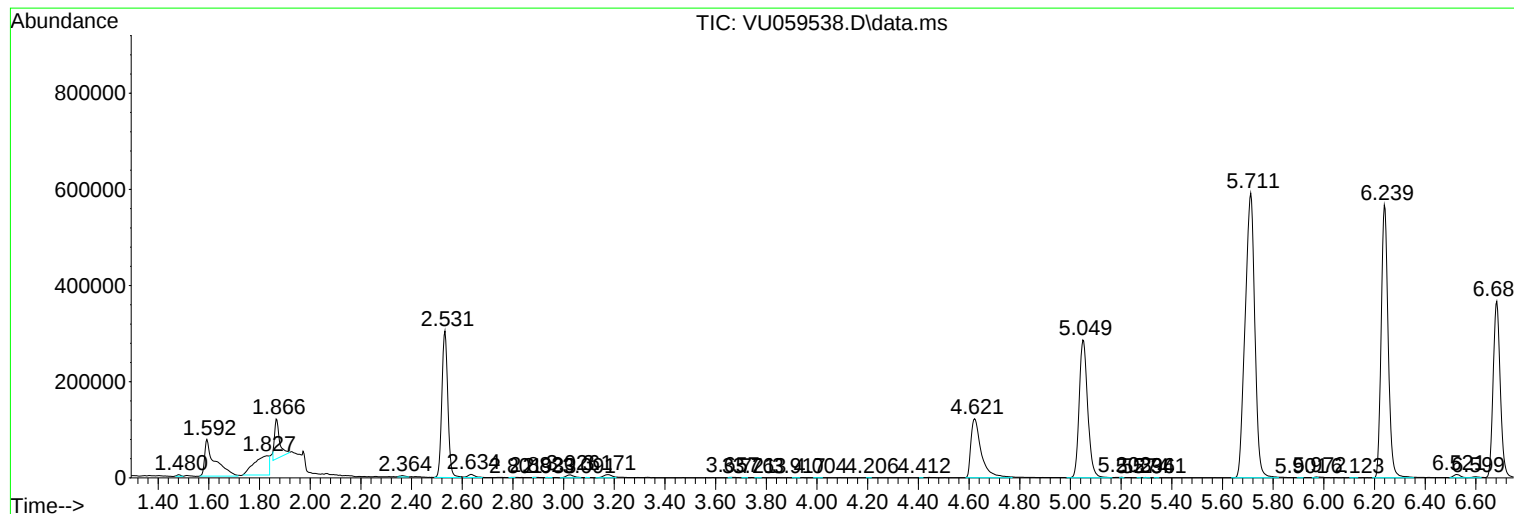

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
Data File : VU059536.D
Acq On : 26 Jun 2024 20:57
Operator : MD/SY
Sample : P3055-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08D1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
Data File : VU059536.D
Acq On : 26 Jun 2024 20:57
Operator : MD/SY
Sample : P3055-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08D1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc