

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
 Data File : VU059537.D
 Acq On : 26 Jun 2024 21:21
 Operator : MD/SY
 Sample : P3055-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08D2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M

Title : VOC Analysis

Signal : TIC: VU059539.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.483	56	60	66	rVB4	1651	1790	0.26%	0.033%
2	1.595	87	95	115	rBV	82516	101789	15.04%	1.863%
3	1.679	116	121	126	rVV	2355	2543	0.38%	0.047%
4	1.782	138	153	166	rBV3	22291	47665	7.04%	0.872%
5	1.901	182	190	209	rVB	62456	90799	13.42%	1.662%
6	2.222	288	290	292	rBV2	696	263	0.04%	0.005%
7	2.557	382	394	407	rBV	134201	218578	32.31%	4.000%
8	2.621	407	414	427	rVB2	5928	9768	1.44%	0.179%
9	2.769	456	460	461	rBV2	318	231	0.03%	0.004%
10	3.039	535	544	555	rVB4	2516	4770	0.70%	0.087%
11	3.171	574	585	586	rBV3	3442	3927	0.58%	0.072%
12	3.264	606	614	619	rBV2	267	402	0.06%	0.007%
13	3.322	626	632	635	rBV2	194	247	0.04%	0.005%
14	3.351	635	641	647	rVB3	646	833	0.12%	0.015%
15	3.476	676	680	684	rVB2	260	192	0.03%	0.004%
16	3.586	711	714	720	rVB3	256	216	0.03%	0.004%
17	3.640	726	731	735	rBV2	183	190	0.03%	0.003%
18	3.785	764	776	779	rBV2	261	367	0.05%	0.007%
19	3.997	837	842	845	rVV2	186	181	0.03%	0.003%
20	4.425	969	975	983	rBV4	672	1174	0.17%	0.021%
21	4.615	1024	1034	1069	rBV	70638	182271	26.94%	3.335%
22	4.926	1128	1131	1137	rVB2	283	280	0.04%	0.005%
23	5.055	1154	1171	1195	rBV	127400	308035	45.53%	5.637%
24	5.216	1216	1221	1225	rBV	354	357	0.05%	0.007%
25	5.338	1255	1259	1265	rBV2	160	181	0.03%	0.003%
26	5.402	1275	1279	1283	rVB2	343	246	0.04%	0.005%
27	5.569	1329	1331	1339	rVB	223	212	0.03%	0.004%
28	5.717	1356	1377	1405	rVV2	248385	676605	100.00%	12.382%
29	6.007	1464	1467	1471	rVB2	246	179	0.03%	0.003%
30	6.052	1477	1481	1484	rVB2	223	187	0.03%	0.003%
31	6.164	1514	1516	1523	rVB2	261	246	0.04%	0.005%
32	6.241	1528	1540	1566	rBV	244594	463765	68.54%	8.487%
33	6.499	1615	1620	1621	rBV2	277	210	0.03%	0.004%
34	6.531	1621	1630	1641	rVB4	2216	4018	0.59%	0.074%
35	6.573	1641	1643	1647	rBV2	363	230	0.03%	0.004%
36	6.685	1663	1678	1700	rVV	152930	300953	44.48%	5.507%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
 Data File : VU059537.D
 Acq On : 26 Jun 2024 21:21
 Operator : MD/SY
 Sample : P3055-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08D2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

37	6.801	1711	1714	1716	rVV2	333	252	0.04%	0.005%
38	6.814	1716	1718	1724	rVB4	707	538	0.08%	0.010%
39	7.106	1798	1809	1821	rBV4	3193	6640	0.98%	0.122%
40	7.196	1832	1837	1843	rBV3	809	1016	0.15%	0.019%
41	7.473	1920	1923	1928	rVB2	263	225	0.03%	0.004%
42	7.560	1938	1950	1978	rVV2	74332	134443	19.87%	2.460%
43	7.708	1992	1996	1997	rBV2	571	300	0.04%	0.005%
44	7.894	2039	2054	2069	rBV	283341	498427	73.67%	9.121%
45	8.097	2113	2117	2123	rVB2	416	425	0.06%	0.008%
46	8.135	2123	2129	2130	rBV2	326	273	0.04%	0.005%
47	8.177	2131	2142	2165	rVV	52187	87666	12.96%	1.604%
48	8.286	2174	2176	2181	rVB3	351	331	0.05%	0.006%
49	8.341	2187	2193	2196	rVB	281	281	0.04%	0.005%
50	8.463	2223	2231	2241	rBV3	1730	2671	0.39%	0.049%
51	8.627	2271	2282	2314	rBV	181800	350135	51.75%	6.407%
52	8.794	2328	2334	2347	rVB6	2375	3890	0.57%	0.071%
53	8.852	2351	2352	2357	rVB3	316	208	0.03%	0.004%
54	8.984	2390	2393	2398	rVB2	188	210	0.03%	0.004%
55	9.016	2398	2403	2408	rBV	224	250	0.04%	0.005%
56	9.058	2412	2416	2419	rBV	261	180	0.03%	0.003%
57	9.087	2423	2425	2430	rBV2	278	200	0.03%	0.004%
58	9.135	2436	2440	2444	rVB	222	176	0.03%	0.003%
59	9.412	2513	2526	2566	rVV	347825	591106	87.36%	10.817%
60	9.550	2566	2569	2570	rBV2	306	194	0.03%	0.004%
61	9.698	2606	2615	2625	rVB3	1688	2965	0.44%	0.054%
62	9.891	2672	2675	2681	rVB2	229	189	0.03%	0.003%
63	9.962	2688	2697	2700	rBV2	407	574	0.08%	0.011%
64	10.100	2735	2740	2751	rVB3	648	859	0.13%	0.016%
65	10.357	2812	2820	2822	rBV2	158	230	0.03%	0.004%
66	10.486	2851	2860	2863	rBV2	273	415	0.06%	0.008%
67	10.531	2870	2874	2877	rBV2	261	209	0.03%	0.004%
68	10.573	2882	2887	2891	rBV4	735	647	0.10%	0.012%
69	10.749	2929	2942	2961	rBV	240008	383945	56.75%	7.026%
70	10.891	2976	2986	2996	rVB2	3047	4564	0.67%	0.084%
71	11.026	3024	3028	3030	rVB3	218	179	0.03%	0.003%
72	11.055	3030	3037	3039	rBV2	216	244	0.04%	0.004%
73	11.322	3114	3120	3128	rVB3	1810	2454	0.36%	0.045%
74	11.383	3136	3139	3141	rBV	391	216	0.03%	0.004%
75	11.482	3162	3170	3187	rBV6	4992	10769	1.59%	0.197%
76	11.807	3260	3271	3296	rBV	309861	502960	74.34%	9.204%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
 Data File : VU059537.D
 Acq On : 26 Jun 2024 21:21
 Operator : MD/SY
 Sample : P3055-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08D2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

77	11.978	3321	3324	3327	rVB3	385	185	0.03%	0.003%
78	12.190	3377	3390	3411	rBV	266243	440432	65.09%	8.060%
79	12.418	3457	3461	3467	rBV2	380	400	0.06%	0.007%
80	12.476	3475	3479	3482	rBV2	318	255	0.04%	0.005%
81	12.492	3482	3484	3488	rVB2	355	188	0.03%	0.003%
82	12.608	3515	3520	3523	rBV2	292	294	0.04%	0.005%
83	12.772	3560	3571	3579	rBV4	1060	2025	0.30%	0.037%
84	13.315	3738	3740	3744	rVB	314	202	0.03%	0.004%
85	13.489	3791	3794	3797	rBV	332	195	0.03%	0.004%
86	13.547	3809	3812	3817	rVB2	452	382	0.06%	0.007%
87	13.569	3817	3819	3822	rBV2	347	210	0.03%	0.004%
88	13.653	3842	3845	3847	rBV2	291	185	0.03%	0.003%
89	13.907	3921	3924	3929	rBV2	423	410	0.06%	0.008%
90	13.958	3937	3940	3944	rBV	243	191	0.03%	0.003%
91	13.978	3944	3946	3952	rVB3	264	234	0.03%	0.004%
92	14.630	4146	4149	4152	rBV	398	284	0.04%	0.005%
93	14.743	4181	4184	4191	rBV2	357	404	0.06%	0.007%
94	14.968	4251	4254	4259	rVB2	414	301	0.04%	0.006%
95	15.000	4260	4264	4266	rBV2	392	320	0.05%	0.006%
96	15.193	4321	4324	4327	rVB3	371	283	0.04%	0.005%
97	15.215	4327	4331	4334	rBV3	607	586	0.09%	0.011%
98	15.408	4389	4391	4395	rBV3	423	374	0.06%	0.007%
99	15.614	4452	4455	4457	rBV2	496	284	0.04%	0.005%
100	15.942	4554	4557	4562	rBV3	819	633	0.09%	0.012%




Sum of corrected areas: 5464613

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
Data File : VU059537.D
Acq On : 26 Jun 2024 21:21
Operator : MD/SY
Sample : P3055-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08D2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

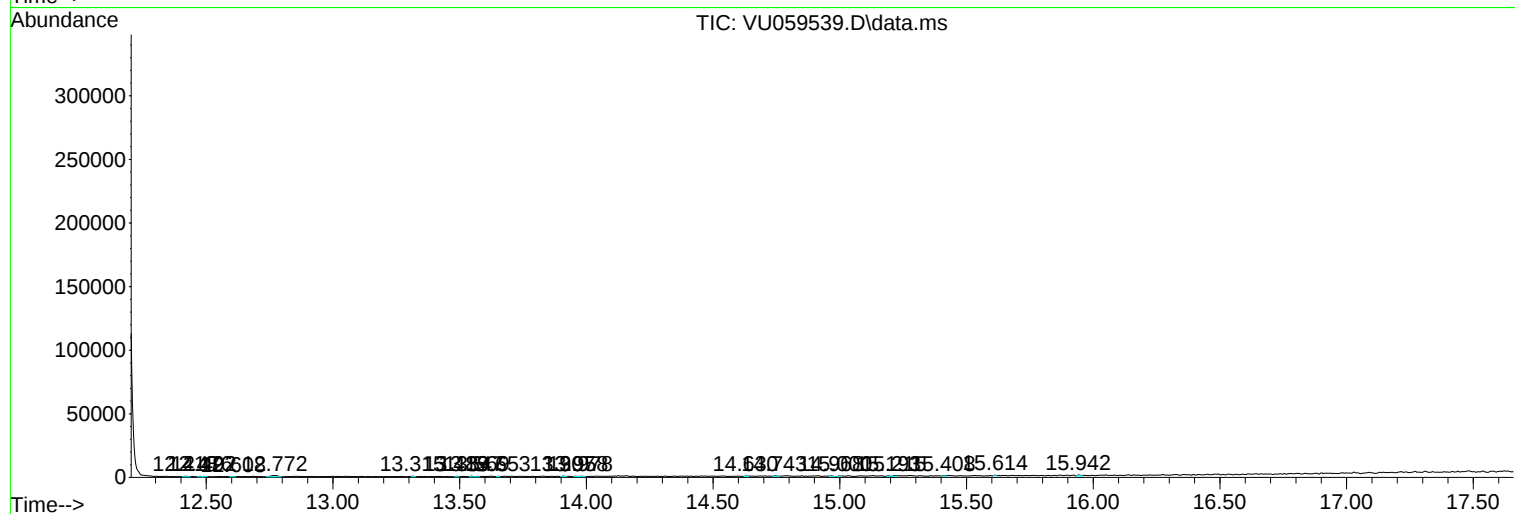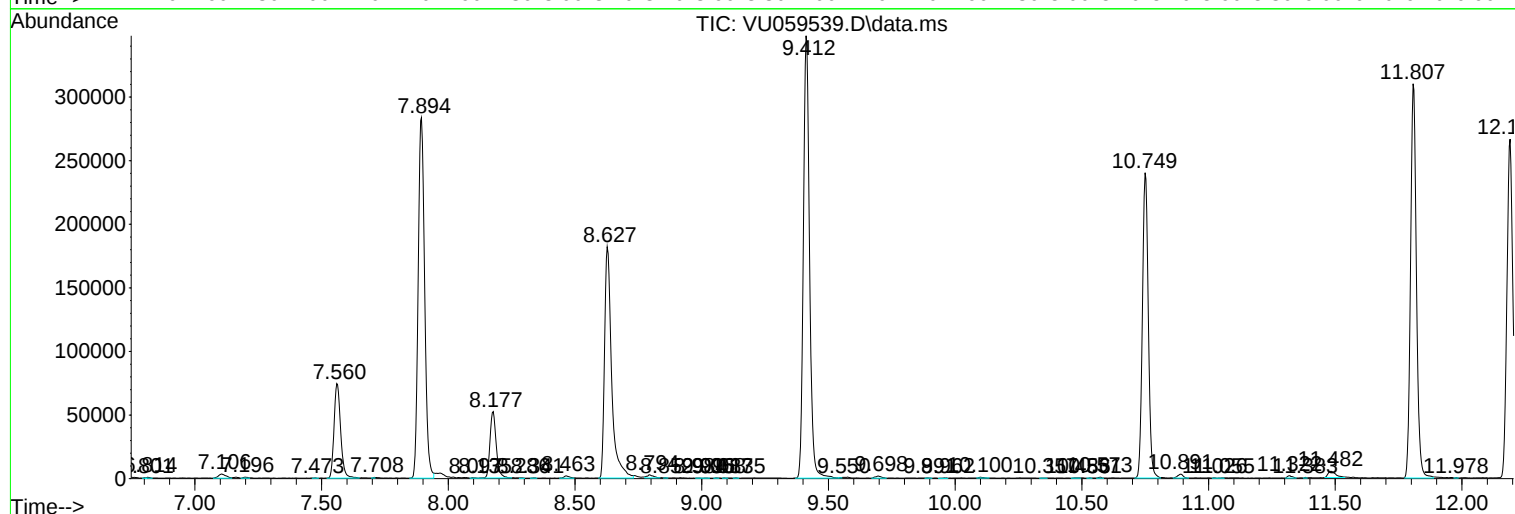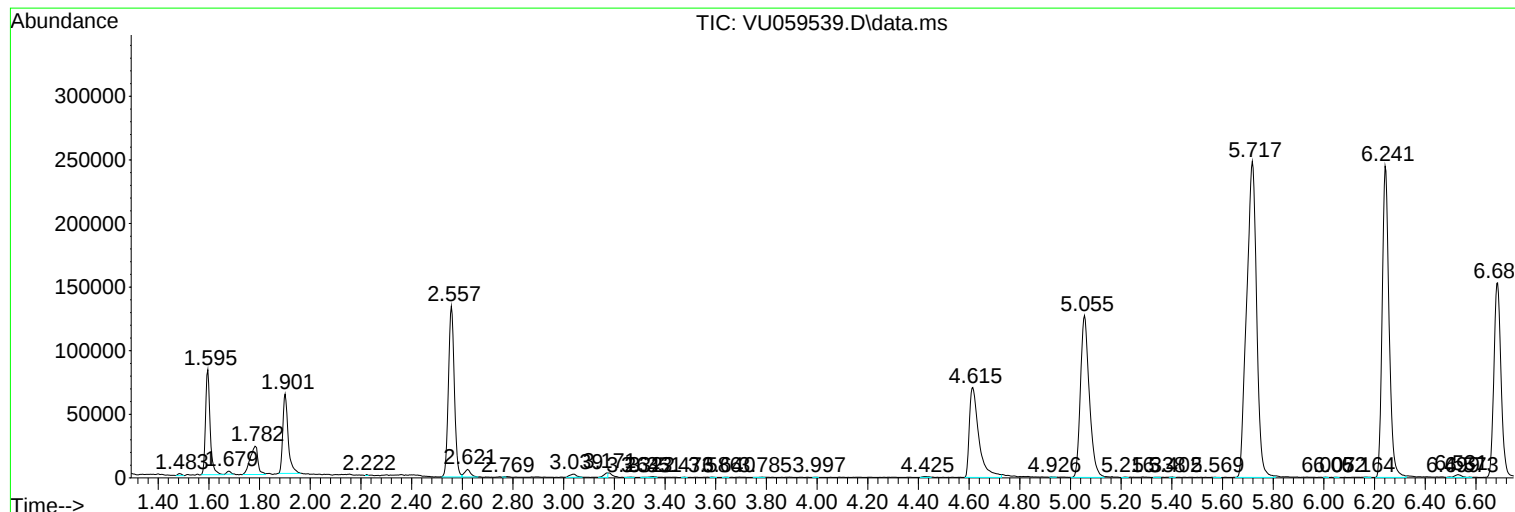

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
Data File : VU059537.D
Acq On : 26 Jun 2024 21:21
Operator : MD/SY
Sample : P3055-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08D2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
Data File : VU059537.D
Acq On : 26 Jun 2024 21:21
Operator : MD/SY
Sample : P3055-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08D2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------