

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
 Data File : VU059538.D
 Acq On : 26 Jun 2024 21:43
 Operator : MD/SY
 Sample : P3055-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08D4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

Signal : TIC: VU059540.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.592	87	94	117	rVB	81013	101869	15.25%	1.897%
2	1.895	181	188	209	rVB	60499	89577	13.41%	1.668%
3	2.554	381	393	408	rBV	133549	215644	32.29%	4.016%
4	2.753	452	455	461	rVB3	371	391	0.06%	0.007%
5	2.946	510	515	518	rBV3	298	318	0.05%	0.006%
6	3.036	533	543	559	rVB5	3376	6580	0.99%	0.123%
7	3.123	567	570	573	rBV2	172	136	0.02%	0.003%
8	3.174	576	586	601	rVB2	2100	4081	0.61%	0.076%
9	3.412	657	660	662	rBV	139	76	0.01%	0.001%
10	3.557	702	705	708	rBV	180	128	0.02%	0.002%
11	3.663	736	738	739	rBV2	94	44	0.01%	0.001%
12	3.695	745	748	750	rBV	259	172	0.03%	0.003%
13	3.811	781	784	787	rBV	206	131	0.02%	0.002%
14	3.933	819	822	826	rBV2	101	72	0.01%	0.001%
15	3.988	836	839	845	rBV2	235	168	0.03%	0.003%
16	4.116	876	879	881	rBV2	84	57	0.01%	0.001%
17	4.184	892	900	903	rBV	226	224	0.03%	0.004%
18	4.203	903	906	911	rBV2	234	201	0.03%	0.004%
19	4.290	930	933	936	rBV	155	103	0.02%	0.002%
20	4.386	960	963	968	rBV2	187	187	0.03%	0.003%
21	4.489	993	995	997	rBV	108	71	0.01%	0.001%
22	4.570	1017	1020	1023	rBV	216	162	0.02%	0.003%
23	4.611	1023	1033	1064	rBV	71713	176647	26.45%	3.290%
24	4.910	1125	1126	1127	rBV	154	51	0.01%	0.001%
25	5.052	1154	1170	1192	rBV	123040	271014	40.58%	5.048%
26	5.229	1223	1225	1228	rVB2	215	105	0.02%	0.002%
27	5.287	1239	1243	1247	rVB3	616	477	0.07%	0.009%
28	5.306	1247	1249	1251	rVB2	149	67	0.01%	0.001%
29	5.348	1256	1262	1265	rVB2	162	193	0.03%	0.004%
30	5.370	1265	1269	1273	rVB	275	208	0.03%	0.004%
31	5.393	1273	1276	1278	rBV	108	84	0.01%	0.002%
32	5.528	1314	1318	1321	rVB2	184	137	0.02%	0.003%
33	5.557	1322	1327	1329	rBV	231	209	0.03%	0.004%
34	5.615	1343	1345	1346	rBV	92	44	0.01%	0.001%
35	5.714	1357	1376	1405	rBV2	243665	667793	100.00%	12.437%
36	5.917	1436	1439	1442	rVB3	225	135	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
 Data File : VU059538.D
 Acq On : 26 Jun 2024 21:43
 Operator : MD/SY
 Sample : P3055-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08D4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

37	5.936	1442	1445	1447	rBV2	182	138	0.02%	0.003%
38	5.968	1452	1455	1456	rBV2	183	91	0.01%	0.002%
39	5.994	1460	1463	1465	rBV2	168	115	0.02%	0.002%
40	6.026	1469	1473	1477	rBV	233	221	0.03%	0.004%
41	6.062	1481	1484	1486	rBV2	151	94	0.01%	0.002%
42	6.242	1527	1540	1568	rBV	243311	471675	70.63%	8.785%
43	6.528	1621	1629	1640	rBV6	2254	3744	0.56%	0.070%
44	6.618	1655	1657	1661	rVB2	199	116	0.02%	0.002%
45	6.682	1661	1677	1695	rBV	155642	300501	45.00%	5.597%
46	6.798	1707	1713	1716	rBV3	602	533	0.08%	0.010%
47	6.952	1757	1761	1765	rVB2	228	212	0.03%	0.004%
48	6.981	1765	1770	1772	rBV2	194	178	0.03%	0.003%
49	7.100	1803	1807	1812	rVB3	404	356	0.05%	0.007%
50	7.181	1827	1832	1834	rBV2	465	366	0.05%	0.007%
51	7.309	1867	1872	1876	rBV2	229	212	0.03%	0.004%
52	7.328	1876	1878	1881	rVB2	74	43	0.01%	0.001%
53	7.348	1881	1884	1887	rBV	163	130	0.02%	0.002%
54	7.435	1907	1911	1915	rBV2	154	144	0.02%	0.003%
55	7.460	1915	1919	1925	rBV2	252	273	0.04%	0.005%
56	7.560	1934	1950	1974	rBV	75295	132502	19.84%	2.468%
57	7.701	1990	1994	1998	rBV3	543	528	0.08%	0.010%
58	7.891	2040	2053	2073	rBV	283895	498800	74.69%	9.290%
59	8.103	2114	2119	2122	rBV2	228	211	0.03%	0.004%
60	8.174	2131	2141	2161	rBV	51142	87821	13.15%	1.636%
61	8.418	2213	2217	2220	rBV2	262	217	0.03%	0.004%
62	8.467	2223	2232	2239	rBV	2818	4147	0.62%	0.077%
63	8.576	2260	2266	2268	rBV2	319	215	0.03%	0.004%
64	8.627	2272	2282	2319	rBV	186926	356009	53.31%	6.631%
65	8.881	2357	2361	2366	rBV3	301	293	0.04%	0.005%
66	8.984	2386	2393	2398	rBV2	215	278	0.04%	0.005%
67	9.090	2423	2426	2427	rBV	133	62	0.01%	0.001%
68	9.145	2440	2443	2446	rVB	286	184	0.03%	0.003%
69	9.158	2446	2447	2448	rBV	191	53	0.01%	0.001%
70	9.354	2506	2508	2513	rVB2	178	140	0.02%	0.003%
71	9.412	2513	2526	2554	rBV	359846	602340	90.20%	11.218%
72	9.634	2591	2595	2597	rBV2	203	184	0.03%	0.003%
73	9.737	2624	2627	2628	rBV	153	88	0.01%	0.002%
74	9.830	2649	2656	2661	rBV2	257	328	0.05%	0.006%
75	9.856	2661	2664	2665	rBV	156	84	0.01%	0.002%
76	9.920	2682	2684	2688	rVB2	132	79	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
 Data File : VU059538.D
 Acq On : 26 Jun 2024 21:43
 Operator : MD/SY
 Sample : P3055-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08D4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

77	9.942	2688	2691	2697	rBV	227	170	0.03%	0.003%
78	9.968	2697	2699	2701	rBV	140	86	0.01%	0.002%
79	10.097	2730	2739	2750	rBV2	12870	19614	2.94%	0.365%
80	10.171	2759	2762	2765	rBV2	330	151	0.02%	0.003%
81	10.286	2793	2798	2802	rBV4	359	414	0.06%	0.008%
82	10.383	2826	2828	2829	rBV4	141	45	0.01%	0.001%
83	10.749	2929	2942	2966	rBV	236242	382084	57.22%	7.116%
84	10.888	2976	2985	2995	rVB2	4775	7231	1.08%	0.135%
85	11.325	3115	3121	3128	rBV3	1444	1623	0.24%	0.030%
86	11.479	3166	3169	3171	rBV	256	119	0.02%	0.002%
87	11.807	3259	3271	3293	rBV	314683	517219	77.45%	9.633%
88	12.190	3377	3390	3413	rBV	258274	439059	65.75%	8.177%
89	13.846	3903	3905	3909	rBV2	300	159	0.02%	0.003%




Sum of corrected areas: 5369235

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
Data File : VU059538.D
Acq On : 26 Jun 2024 21:43
Operator : MD/SY
Sample : P3055-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08D4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

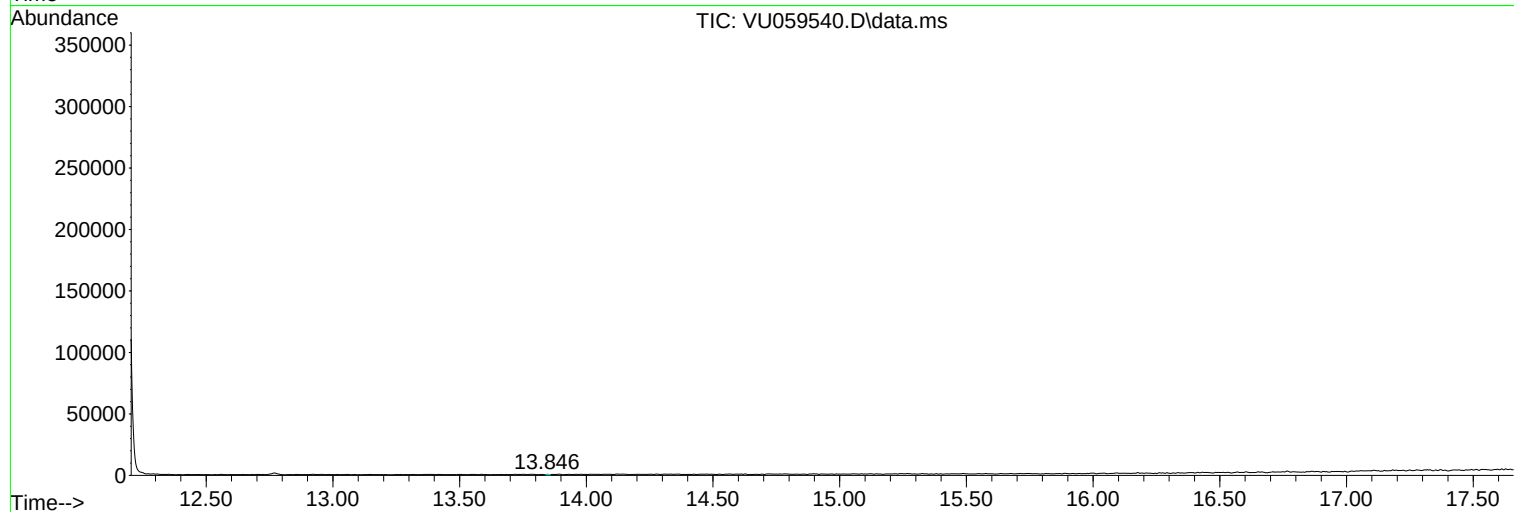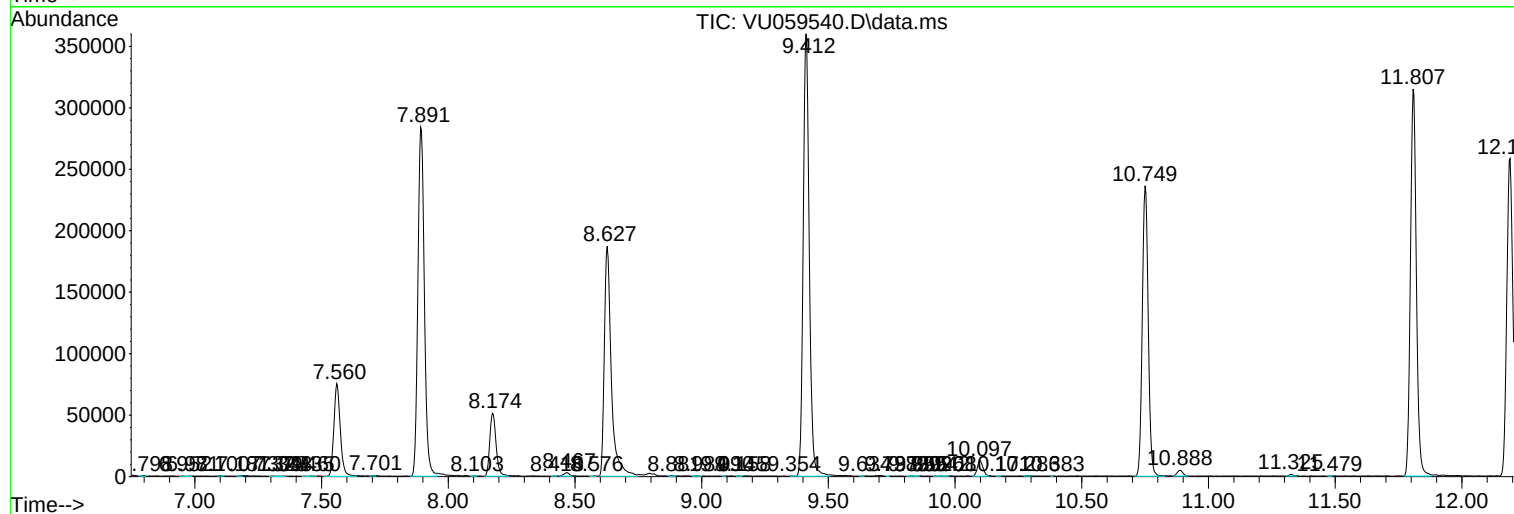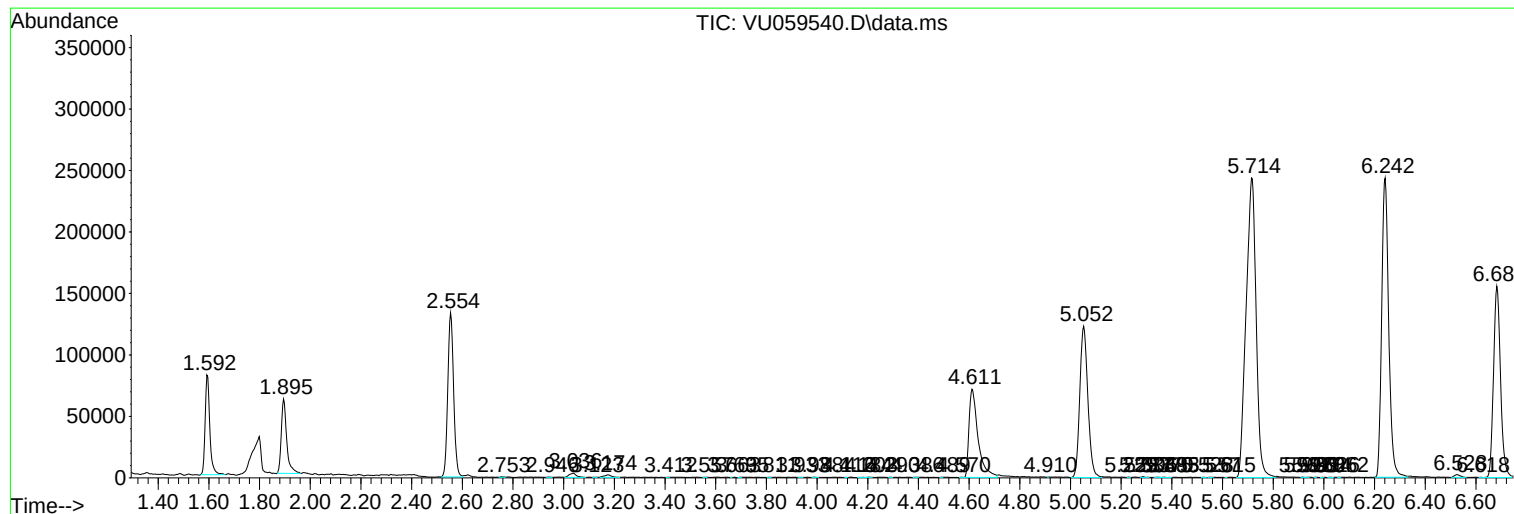

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
Data File : VU059538.D
Acq On : 26 Jun 2024 21:43
Operator : MD/SY
Sample : P3055-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08D4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
Data File : VU059538.D
Acq On : 26 Jun 2024 21:43
Operator : MD/SY
Sample : P3055-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08D4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------