

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
 Data File : VU059543.D
 Acq On : 26 Jun 2024 23:38
 Operator : MD/SY
 Sample : P3055-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08D7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M

Title : VOC Analysis

Signal : TIC: VU059545.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.489	57	62	68	rVB	3071	3340	0.52%	0.064%
2	1.596	87	95	114	rBV	82782	101517	15.76%	1.933%
3	1.766	139	148	157	rBV3	5976	9327	1.45%	0.178%
4	1.907	184	192	208	rBV	63760	90898	14.11%	1.731%
5	2.457	361	363	366	rVB3	345	166	0.03%	0.003%
6	2.560	383	395	408	rBV	125686	206163	32.00%	3.926%
7	2.624	410	415	427	rVB2	3608	6112	0.95%	0.116%
8	2.759	454	457	460	rVB3	353	215	0.03%	0.004%
9	2.837	477	481	483	rBV	338	216	0.03%	0.004%
10	2.895	495	499	500	rBV	289	209	0.03%	0.004%
11	2.997	525	531	535	rBV	343	338	0.05%	0.006%
12	3.036	535	543	554	rVB4	2892	5198	0.81%	0.099%
13	3.081	554	557	560	rBV	213	179	0.03%	0.003%
14	3.171	579	585	588	rBV3	751	962	0.15%	0.018%
15	3.290	618	622	626	rVV2	215	203	0.03%	0.004%
16	3.358	640	643	647	rVV2	237	175	0.03%	0.003%
17	3.383	648	651	656	rVV2	183	182	0.03%	0.003%
18	3.412	656	660	668	rVB2	206	234	0.04%	0.004%
19	3.499	681	687	689	rBV2	165	185	0.03%	0.004%
20	3.605	714	720	725	rVB2	244	250	0.04%	0.005%
21	3.949	824	827	831	rVB2	264	217	0.03%	0.004%
22	3.984	831	838	839	rBV2	280	311	0.05%	0.006%
23	4.007	839	845	847	rBV2	196	216	0.03%	0.004%
24	4.116	874	879	883	rVB2	157	159	0.02%	0.003%
25	4.267	921	926	931	rBV2	292	379	0.06%	0.007%
26	4.351	949	952	956	rVB2	264	163	0.03%	0.003%
27	4.496	992	997	1000	rVB2	183	162	0.03%	0.003%
28	4.618	1025	1035	1059	rBV	67658	168035	26.08%	3.200%
29	4.811	1092	1095	1097	rBV2	627	366	0.06%	0.007%
30	5.058	1156	1172	1195	rBV2	125674	328527	50.99%	6.257%
31	5.721	1357	1378	1406	rBV2	236974	644330	100.00%	12.272%
32	5.997	1460	1464	1466	rBV2	276	206	0.03%	0.004%
33	6.091	1489	1493	1495	rBV2	291	198	0.03%	0.004%
34	6.174	1515	1519	1525	rVB	231	259	0.04%	0.005%
35	6.245	1526	1541	1561	rBV	235134	454013	70.46%	8.647%
36	6.496	1614	1619	1622	rBV2	218	231	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
Data File : VU059543.D
Acq On : 26 Jun 2024 23:38
Operator : MD/SY
Sample : P3055-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08D7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Title : VOC Analysis

37	6.531	1622	1630	1643	rVB5	2206	4025	0.62%	0.077%
38	6.685	1664	1678	1702	rBV	146567	289394	44.91%	5.512%
39	6.808	1714	1716	1719	rVB2	666	356	0.06%	0.007%
40	7.103	1797	1808	1824	rBV2	7224	13560	2.10%	0.258%

41	7.200	1832	1838	1844	rBV3	572	731	0.11%	0.014%
42	7.563	1939	1951	1972	rBV	68533	125195	19.43%	2.384%
43	7.698	1990	1993	1995	rBV3	292	160	0.02%	0.003%
44	7.711	1995	1997	2006	rVB4	654	677	0.11%	0.013%
45	7.753	2007	2010	2013	rBV	299	157	0.02%	0.003%

46	7.824	2029	2032	2040	rVB2	250	302	0.05%	0.006%
47	7.894	2041	2054	2074	rBV	272005	475115	73.74%	9.049%
48	8.100	2115	2118	2121	rVB2	333	209	0.03%	0.004%
49	8.177	2132	2142	2156	rBV	48275	82586	12.82%	1.573%
50	8.393	2206	2209	2215	rBV	278	228	0.04%	0.004%

51	8.467	2226	2232	2240	rBV3	822	1258	0.20%	0.024%
52	8.627	2272	2282	2314	rBV	168498	338776	52.58%	6.452%
53	8.804	2331	2337	2346	rVB6	2252	4003	0.62%	0.076%
54	8.878	2358	2360	2364	rVB2	315	171	0.03%	0.003%
55	8.914	2368	2371	2373	rBV2	224	154	0.02%	0.003%

56	9.270	2476	2482	2485	rBV2	234	262	0.04%	0.005%
57	9.332	2498	2501	2508	rVB2	198	186	0.03%	0.004%
58	9.412	2514	2526	2548	rBV	338553	581574	90.26%	11.076%
59	9.618	2587	2590	2593	rBV2	196	161	0.02%	0.003%
60	9.701	2612	2616	2620	rVB2	320	248	0.04%	0.005%

61	10.119	2741	2746	2748	rBV2	195	168	0.03%	0.003%
62	10.312	2799	2806	2809	rBV	299	288	0.04%	0.005%
63	10.386	2826	2829	2835	rBV2	169	210	0.03%	0.004%
64	10.576	2883	2888	2892	rBV2	158	181	0.03%	0.003%
65	10.666	2911	2916	2919	rBV2	239	215	0.03%	0.004%

66	10.749	2929	2942	2966	rBV	227402	370085	57.44%	7.048%
67	10.894	2979	2987	2993	rVB4	1197	1805	0.28%	0.034%
68	10.930	2993	2998	3000	rBV2	223	156	0.02%	0.003%
69	10.946	3000	3003	3007	rBV	156	165	0.03%	0.003%
70	11.042	3030	3033	3039	rVB2	296	279	0.04%	0.005%

71	11.139	3057	3063	3064	rBV	188	177	0.03%	0.003%
72	11.505	3172	3177	3180	rBV3	536	492	0.08%	0.009%
73	11.746	3249	3252	3258	rBV3	371	264	0.04%	0.005%
74	11.807	3258	3271	3299	rBV	302221	501705	77.86%	9.555%
75	11.975	3319	3323	3326	rBV2	360	270	0.04%	0.005%

76	12.087	3355	3358	3363	rBV2	201	158	0.02%	0.003%
----	--------	------	------	------	------	-----	-----	-------	--------

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
 Data File : VU059543.D
 Acq On : 26 Jun 2024 23:38
 Operator : MD/SY
 Sample : P3055-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08D7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

77	12.190	3377	3390	3414	rBV	253593	424545	65.89%	8.086%
78	12.775	3565	3572	3575	rBV	414	474	0.07%	0.009%
79	12.807	3579	3582	3586	rBV2	240	201	0.03%	0.004%
80	12.875	3600	3603	3608	rBV2	232	236	0.04%	0.004%
81	12.929	3617	3620	3623	rVB	341	211	0.03%	0.004%
82	13.000	3638	3642	3646	rVB2	257	200	0.03%	0.004%
83	13.122	3676	3680	3685	rVB2	384	294	0.05%	0.006%
84	13.158	3688	3691	3697	rBV	178	169	0.03%	0.003%
85	13.418	3766	3772	3777	rBV2	302	389	0.06%	0.007%
86	13.479	3787	3791	3793	rBV2	179	158	0.02%	0.003%
87	13.598	3826	3828	3832	rVB3	343	215	0.03%	0.004%
88	13.692	3854	3857	3860	rVB2	269	183	0.03%	0.003%
89	13.711	3860	3863	3870	rVB	226	198	0.03%	0.004%
90	13.746	3871	3874	3877	rBV2	321	285	0.04%	0.005%
91	13.807	3890	3893	3894	rBV	455	251	0.04%	0.005%
92	14.013	3954	3957	3958	rBV	374	214	0.03%	0.004%
93	14.315	4048	4051	4052	rBV	363	215	0.03%	0.004%
94	14.794	4197	4200	4202	rBV2	358	272	0.04%	0.005%
95	14.836	4211	4213	4217	rVB2	379	243	0.04%	0.005%
96	15.052	4277	4280	4283	rBV2	319	239	0.04%	0.005%
97	15.103	4293	4296	4300	rBV2	509	488	0.08%	0.009%
98	15.183	4318	4321	4325	rBV	379	324	0.05%	0.006%
99	15.653	4464	4467	4469	rBV	391	306	0.05%	0.006%
100	15.746	4493	4496	4498	rBV2	602	350	0.05%	0.007%




Sum of corrected areas: 5250607

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
Data File : VU059543.D
Acq On : 26 Jun 2024 23:38
Operator : MD/SY
Sample : P3055-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08D7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

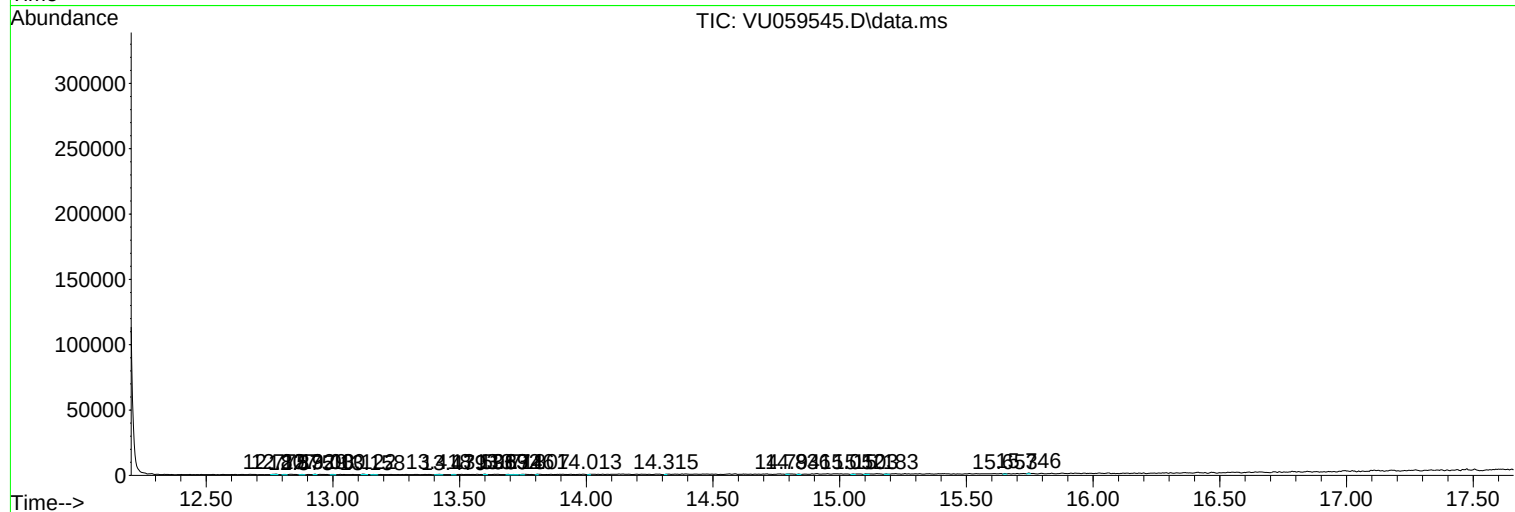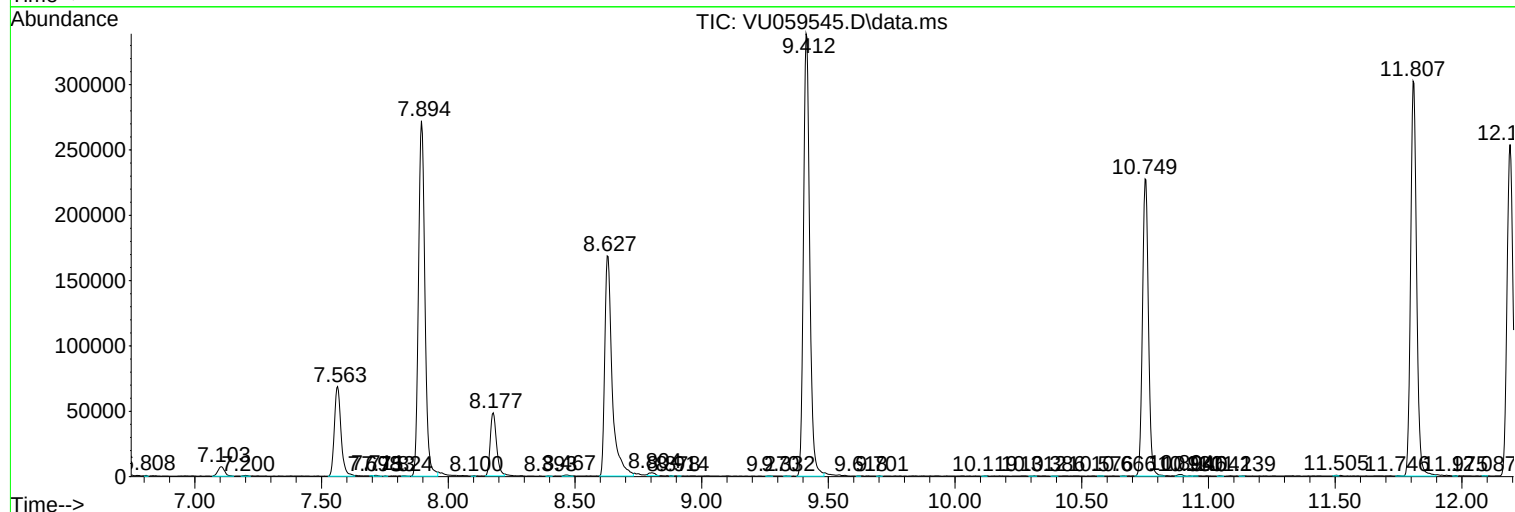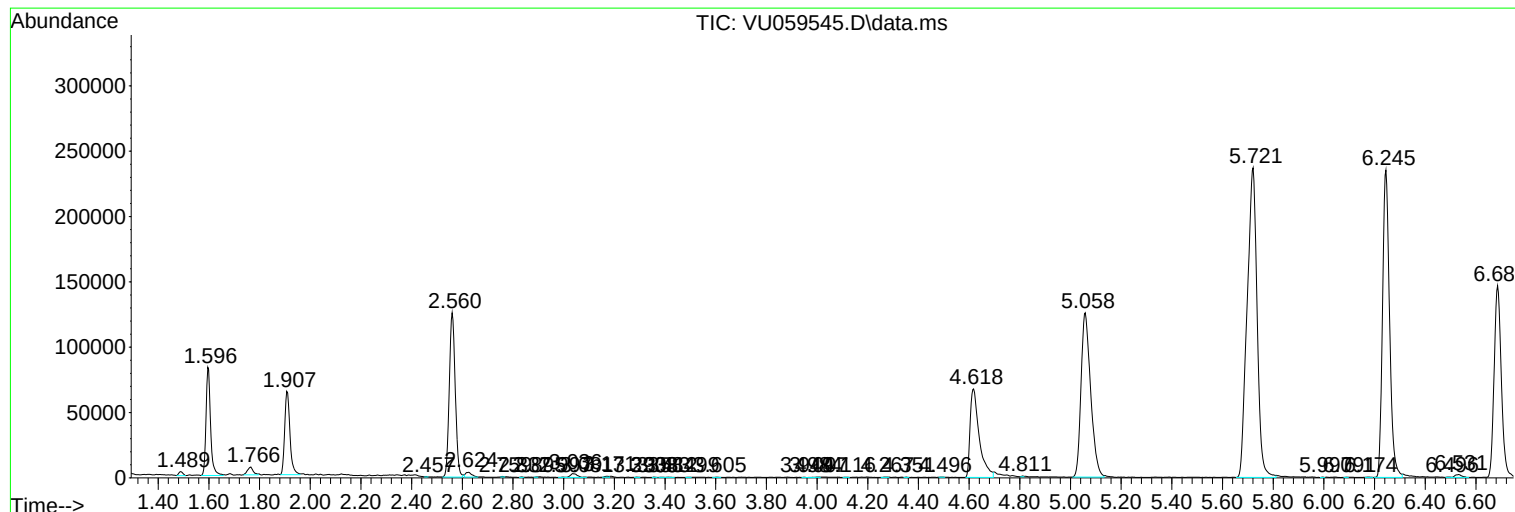

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
Data File : VU059543.D
Acq On : 26 Jun 2024 23:38
Operator : MD/SY
Sample : P3055-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08D7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
Data File : VU059543.D
Acq On : 26 Jun 2024 23:38
Operator : MD/SY
Sample : P3055-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08D7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------