


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062624\
Data File : VU059521.D
Acq On : 26 Jun 2024 12:43
Operator : MD/SY
Sample : BFB068
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB068

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Title : VOC Analysis
Last Update : Thu Jun 27 04:10:00 2024

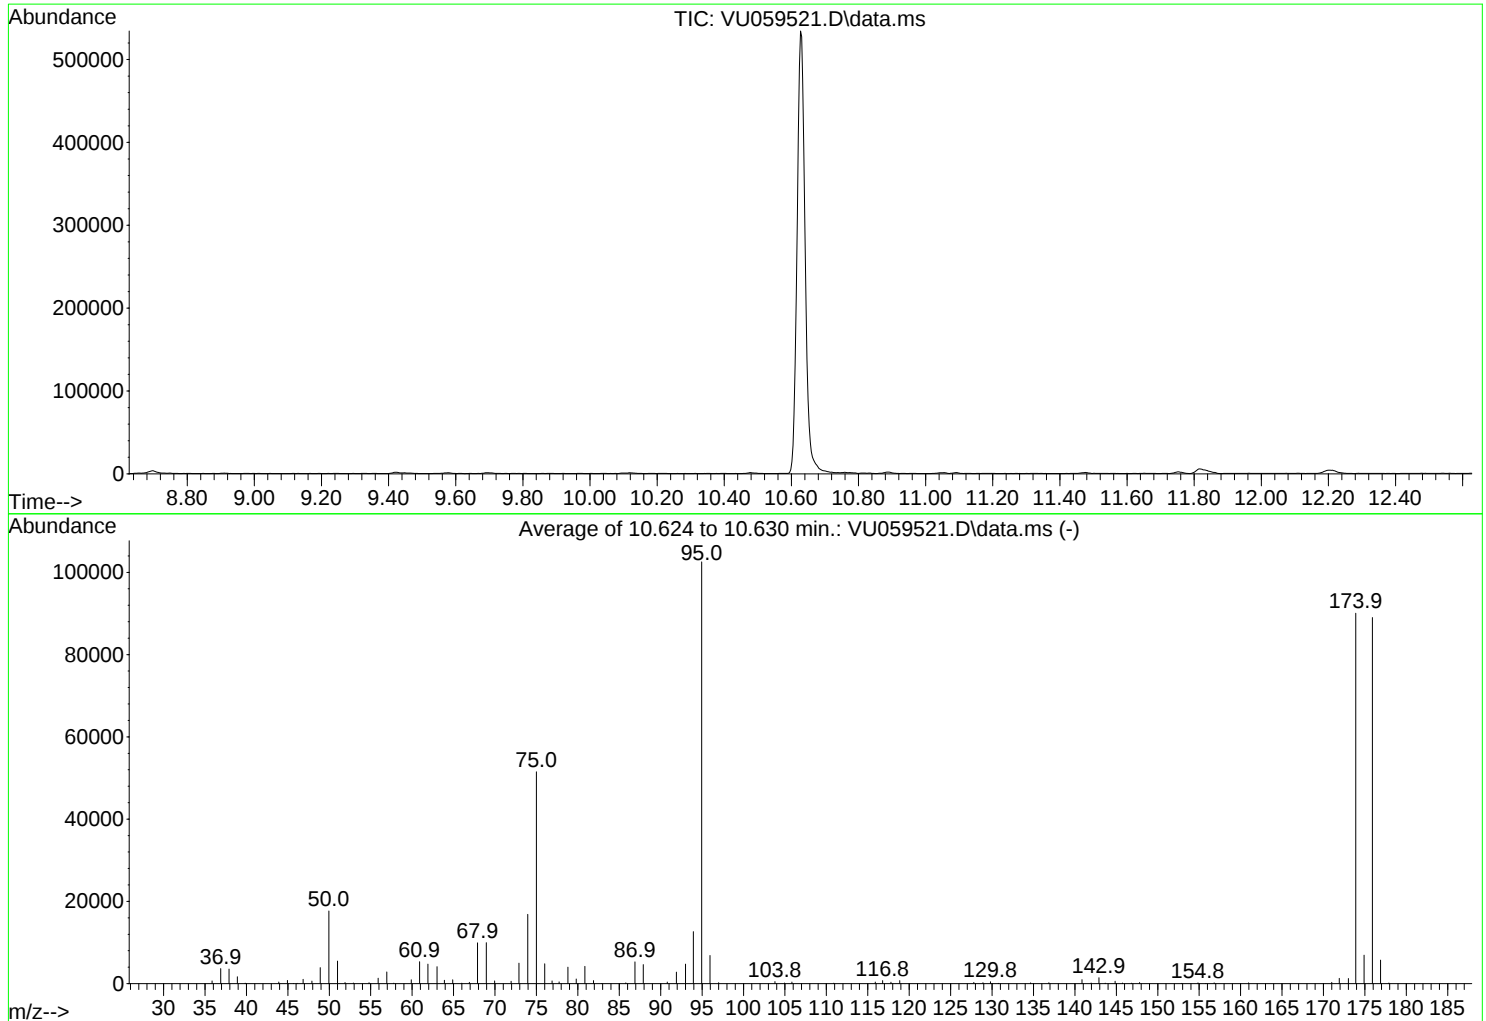

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2891

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.2	17651	PASS
75	95	30	80	50.2	51517	PASS
95	95	100	100	100.0	102557	PASS
96	95	5	9	6.7	6855	PASS
173	174	0.00	2	1.4	1254	PASS
174	95	50	120	87.8	90053	PASS
175	174	5	9	7.7	6924	PASS
176	174	95	101	98.9	89024	PASS
177	176	5	9	6.4	5715	PASS

m/z	Abundance
39.90	274.0
43.90	337.0

Instrument :
MSVOA_U
ClientSampleId :
BFB068

m/z	Abundance
35.90	644.0
36.90	3359.0
37.90	3481.0
38.90	1595.0
39.80	396.0
43.90	673.0
45.00	862.0
46.10	141.0
46.80	998.0
47.90	569.0
48.90	3853.0
49.90	16928.0
51.00	5304.0
51.90	319.0
52.90	190.0
54.80	258.0
55.90	1147.0
57.00	2692.0
57.80	128.0
59.90	977.0
60.90	5060.0
61.90	4553.0
63.00	4048.0
63.90	740.0
64.90	981.0
66.00	104.0
66.90	340.0
67.90	9555.0
69.00	9478.0
69.90	648.0
72.00	585.0
72.90	4765.0
73.90	16416.0
75.00	48960.0
76.00	4820.0
76.90	697.0
77.80	329.0
78.80	3993.0
79.80	1095.0
80.90	4238.0
81.90	654.0
85.80	184.0
86.90	5158.0
87.90	4481.0
90.80	404.0
91.90	2673.0
93.00	4700.0
94.00	12208.0
95.00	98288.0
96.00	6705.0
97.00	285.0
103.80	459.0
105.00	165.0
105.90	349.0
115.90	470.0
116.80	787.0
117.80	313.0
118.80	726.0
127.80	321.0
128.90	171.0
129.80	447.0
130.80	128.0
134.60	181.0
136.80	205.0
140.80	887.0
141.90	148.0
142.90	1344.0
143.70	117.0
144.90	592.0
145.70	144.0
146.80	118.0
147.80	317.0
154.90	204.0
156.80	171.0
160.90	171.0
171.00	295.0
171.90	1189.0
173.00	1285.0
173.90	84448.0
174.90	6554.0
175.90	82208.0
176.90	5325.0
177.90	128.0

Instrument :
MSVOA_U
ClientSampleId :
BFB068

m/z	Abundance
35.80	708.0
36.90	3767.0
37.90	3651.0
38.90	1733.0
39.90	397.0
43.90	753.0
45.00	778.0
46.10	106.0
46.90	1106.0
47.90	657.0
48.90	4000.0
49.90	18168.0
51.00	5712.0
51.90	301.0
52.90	188.0
54.80	248.0
55.90	1364.0
57.00	2928.0
57.80	155.0
59.90	974.0
60.90	5568.0
61.90	4926.0
63.00	4216.0
63.90	859.0
64.90	983.0
66.00	125.0
66.90	326.0
67.90	10231.0
68.90	10238.0
70.00	683.0
72.00	587.0
72.90	5099.0
73.90	17440.0
75.00	53192.0
76.00	4990.0
76.90	661.0
77.70	455.0
78.80	4134.0
79.80	1191.0
80.80	4351.0
81.90	791.0
85.80	175.0
86.90	5526.0
87.90	4852.0
90.80	426.0
91.90	2851.0
93.00	4892.0
94.00	13013.0
95.00	105752.0
95.90	7051.0
97.00	233.0
103.80	550.0
104.90	156.0
105.80	425.0
110.90	175.0
115.90	418.0
116.80	764.0
117.80	355.0
118.80	767.0
127.80	341.0
128.90	246.0
129.80	491.0
130.70	115.0
134.60	187.0
136.90	267.0
140.80	999.0
141.90	162.0
142.90	1477.0
143.60	134.0
144.80	608.0
145.70	153.0
146.80	136.0
147.80	278.0
152.90	106.0
154.90	219.0
156.80	186.0
161.00	218.0
170.00	123.0
171.00	328.0
171.90	1359.0
173.00	1276.0
173.90	92752.0
174.90	7147.0
175.90	91888.0
176.90	5877.0
177.90	170.0

Instrument :
MSVOA_U
ClientSampleId :
BFB068

m/z	Abundance
35.90	686.0
36.90	3887.0
37.90	3458.0
38.90	1727.0
39.90	414.0
43.90	805.0
44.90	670.0
45.70	105.0
46.90	1040.0
47.90	601.0
48.90	3796.0
50.00	17856.0
51.00	5498.0
51.90	255.0
52.90	150.0
54.80	198.0
55.90	1469.0
56.90	2937.0
57.80	102.0
59.90	829.0
60.90	5357.0
61.90	4803.0
63.00	4099.0
63.90	842.0
64.90	866.0
66.00	115.0
66.90	288.0
67.90	9999.0
68.90	10161.0
70.00	712.0
71.90	572.0
72.90	5057.0
74.00	16696.0
75.00	52400.0
76.00	4652.0
76.90	604.0
77.70	462.0
78.80	3870.0
79.80	1141.0
80.80	4072.0
81.90	829.0
82.90	110.0
85.80	180.0
86.90	5215.0
87.90	4555.0
90.80	390.0
91.90	2940.0
93.00	4672.0
93.90	12742.0
94.90	103632.0
95.90	6808.0
97.00	214.0
103.80	566.0
104.90	154.0
105.80	451.0
110.90	219.0
115.90	339.0
116.80	688.0
117.80	360.0
118.90	738.0
127.80	331.0
128.90	268.0
129.80	487.0
134.70	191.0
136.90	282.0
140.90	1080.0
142.00	125.0
142.90	1520.0
143.60	123.0
144.80	566.0
145.80	170.0
146.90	104.0
147.80	214.0
152.90	106.0
154.80	219.0
155.80	110.0
156.80	194.0
160.90	203.0
171.00	316.0
171.90	1353.0
173.00	1201.0
173.90	92960.0
174.90	7071.0
175.90	92976.0
176.90	5943.0
177.90	162.0

Instrument :
MSVOA_U
ClientSampleId :
BFB068